

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035496.D
 Acq On : 17 Jun 2022 15:49
 Operator : CG/JU
 Sample : N3226-19
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	38	rVB2	23571	37221	1.20%	0.130%
2	3.910	136	140	148	rVB	31373	50736	1.64%	0.177%
3	4.010	153	157	161	rVB2	14005	21363	0.69%	0.075%
4	4.240	192	196	201	rBV3	22041	31457	1.02%	0.110%
5	4.557	247	250	258	rVB	15413	25068	0.81%	0.088%
6	4.657	263	267	272	rVB6	8666	14971	0.48%	0.052%
7	4.922	308	312	322	rBV2	44694	92271	2.99%	0.322%
8	5.528	412	415	419	rVB2	5950	7380	0.24%	0.026%
9	6.163	519	523	524	rBV4	3358	4794	0.16%	0.017%
10	7.016	661	668	684	rBV	149611	418671	13.55%	1.462%
11	7.151	686	691	709	rVB	217570	400497	12.96%	1.398%
12	7.357	720	726	738	rBV	261038	502920	16.28%	1.756%
13	7.651	773	776	780	rVB5	3263	5590	0.18%	0.020%
14	7.816	797	804	816	rBV	624209	1076212	34.83%	3.757%
15	8.557	924	930	945	rBV	176966	454216	14.70%	1.586%
16	8.669	946	949	958	rVB3	19796	41847	1.35%	0.146%
17	8.981	996	1002	1021	rVV	220552	470269	15.22%	1.642%
18	9.710	1119	1126	1144	rBV	168427	372924	12.07%	1.302%
19	10.275	1216	1222	1249	rBV2	128424	521424	16.88%	1.820%
20	10.610	1272	1279	1295	rBV	908245	1601254	51.83%	5.590%
21	10.780	1298	1308	1327	rBV	145572	471205	15.25%	1.645%
22	12.180	1540	1546	1554	rBV4	12258	30531	0.99%	0.107%
23	12.245	1556	1557	1565	rVB7	5384	7579	0.25%	0.026%
24	13.086	1695	1700	1703	rVB6	2964	4439	0.14%	0.015%
25	13.292	1733	1735	1740	rVB5	2370	3189	0.10%	0.011%
26	13.374	1743	1749	1751	rVV5	3577	3975	0.13%	0.014%
27	13.445	1758	1761	1765	rBV6	2482	4075	0.13%	0.014%
28	13.763	1811	1815	1817	rBV3	2375	3385	0.11%	0.012%
29	13.874	1828	1834	1851	rBV	590051	938146	30.36%	3.275%
30	14.151	1875	1881	1896	rBV	723442	1124023	36.38%	3.924%
31	14.368	1915	1918	1922	rVB6	2125	3723	0.12%	0.013%
32	14.457	1926	1933	1943	rBV	1382821	2079058	67.29%	7.259%
33	14.657	1964	1967	1969	rBV3	2759	3479	0.11%	0.012%
34	14.733	1974	1980	2011	rBV	197171	797301	25.81%	2.784%
35	14.951	2011	2017	2026	rVB	13314	45719	1.48%	0.160%
36	15.263	2064	2070	2075	rBV6	5866	8395	0.27%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035496.D
 Acq On : 17 Jun 2022 15:49
 Operator : CG/JU
 Sample : N3226-19
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

37	15.451	2095	2102	2122	rBV	972810	1560293	50.50%	5.447%
38	15.610	2124	2129	2140	rVV	89375	211076	6.83%	0.737%
39	15.698	2142	2144	2151	rVV4	17828	34901	1.13%	0.122%
40	15.751	2151	2153	2159	rVV6	4960	8039	0.26%	0.028%
41	15.886	2170	2176	2177	rBV6	1769	3178	0.10%	0.011%
42	15.951	2183	2187	2191	rVB7	4559	6918	0.22%	0.024%
43	16.033	2198	2201	2203	rBV4	2584	3110	0.10%	0.011%
44	16.121	2211	2216	2217	rBV5	6349	6853	0.22%	0.024%
45	16.180	2222	2226	2228	rBV5	2958	4472	0.14%	0.016%
46	16.357	2254	2256	2260	rVB5	3483	3573	0.12%	0.012%
47	16.957	2353	2358	2359	rBV5	2623	4294	0.14%	0.015%
48	16.974	2359	2361	2364	rVV4	4710	4032	0.13%	0.014%
49	17.133	2383	2388	2393	rVV9	8229	13424	0.43%	0.047%
50	17.204	2393	2400	2411	rVV	1655628	2396824	77.58%	8.368%
51	17.304	2411	2417	2433	rVV2	981786	1624600	52.58%	5.672%
52	17.421	2433	2437	2446	rVV6	34639	73003	2.36%	0.255%
53	17.498	2446	2450	2454	rVB2	6839	11399	0.37%	0.040%
54	17.645	2473	2475	2477	rBV3	3035	3393	0.11%	0.012%
55	17.827	2504	2506	2509	rBV4	3220	4623	0.15%	0.016%
56	17.880	2512	2515	2521	rVB5	11738	19484	0.63%	0.068%
57	17.992	2532	2534	2537	rBV4	3743	4826	0.16%	0.017%
58	18.051	2542	2544	2549	rBV6	5161	7813	0.25%	0.027%
59	18.109	2550	2554	2563	rBV2	74394	132218	4.28%	0.462%
60	18.180	2563	2566	2570	rVB	11915	17481	0.57%	0.061%
61	18.398	2601	2603	2606	rBV3	3827	4723	0.15%	0.016%
62	19.168	2730	2734	2737	rBV5	16135	26002	0.84%	0.091%
63	19.245	2744	2747	2749	rBV2	16143	19259	0.62%	0.067%
64	19.274	2749	2752	2758	rVB	24243	37095	1.20%	0.130%
65	19.392	2768	2772	2779	rBV	56636	89272	2.89%	0.312%
66	19.598	2802	2807	2822	rBV	1427588	2034706	65.86%	7.104%
67	21.109	3061	3064	3072	rBV4	108231	186047	6.02%	0.650%
68	21.392	3107	3112	3123	rBV2	1916288	2938188	95.10%	10.258%
69	23.586	3479	3485	3500	rVB2	1058730	2378787	76.99%	8.305%
70	23.733	3504	3510	3525	rVB2	1426113	3089564	100.00%	10.787%




Sum of corrected areas: 28642777

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035496.D
Acq On : 17 Jun 2022 15:49
Operator : CG/JU
Sample : N3226-19
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

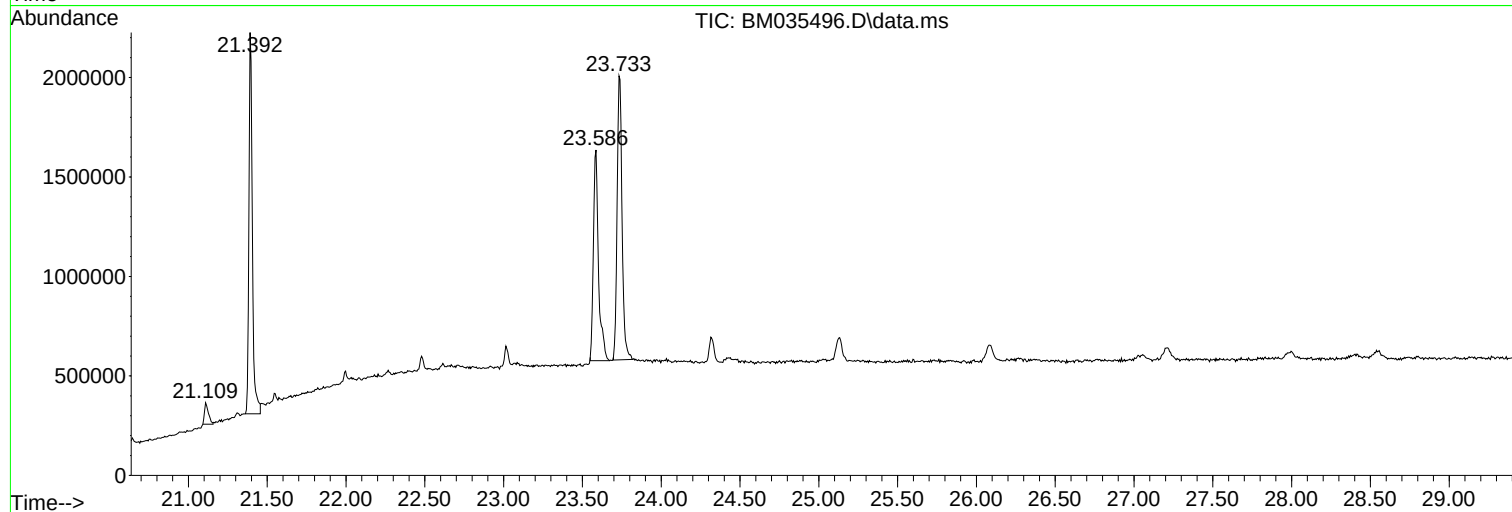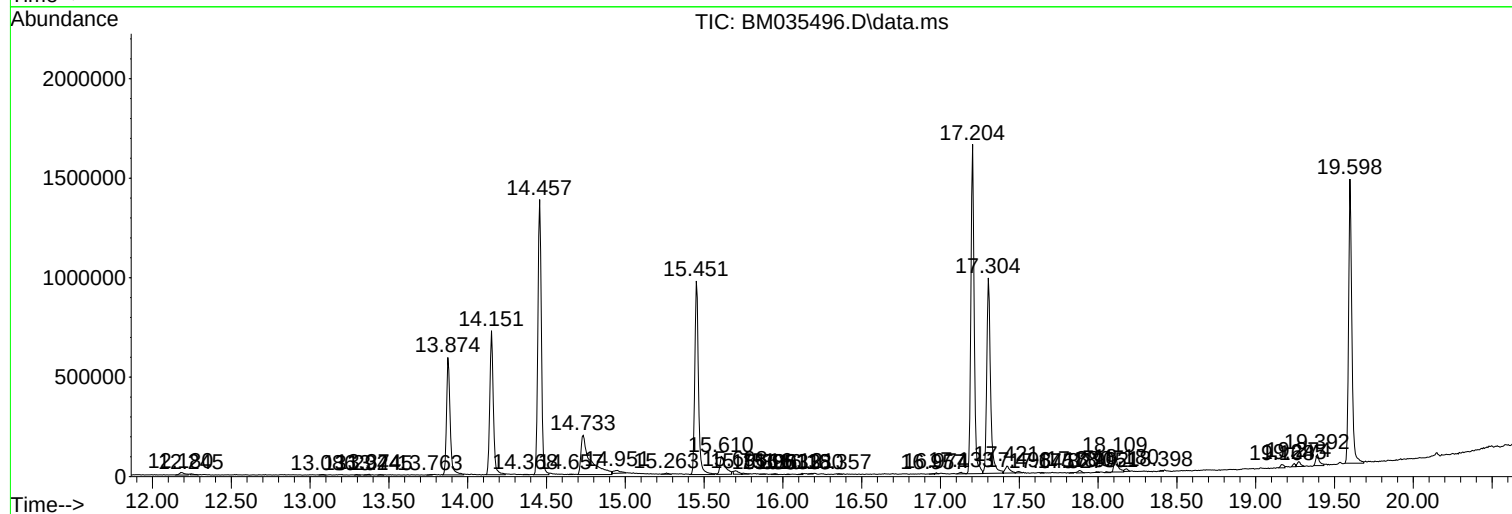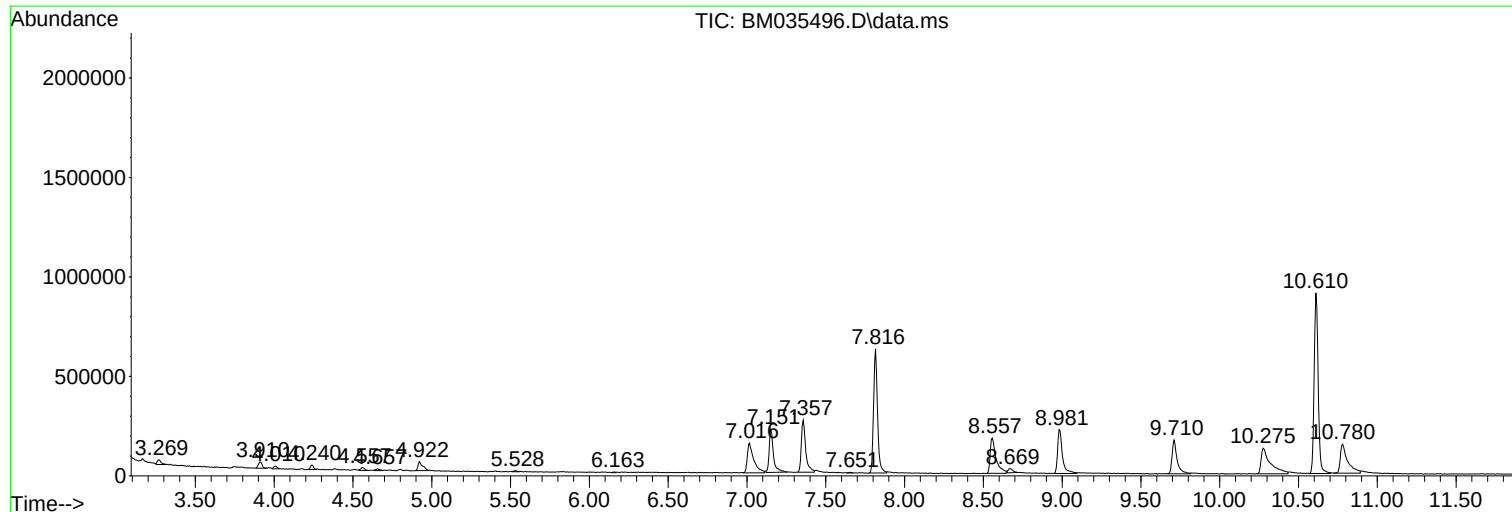

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035496.D
Acq On : 17 Jun 2022 15:49
Operator : CG/JU
Sample : N3226-19
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035496.D
Acq On : 17 Jun 2022 15:49
Operator : CG/JU
Sample : N3226-19
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc