

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035497.D
 Acq On : 17 Jun 2022 16:26
 Operator : CG/JU
 Sample : N3226-20
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035497.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	40	rVB	40516	66651	1.96%	0.166%
2	3.722	105	108	117	rBV2	24796	58453	1.72%	0.146%
3	3.911	135	140	147	rVB	41539	68897	2.03%	0.172%
4	4.511	240	242	246	rVB4	7702	8740	0.26%	0.022%
5	4.563	246	251	260	rVB2	21674	37774	1.11%	0.094%
6	4.799	288	291	296	rBV3	8332	11981	0.35%	0.030%
7	4.922	308	312	324	rBV	55622	94080	2.77%	0.235%
8	5.534	411	416	419	rBV2	7069	12342	0.36%	0.031%
9	7.004	660	666	685	rBV	353671	834131	24.57%	2.082%
10	7.152	685	691	706	rVB	399459	690093	20.33%	1.722%
11	7.352	719	725	737	rBV	496046	906164	26.69%	2.261%
12	7.652	772	776	780	rVB5	2976	4065	0.12%	0.010%
13	7.816	797	804	817	rBV	670965	1178633	34.72%	2.941%
14	8.546	922	928	942	rBV	482583	1044411	30.76%	2.606%
15	8.663	943	948	959	rVB	44866	100642	2.96%	0.251%
16	8.981	995	1002	1018	rBV	445497	855914	25.21%	2.136%
17	9.410	1072	1075	1079	rVB5	3204	4063	0.12%	0.010%
18	9.704	1117	1125	1138	rBV	344187	688797	20.29%	1.719%
19	10.104	1186	1193	1196	rBV7	4226	9032	0.27%	0.023%
20	10.263	1214	1220	1245	rBV	337052	992479	29.23%	2.477%
21	10.610	1272	1279	1294	rBV	1050450	1784002	52.55%	4.452%
22	10.769	1298	1306	1341	rBV	320490	948337	27.93%	2.367%
23	12.251	1553	1558	1566	rVV5	6274	15109	0.45%	0.038%
24	13.081	1695	1699	1702	rBV6	3344	4650	0.14%	0.012%
25	13.292	1730	1735	1741	rVB7	2861	4792	0.14%	0.012%
26	13.804	1816	1822	1826	rVB8	3559	6368	0.19%	0.016%
27	13.875	1826	1834	1849	rBV	1063835	1736738	51.16%	4.334%
28	14.151	1874	1881	1896	rBV	1350009	2109386	62.13%	5.264%
29	14.369	1917	1918	1922	rVB4	5116	3923	0.12%	0.010%
30	14.457	1926	1933	1951	rBV	1612766	2441012	71.90%	6.092%
31	14.757	1974	1984	2005	rBV5	101083	520518	15.33%	1.299%
32	14.922	2007	2012	2025	rVB7	36751	101339	2.99%	0.253%
33	15.263	2064	2070	2073	rBV6	5984	9347	0.28%	0.023%
34	15.451	2094	2102	2119	rBV	1819123	2770097	81.60%	6.913%
35	15.598	2121	2127	2140	rVV	337736	655536	19.31%	1.636%
36	15.698	2140	2144	2155	rVV2	29929	69942	2.06%	0.175%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035497.D
 Acq On : 17 Jun 2022 16:26
 Operator : CG/JU
 Sample : N3226-20
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

37	15.874	2172	2174	2180	rVB6	2886	3899	0.11%	0.010%
38	16.027	2196	2200	2203	rVB6	3581	4849	0.14%	0.012%
39	16.180	2221	2226	2229	rVV7	7100	13704	0.40%	0.034%
40	16.239	2232	2236	2241	rVB6	7382	10100	0.30%	0.025%
41	16.645	2303	2305	2310	rVB6	3173	3766	0.11%	0.009%
42	16.886	2340	2346	2351	rBV8	4211	7987	0.24%	0.020%
43	16.974	2357	2361	2362	rBV4	4909	4787	0.14%	0.012%
44	16.992	2362	2364	2367	rVB3	3170	4255	0.13%	0.011%
45	17.133	2383	2388	2393	rBV7	6558	10875	0.32%	0.027%
46	17.204	2393	2400	2410	rBV	1892763	2823783	83.18%	7.047%
47	17.304	2411	2417	2431	rVV2	1788020	2850680	83.97%	7.114%
48	17.427	2435	2438	2445	rVV7	19975	40357	1.19%	0.101%
49	17.498	2446	2450	2453	rVB5	8269	12539	0.37%	0.031%
50	17.627	2470	2472	2476	rBV5	3772	4288	0.13%	0.011%
51	17.710	2481	2486	2490	rBV7	6569	9431	0.28%	0.024%
52	17.886	2512	2516	2521	rVB3	15559	19746	0.58%	0.049%
53	18.110	2549	2554	2563	rBV	168857	280021	8.25%	0.699%
54	18.174	2563	2565	2570	rVB	13038	21735	0.64%	0.054%
55	18.321	2588	2590	2592	rBV3	3740	3761	0.11%	0.009%
56	18.915	2688	2691	2696	rBV7	9002	16171	0.48%	0.040%
57	19.033	2708	2711	2716	rBV5	7605	12926	0.38%	0.032%
58	19.163	2730	2733	2743	rBV9	27631	50392	1.48%	0.126%
59	19.245	2743	2747	2749	rBV3	34911	42757	1.26%	0.107%
60	19.386	2767	2771	2779	rBV2	83299	148366	4.37%	0.370%
61	19.533	2794	2796	2799	rVB2	15169	10826	0.32%	0.027%
62	19.598	2801	2807	2815	rBV	2230197	3136154	92.38%	7.827%
63	20.645	2982	2985	2988	rBV	41037	47398	1.40%	0.118%
64	21.109	3060	3064	3074	rBV2	320131	588623	17.34%	1.469%
65	21.392	3107	3112	3123	rBV	2063720	2849331	83.93%	7.111%
66	23.580	3478	3484	3498	rBV2	1558989	3394903	100.00%	8.472%
67	23.733	3504	3510	3521	rVB2	1341598	2793307	82.28%	6.971%




Sum of corrected areas: 40070155

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035497.D
Acq On : 17 Jun 2022 16:26
Operator : CG/JU
Sample : N3226-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4P0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

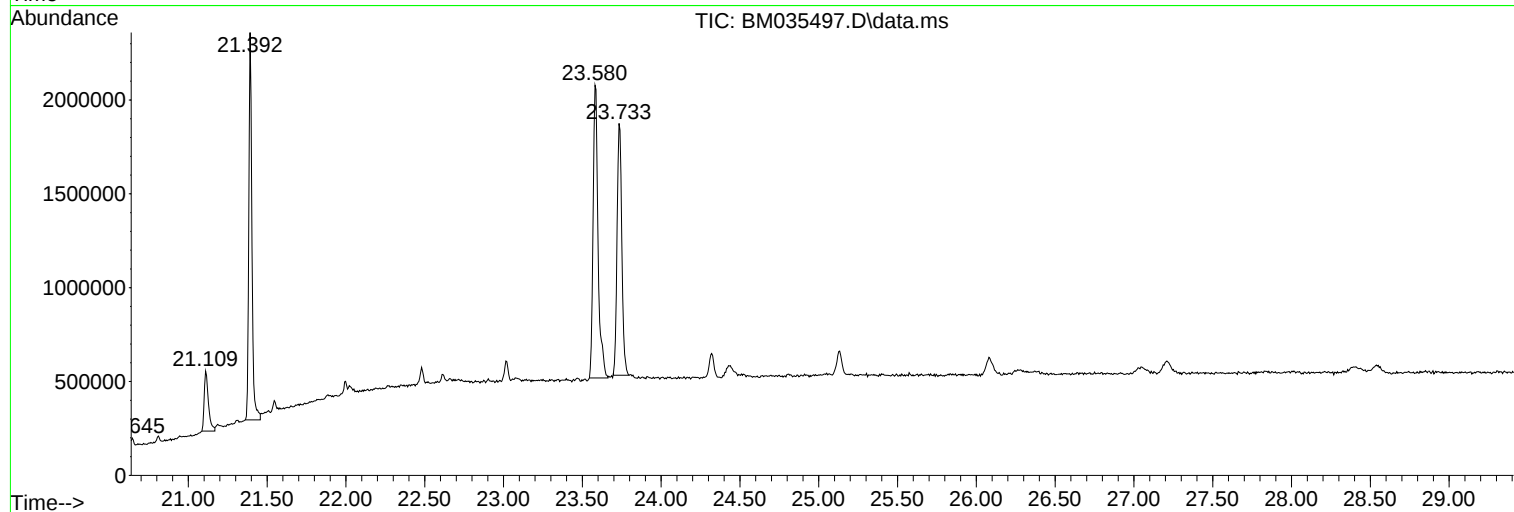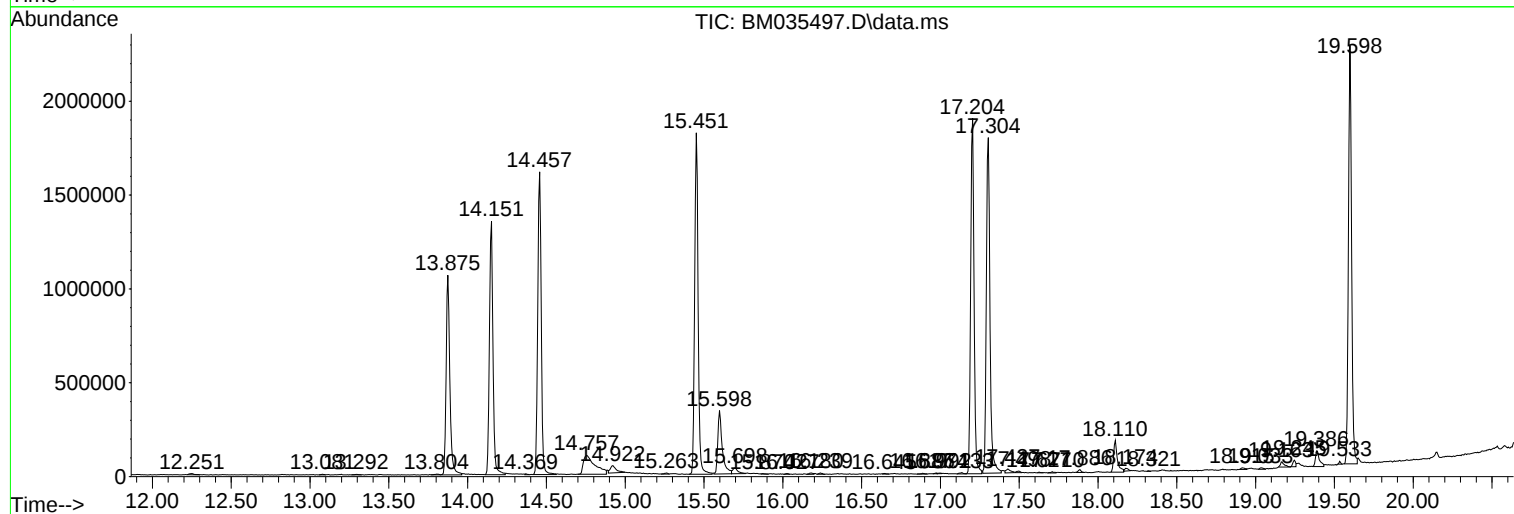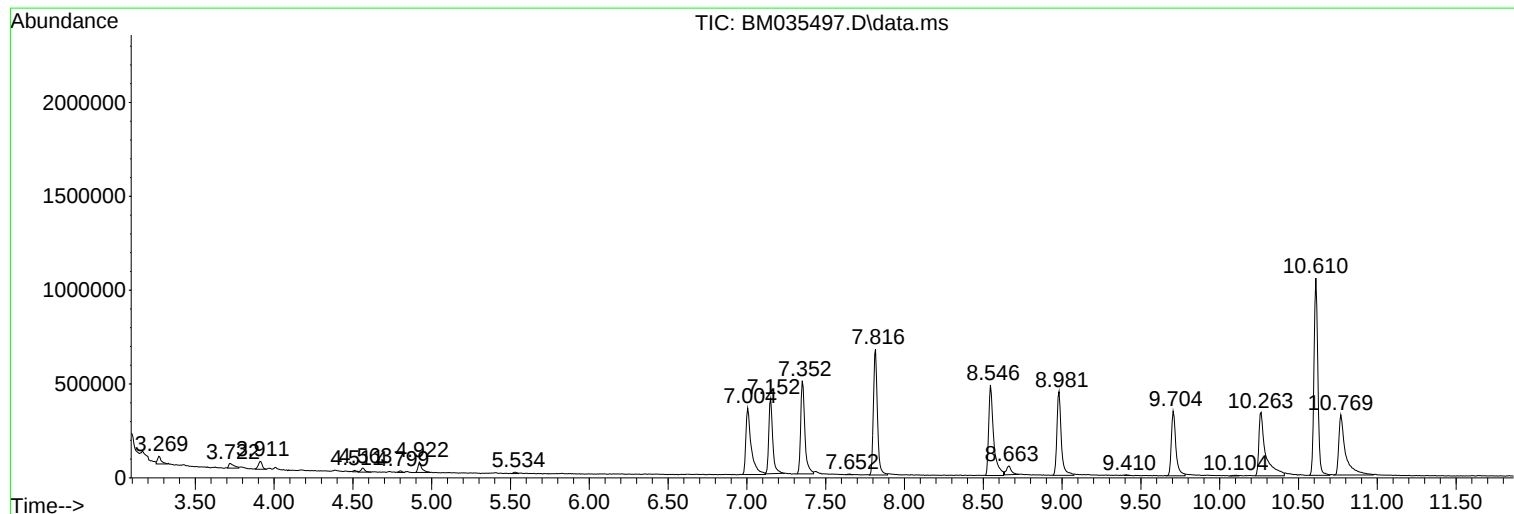

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035497.D
Acq On : 17 Jun 2022 16:26
Operator : CG/JU
Sample : N3226-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4P0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.110	4.13 ng/ul	588623	Chrysene-d12	21.392

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			5-Eicosene, (E)-	280	C20H40	074685-30-6	96
2			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	95
3			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	94
4			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	94
5			Cyclotetracosane	336	C24H48	000297-03-0	94

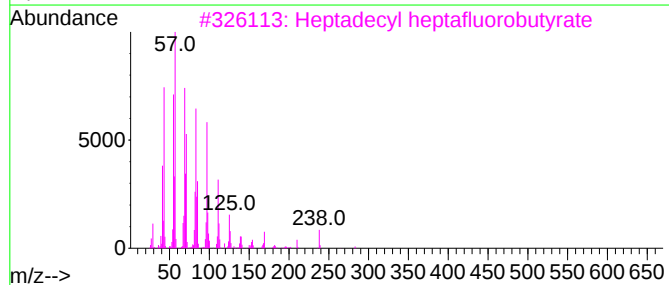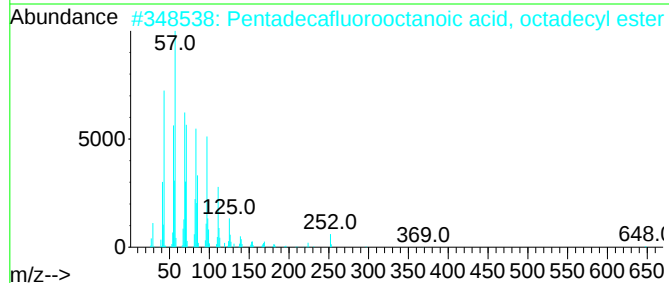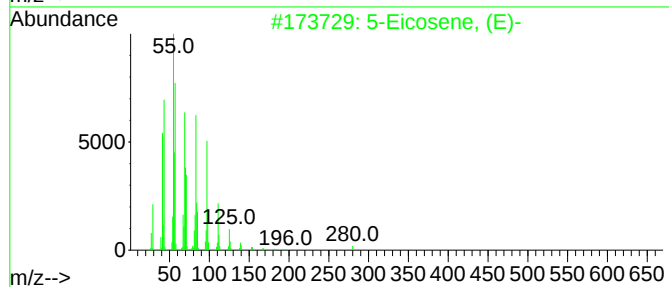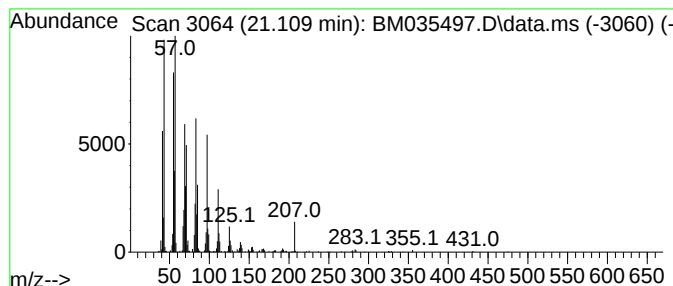

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035497.D
Acq On : 17 Jun 2022 16:26
Operator : CG/JU
Sample : N3226-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4P0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.110	4.1	ng/u1	588623	5	21.392	2849330	20.0