

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035501.D
 Acq On : 17 Jun 2022 18:54
 Operator : CG/JU
 Sample : N3226-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035501.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	36	rVB2	29302	38701	1.25%	0.123%
2	3.699	101	104	121	rBV	154445	324948	10.52%	1.034%
3	3.910	137	140	145	rVB2	14781	25082	0.81%	0.080%
4	4.010	153	157	162	rVB	20412	29326	0.95%	0.093%
5	4.563	249	251	260	rVB5	7265	10199	0.33%	0.032%
6	4.799	289	291	295	rVB5	4121	4549	0.15%	0.014%
7	4.928	309	313	318	rVB	16253	24416	0.79%	0.078%
8	5.528	413	415	420	rBV3	3800	4482	0.15%	0.014%
9	6.816	631	634	637	rVB4	2258	3564	0.12%	0.011%
10	6.951	652	657	658	rBV5	2723	3327	0.11%	0.011%
11	7.010	662	667	683	rBV	194872	518401	16.78%	1.650%
12	7.151	686	691	704	rVB	249641	430841	13.95%	1.371%
13	7.357	719	726	739	rBV	311751	604786	19.58%	1.924%
14	7.816	797	804	817	rBV	620752	1087881	35.21%	3.462%
15	8.081	847	849	857	rVB8	2804	4592	0.15%	0.015%
16	8.363	895	897	902	rVB5	4181	5209	0.17%	0.017%
17	8.487	912	918	920	rBV7	2686	3603	0.12%	0.011%
18	8.551	923	929	946	rBV	278776	685698	22.20%	2.182%
19	8.669	946	949	957	rVV4	18861	45438	1.47%	0.145%
20	8.745	961	962	968	rVB6	2657	3622	0.12%	0.012%
21	8.981	996	1002	1011	rBV	264350	522049	16.90%	1.661%
22	9.710	1118	1126	1144	rBV	194319	439890	14.24%	1.400%
23	9.969	1167	1170	1175	rVB7	3130	4328	0.14%	0.014%
24	10.051	1179	1184	1189	rVB7	2141	4153	0.13%	0.013%
25	10.145	1196	1200	1206	rVB6	3430	6359	0.21%	0.020%
26	10.198	1206	1209	1212	rBV4	3019	4878	0.16%	0.016%
27	10.269	1215	1221	1250	rBV	173867	629225	20.37%	2.002%
28	10.610	1272	1279	1291	rBV	922286	1648554	53.36%	5.246%
29	10.769	1300	1306	1329	rBV	221875	675639	21.87%	2.150%
30	10.998	1343	1345	1352	rVB7	3443	5076	0.16%	0.016%
31	11.104	1359	1363	1367	rVB6	4384	6920	0.22%	0.022%
32	11.292	1390	1395	1397	rVV6	2618	3876	0.13%	0.012%
33	11.322	1397	1400	1404	rVB5	2460	3862	0.13%	0.012%
34	11.469	1423	1425	1430	rVB5	2167	3122	0.10%	0.010%
35	11.539	1431	1437	1438	rBV6	2719	3681	0.12%	0.012%
36	11.651	1450	1456	1459	rBV5	9224	16150	0.52%	0.051%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035501.D
 Acq On : 17 Jun 2022 18:54
 Operator : CG/JU
 Sample : N3226-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

37	11.804	1478	1482	1485	rBV6	2253	3523	0.11%	0.011%
38	11.898	1490	1498	1504	rBV10	4052	7693	0.25%	0.024%
39	12.051	1517	1524	1531	rBV3	24213	46119	1.49%	0.147%
40	12.181	1543	1546	1549	rBV4	3140	3375	0.11%	0.011%
41	12.245	1554	1557	1559	rVV5	6047	7381	0.24%	0.023%
42	12.263	1559	1560	1568	rVB6	5788	8677	0.28%	0.028%
43	12.339	1570	1573	1578	rBV6	1949	3494	0.11%	0.011%
44	12.445	1586	1591	1594	rBV5	2910	4191	0.14%	0.013%
45	12.680	1629	1631	1637	rVB6	3593	6134	0.20%	0.020%
46	12.733	1637	1640	1647	rBV9	3561	6623	0.21%	0.021%
47	12.869	1657	1663	1666	rVB6	3619	5692	0.18%	0.018%
48	12.951	1672	1677	1679	rBV4	4550	5442	0.18%	0.017%
49	13.004	1680	1686	1692	rVV4	11523	20010	0.65%	0.064%
50	13.063	1694	1696	1705	rVB8	2321	4482	0.15%	0.014%
51	13.292	1725	1735	1742	rBV	29647	54409	1.76%	0.173%
52	13.380	1746	1750	1755	rVB6	4358	8044	0.26%	0.026%
53	13.604	1785	1788	1792	rVB4	2818	3593	0.12%	0.011%
54	13.727	1806	1809	1811	rBV4	2667	3112	0.10%	0.010%
55	13.875	1828	1834	1844	rBV	643069	1060206	34.32%	3.374%
56	13.945	1844	1846	1850	rVB2	18382	24725	0.80%	0.079%
57	14.075	1862	1868	1873	rVB5	6850	9604	0.31%	0.031%
58	14.151	1873	1881	1894	rBV	818778	1290306	41.77%	4.106%
59	14.363	1913	1917	1922	rBV2	34902	46407	1.50%	0.148%
60	14.457	1926	1933	1945	rBV	1415659	2144715	69.42%	6.825%
61	14.592	1954	1956	1961	rVB6	3664	5085	0.16%	0.016%
62	14.774	1979	1987	2000	rBV6	47855	236197	7.65%	0.752%
63	14.933	2012	2014	2019	rVB5	4549	5712	0.18%	0.018%
64	15.169	2047	2054	2057	rBV6	5388	9879	0.32%	0.031%
65	15.316	2074	2079	2083	rBV	26972	34996	1.13%	0.111%
66	15.451	2096	2102	2118	rBV	1084896	1714820	55.51%	5.457%
67	15.604	2122	2128	2140	rVV	159617	346522	11.22%	1.103%
68	15.716	2141	2147	2153	rVB4	25654	71899	2.33%	0.229%
69	15.939	2180	2185	2189	rVB8	10747	20048	0.65%	0.064%
70	15.980	2189	2192	2193	rBV3	3443	3103	0.10%	0.010%
71	16.174	2221	2225	2227	rVV	33226	42116	1.36%	0.134%
72	16.198	2227	2229	2234	rVV2	37775	49171	1.59%	0.156%
73	16.239	2234	2236	2240	rVB5	7036	8510	0.28%	0.027%
74	16.521	2278	2284	2285	rBV6	5921	7158	0.23%	0.023%
75	16.727	2316	2319	2323	rBV6	2643	4465	0.14%	0.014%
76	16.780	2326	2328	2331	rVB4	3886	3809	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035501.D
 Acq On : 17 Jun 2022 18:54
 Operator : CG/JU
 Sample : N3226-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

77	16.892	2344	2347	2349	rBV4	3348	3930	0.13%	0.013%
78	16.968	2355	2360	2365	rBV2	25581	35962	1.16%	0.114%
79	17.021	2365	2369	2373	rVB2	17437	25804	0.84%	0.082%
80	17.204	2394	2400	2411	rBV	1715811	2491795	80.66%	7.929%
81	17.304	2411	2417	2432	rVB	1231556	1903177	61.61%	6.056%
82	17.492	2447	2449	2455	rVB6	10835	15977	0.52%	0.051%
83	17.621	2469	2471	2472	rBV2	4995	3443	0.11%	0.011%
84	17.710	2481	2486	2490	rBV	26900	36990	1.20%	0.118%
85	17.880	2511	2515	2518	rBV5	7485	10918	0.35%	0.035%
86	17.986	2532	2533	2536	rBV3	4813	5182	0.17%	0.016%
87	18.115	2549	2555	2564	rBV6	44074	98525	3.19%	0.314%
88	18.174	2564	2565	2569	rVB2	6829	8796	0.28%	0.028%
89	18.398	2600	2603	2609	rBV2	22159	29236	0.95%	0.093%
90	19.033	2708	2711	2716	rVB	22444	26387	0.85%	0.084%
91	19.162	2730	2733	2737	rBV3	18236	26832	0.87%	0.085%
92	19.245	2744	2747	2749	rBV2	13210	16463	0.53%	0.052%
93	19.392	2768	2772	2778	rBV5	32583	48199	1.56%	0.153%
94	19.598	2801	2807	2820	rBV	1665475	2424220	78.47%	7.714%
95	20.145	2898	2900	2905	rVB2	29465	31989	1.04%	0.102%
96	21.109	3061	3064	3069	rBV3	66139	94418	3.06%	0.300%
97	21.392	3107	3112	3122	rBV	2042196	2931366	94.89%	9.328%
98	23.580	3478	3484	3497	rBV2	1342184	2888830	93.51%	9.193%
99	23.733	3504	3510	3524	rVB2	1456527	3089307	100.00%	9.831%




Sum of corrected areas: 31425620

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035501.D
Acq On : 17 Jun 2022 18:54
Operator : CG/JU
Sample : N3226-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

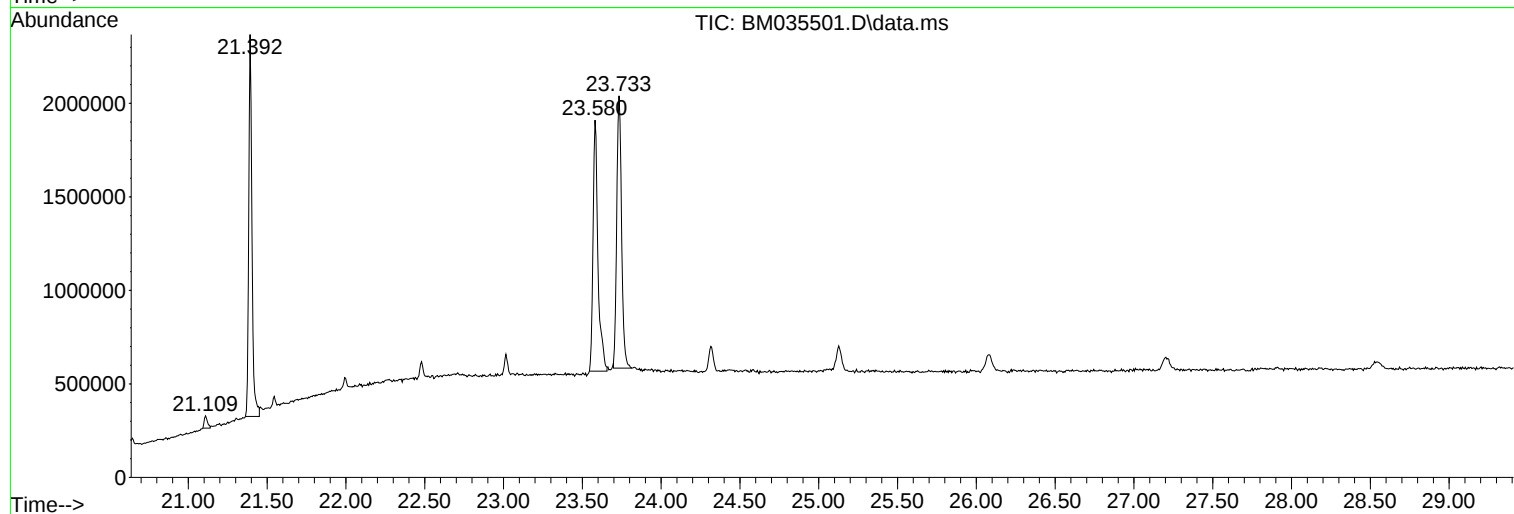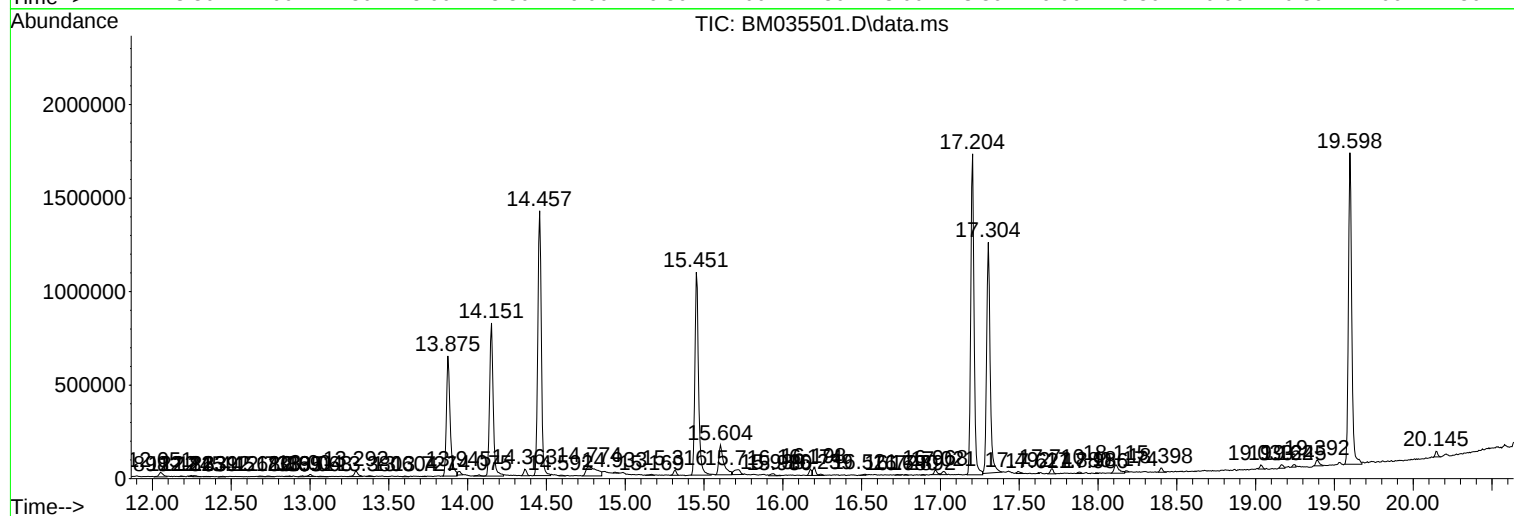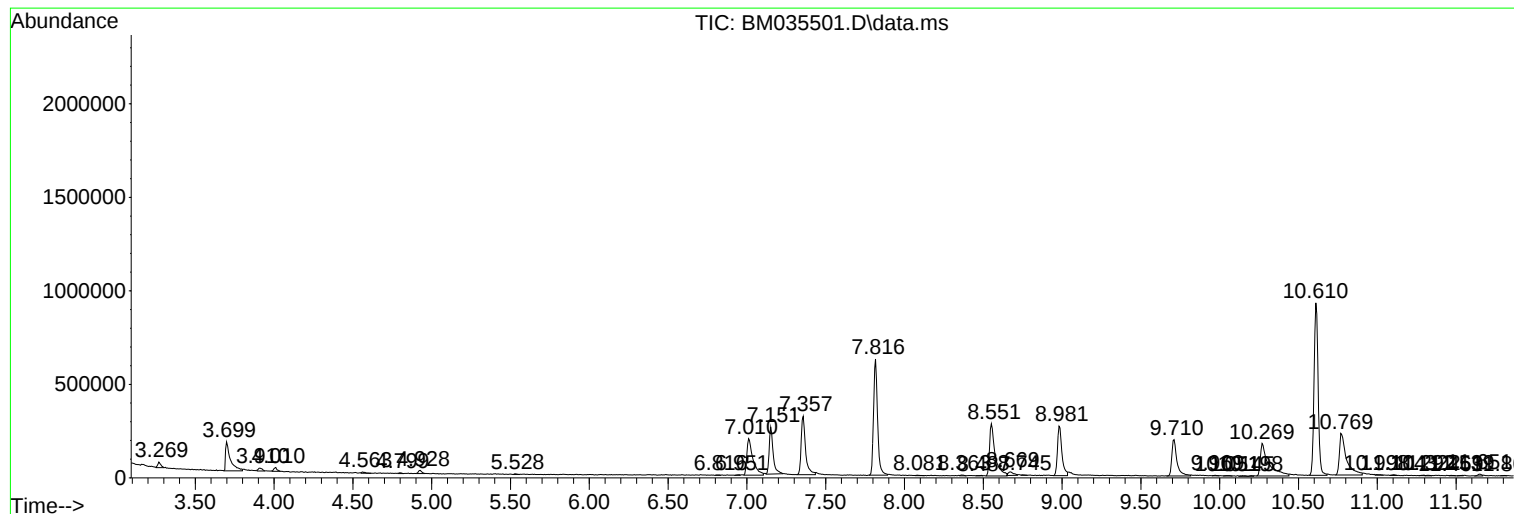

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035501.D
Acq On : 17 Jun 2022 18:54
Operator : CG/JU
Sample : N3226-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035501.D
Acq On : 17 Jun 2022 18:54
Operator : CG/JU
Sample : N3226-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------