

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035503.D
 Acq On : 17 Jun 2022 20:45
 Operator : CG/JU
 Sample : PB145488BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK488

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035503.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	38	rVB	50441	70027	1.37%	0.149%
2	3.687	99	102	125	rBV	460619	841358	16.50%	1.789%
3	4.004	153	156	161	rVB	13390	18731	0.37%	0.040%
4	7.004	660	666	685	rBV	469677	1053269	20.66%	2.240%
5	7.145	685	690	710	rVB	496612	890241	17.46%	1.893%
6	7.351	719	725	744	rBV	662303	1178689	23.12%	2.507%
7	7.816	797	804	820	rBV	661322	1178929	23.13%	2.507%
8	8.539	922	927	948	rBV	640262	1377008	27.01%	2.929%
9	8.975	995	1001	1021	rBV	549655	1056097	20.72%	2.246%
10	9.704	1117	1125	1143	rBV	442512	875276	17.17%	1.861%
11	10.257	1212	1219	1253	rBV	492711	1270327	24.92%	2.702%
12	10.610	1272	1279	1293	rBV	1018005	1743617	34.20%	3.708%
13	10.757	1297	1304	1332	rBV	868500	2106134	41.32%	4.479%
14	12.257	1552	1559	1564	rBV4	6960	17368	0.34%	0.037%
15	13.874	1827	1834	1849	rBV	1226024	2015190	39.53%	4.286%
16	14.151	1872	1881	1897	rBV	1553371	2466129	48.38%	5.245%
17	14.457	1926	1933	1950	rBV	1526539	2265979	44.45%	4.819%
18	14.727	1974	1979	2003	rBV2	133808	660477	12.96%	1.405%
19	15.451	2095	2102	2116	rBV	2043830	3189847	62.58%	6.784%
20	15.592	2121	2126	2140	rVV	424678	868518	17.04%	1.847%
21	15.698	2141	2144	2151	rVB3	30229	53374	1.05%	0.114%
22	16.239	2232	2236	2241	rVV6	7317	11901	0.23%	0.025%
23	17.204	2393	2400	2411	rBV	1764792	2590460	50.82%	5.509%
24	17.304	2411	2417	2436	rVB	2208409	3516275	68.98%	7.478%
25	18.133	2555	2558	2565	rBV9	5044	9788	0.19%	0.021%
26	19.168	2730	2734	2739	rBV4	28487	40467	0.79%	0.086%
27	19.245	2743	2747	2753	rBV2	20493	35807	0.70%	0.076%
28	19.397	2769	2773	2776	rBV5	12282	22648	0.44%	0.048%
29	19.539	2795	2797	2801	rBV4	9041	7851	0.15%	0.017%
30	19.597	2801	2807	2820	rBV	2881774	4137408	81.16%	8.799%
31	21.391	3107	3112	3122	rBV	2071734	3023603	59.31%	6.430%
32	23.580	3477	3484	3499	rBV2	2344526	5097608	100.00%	10.841%
33	23.727	3503	3509	3524	rVB2	1533930	3329875	65.32%	7.082%




Sum of corrected areas: 47020276

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035503.D
Acq On : 17 Jun 2022 20:45
Operator : CG/JU
Sample : PB145488BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

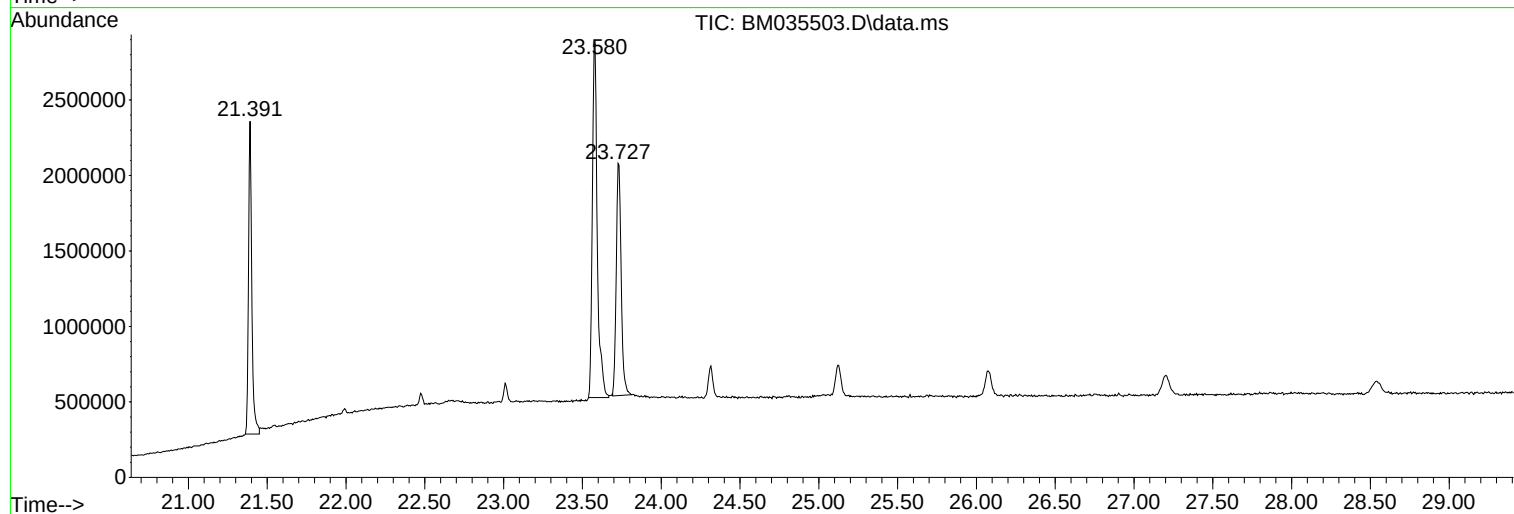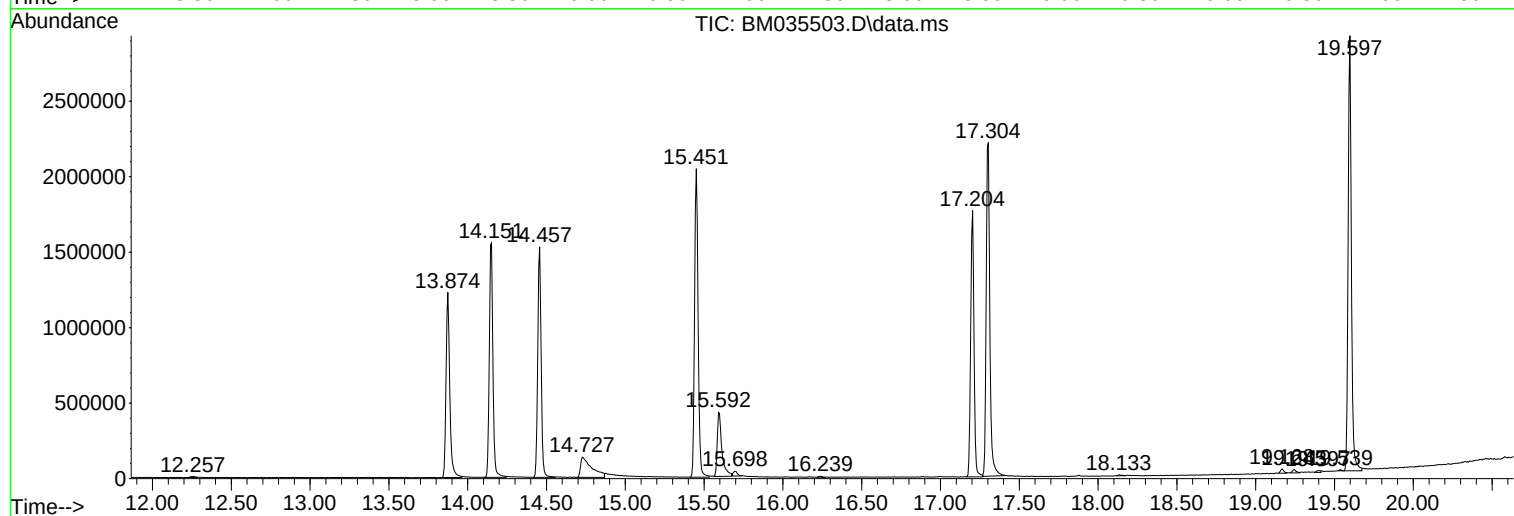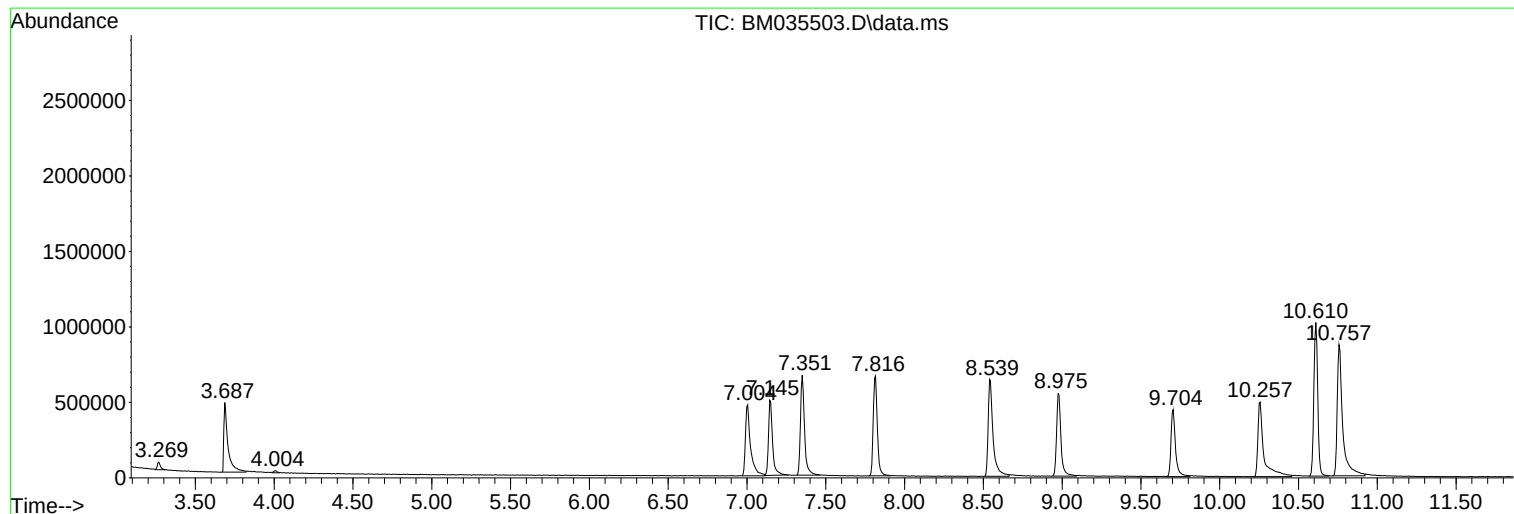

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035503.D
Acq On : 17 Jun 2022 20:45
Operator : CG/JU
Sample : PB145488BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035503.D
Acq On : 17 Jun 2022 20:45
Operator : CG/JU
Sample : PB145488BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc