

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035504.D
 Acq On : 17 Jun 2022 21:22
 Operator : CG/JU
 Sample : N3226-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4L6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035504.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	27	30	38	rVB	62729	91710	1.40%	0.150%
2	3.687	99	102	118	rBV	379258	702654	10.76%	1.152%
3	4.005	153	156	163	rVB2	14606	19284	0.30%	0.032%
4	4.922	309	312	321	rVB2	10991	19306	0.30%	0.032%
5	6.998	659	665	684	rBV	650399	1374006	21.04%	2.253%
6	7.145	684	690	707	rVB	696784	1178725	18.05%	1.932%
7	7.351	718	725	744	rBV	870432	1541198	23.60%	2.527%
8	7.810	797	803	816	rBV	720846	1262780	19.34%	2.070%
9	8.540	920	927	947	rBV	812580	1681932	25.75%	2.757%
10	8.975	994	1001	1018	rBV	784133	1421329	21.76%	2.330%
11	9.698	1114	1124	1140	rBV	590694	1175124	17.99%	1.926%
12	10.251	1212	1218	1254	rBV	700089	1745464	26.73%	2.861%
13	10.610	1271	1279	1295	rBV	1097104	1902768	29.14%	3.119%
14	10.763	1297	1305	1342	rBV	672954	1745996	26.74%	2.862%
15	12.057	1521	1525	1532	rVB9	5054	9420	0.14%	0.015%
16	12.239	1551	1556	1565	rVB4	11210	25061	0.38%	0.041%
17	13.292	1731	1735	1742	rBV8	4703	8269	0.13%	0.014%
18	13.869	1827	1833	1851	rBV	1713758	2695687	41.28%	4.419%
19	14.145	1873	1880	1900	rBV	2164432	3376931	51.71%	5.536%
20	14.363	1913	1917	1921	rVB4	8189	11058	0.17%	0.018%
21	14.457	1923	1933	1943	rBV	1669606	2463933	37.73%	4.039%
22	14.727	1971	1979	2007	rBV2	188881	896799	13.73%	1.470%
23	15.263	2065	2070	2073	rBV4	6221	9859	0.15%	0.016%
24	15.451	2095	2102	2120	rBV	2814701	4277594	65.50%	7.013%
25	15.592	2120	2126	2139	rVV	599477	1071642	16.41%	1.757%
26	15.698	2140	2144	2152	rVB2	40078	77484	1.19%	0.127%
27	16.027	2195	2200	2203	rVB7	7128	10033	0.15%	0.016%
28	16.174	2219	2225	2226	rBV6	9636	13668	0.21%	0.022%
29	16.239	2232	2236	2241	rVB4	10417	13835	0.21%	0.023%
30	16.351	2248	2255	2260	rBV10	7332	17398	0.27%	0.029%
31	16.633	2299	2303	2307	rBV6	5386	8539	0.13%	0.014%
32	16.880	2342	2345	2350	rVB7	5409	8406	0.13%	0.014%
33	16.974	2357	2361	2363	rBV4	9945	12089	0.19%	0.020%
34	17.021	2367	2369	2373	rVB4	7966	8710	0.13%	0.014%
35	17.115	2380	2385	2392	rBV3	25118	47045	0.72%	0.077%
36	17.204	2392	2400	2410	rVV	1934557	2857767	43.76%	4.685%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035504.D
 Acq On : 17 Jun 2022 21:22
 Operator : CG/JU
 Sample : N3226-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4L6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

37	17.304	2410	2417	2435	rVV	2877062	4595115	70.36%	7.533%
38	17.427	2435	2438	2447	rVB8	18226	35993	0.55%	0.059%
39	17.710	2483	2486	2490	rBV6	6266	7193	0.11%	0.012%
40	17.857	2506	2511	2512	rBV5	5284	8420	0.13%	0.014%
41	17.880	2512	2515	2520	rVB3	19708	25349	0.39%	0.042%
42	17.998	2528	2535	2541	rBV9	17008	35319	0.54%	0.058%
43	18.045	2541	2543	2549	rBV5	11404	19502	0.30%	0.032%
44	18.109	2549	2554	2563	rBV	315041	508377	7.78%	0.833%
45	18.409	2600	2605	2610	rBV5	39918	66006	1.01%	0.108%
46	19.033	2709	2711	2714	rBV4	12961	11694	0.18%	0.019%
47	19.162	2729	2733	2740	rBV4	42550	61630	0.94%	0.101%
48	19.239	2742	2746	2749	rBV	60449	91017	1.39%	0.149%
49	19.268	2749	2751	2754	rVB3	30295	34090	0.52%	0.056%
50	19.386	2767	2771	2781	rBV	177957	278305	4.26%	0.456%
51	19.598	2801	2807	2828	rBV	3841929	5508648	84.35%	9.031%
52	20.145	2897	2900	2906	rVB2	56855	64788	0.99%	0.106%
53	20.639	2981	2984	2988	rBV	85347	93968	1.44%	0.154%
54	21.103	3059	3063	3073	rBV	579528	1000669	15.32%	1.640%
55	21.386	3106	3111	3123	rBV	2387882	3395156	51.99%	5.566%
56	21.539	3134	3137	3142	rBV2	120819	151136	2.31%	0.248%
57	21.986	3211	3213	3216	rBV2	115980	144736	2.22%	0.237%
58	23.009	3384	3387	3392	rVB	243084	328101	5.02%	0.538%
59	23.574	3476	3483	3499	rBV2	3054433	6530708	100.00%	10.706%
60	23.727	3503	3509	3525	rVB2	1696750	3668728	56.18%	6.014%
61	24.309	3604	3608	3615	rVB	290224	550938	8.44%	0.903%




Sum of corrected areas: 60999089

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035504.D
Acq On : 17 Jun 2022 21:22
Operator : CG/JU
Sample : N3226-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4L6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

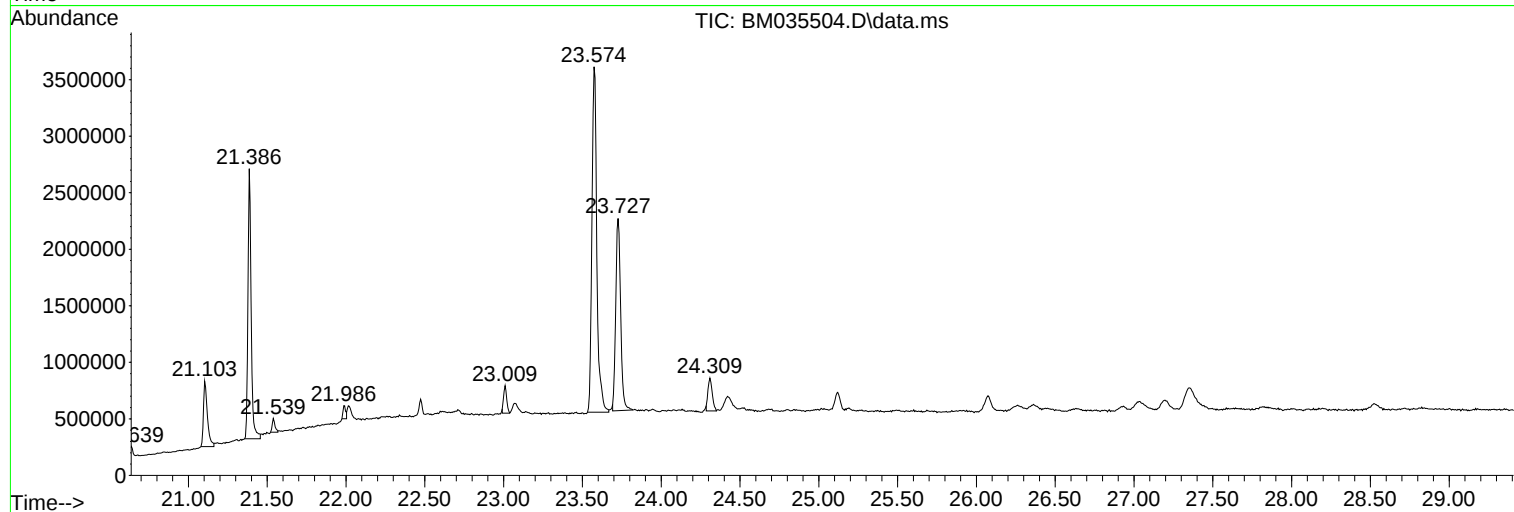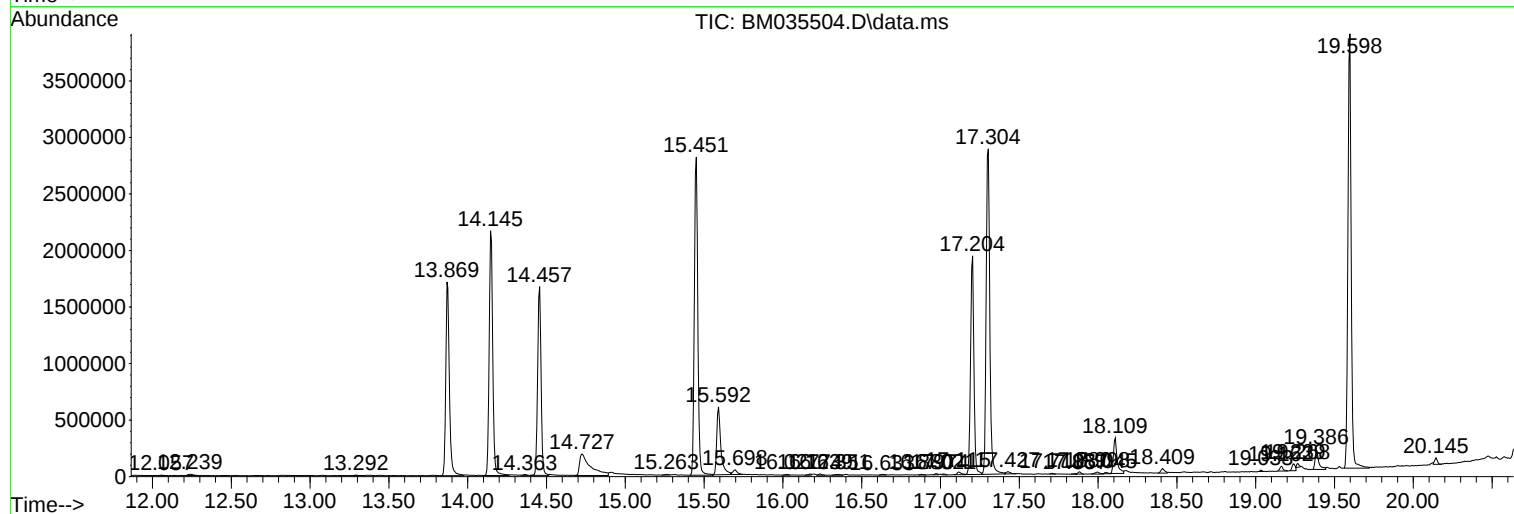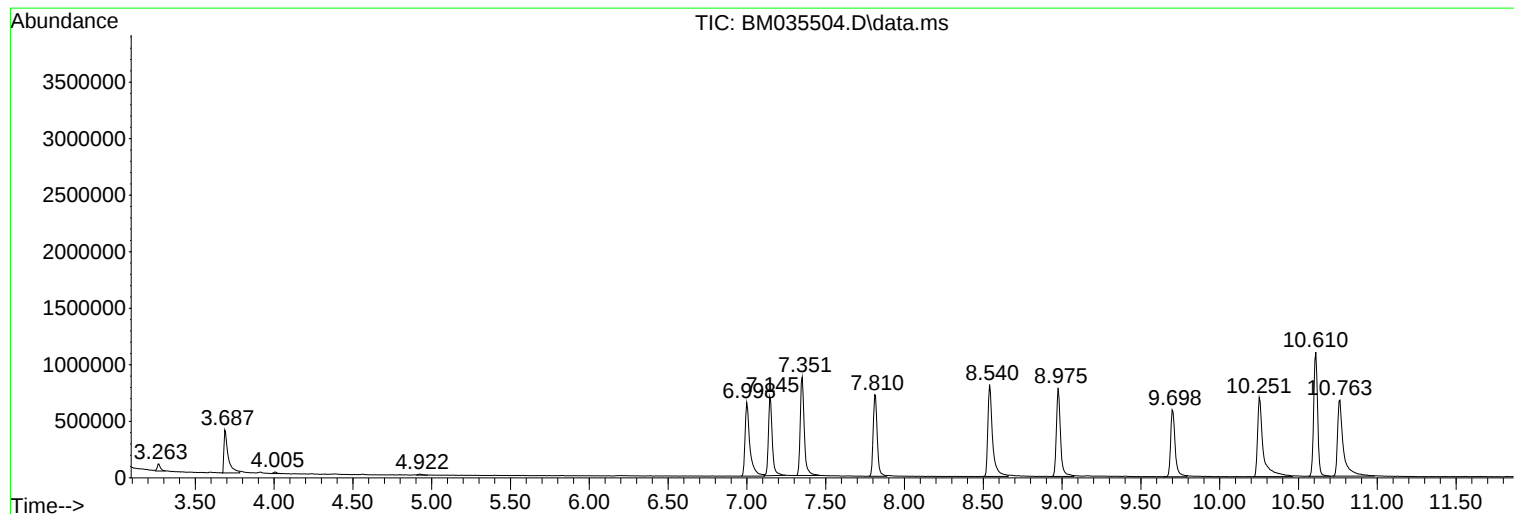

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035504.D
Acq On : 17 Jun 2022 21:22
Operator : CG/JU
Sample : N3226-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4L6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035504.D
Acq On : 17 Jun 2022 21:22
Operator : CG/JU
Sample : N3226-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4L6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc