

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035508.D
 Acq On : 17 Jun 2022 23:48
 Operator : CG/JU
 Sample : N3226-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035508.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	41	rVB	24792	44958	1.50%	0.167%
2	3.910	135	140	146	rVB	37273	58964	1.97%	0.219%
3	4.563	246	251	258	rVB2	15774	28721	0.96%	0.106%
4	4.799	288	291	295	rVB4	7299	10645	0.36%	0.039%
5	4.922	307	312	318	rBV	40747	62694	2.09%	0.232%
6	5.463	402	404	407	rVB3	4081	3417	0.11%	0.013%
7	5.528	413	415	419	rVB3	4798	6224	0.21%	0.023%
8	6.163	520	523	526	rVB4	2368	3358	0.11%	0.012%
9	7.010	661	667	685	rBV	139277	387533	12.93%	1.436%
10	7.151	685	691	707	rVB	193906	361156	12.05%	1.339%
11	7.357	719	726	736	rBV	234376	451339	15.06%	1.673%
12	7.546	756	758	763	rVB6	2196	3058	0.10%	0.011%
13	7.810	797	803	822	rBV	634005	1112994	37.15%	4.125%
14	8.551	923	929	943	rBV2	170635	427493	14.27%	1.585%
15	8.669	946	949	958	rVB	17467	34729	1.16%	0.129%
16	8.981	995	1002	1012	rBV	204339	407314	13.59%	1.510%
17	9.239	1043	1046	1051	rBV6	2252	3392	0.11%	0.013%
18	9.404	1071	1074	1079	rVB6	3024	5558	0.19%	0.021%
19	9.704	1119	1125	1143	rBV	151908	341574	11.40%	1.266%
20	10.275	1215	1222	1242	rBV2	123966	441911	14.75%	1.638%
21	10.610	1270	1279	1300	rBV	933406	1673045	55.84%	6.201%
22	10.781	1300	1308	1330	rBV	133426	441411	14.73%	1.636%
23	12.239	1551	1556	1563	rBV8	3534	7715	0.26%	0.029%
24	12.316	1565	1569	1574	rVV7	3152	6368	0.21%	0.024%
25	12.516	1599	1603	1606	rBV5	3272	5170	0.17%	0.019%
26	12.816	1651	1654	1656	rBV3	4046	5192	0.17%	0.019%
27	12.998	1683	1685	1690	rVB5	2590	4046	0.14%	0.015%
28	13.075	1693	1698	1700	rBV6	4722	5716	0.19%	0.021%
29	13.298	1732	1736	1739	rVB4	3377	3468	0.12%	0.013%
30	13.363	1742	1747	1752	rBV5	8319	12362	0.41%	0.046%
31	13.769	1813	1816	1817	rBV3	4675	4153	0.14%	0.015%
32	13.875	1825	1834	1851	rBV	516230	852365	28.45%	3.159%
33	14.045	1861	1863	1870	rVB5	2231	3169	0.11%	0.012%
34	14.151	1873	1881	1894	rBV	619110	1007538	33.63%	3.735%
35	14.457	1926	1933	1950	rBV	1358012	2138713	71.38%	7.927%
36	14.645	1963	1965	1968	rBV4	3974	5232	0.17%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035508.D
 Acq On : 17 Jun 2022 23:48
 Operator : CG/JU
 Sample : N3226-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

37	14.739	1975	1981	1986	rBV2	73687	182461	6.09%	0.676%
38	14.927	2009	2013	2021	rVB10	13334	31520	1.05%	0.117%
39	15.257	2066	2069	2072	rBV2	5097	6120	0.20%	0.023%
40	15.369	2086	2088	2092	rVB4	4024	4473	0.15%	0.017%
41	15.451	2096	2102	2114	rBV	870427	1376515	45.94%	5.102%
42	15.610	2123	2129	2140	rBV	94823	214908	7.17%	0.797%
43	15.698	2140	2144	2154	rVV7	17176	41722	1.39%	0.155%
44	16.063	2204	2206	2210	rVB5	4206	3811	0.13%	0.014%
45	16.192	2220	2228	2233	rVB8	6913	17221	0.57%	0.064%
46	16.339	2252	2253	2256	rBV3	3528	4023	0.13%	0.015%
47	16.763	2321	2325	2329	rBV6	3799	7614	0.25%	0.028%
48	16.968	2357	2360	2364	rBV6	5589	6399	0.21%	0.024%
49	17.121	2382	2386	2391	rBV5	9480	16419	0.55%	0.061%
50	17.198	2393	2399	2411	rVV	1649854	2480020	82.78%	9.192%
51	17.304	2411	2417	2433	rVV	885418	1466262	48.94%	5.435%
52	17.421	2433	2437	2443	rVV8	21642	43137	1.44%	0.160%
53	17.498	2446	2450	2453	rVB3	5600	7178	0.24%	0.027%
54	17.704	2482	2485	2488	rBV5	4302	5435	0.18%	0.020%
55	17.880	2512	2515	2521	rVB4	10352	13996	0.47%	0.052%
56	17.992	2529	2534	2538	rBV8	8689	14883	0.50%	0.055%
57	18.051	2542	2544	2546	rVV3	4559	3568	0.12%	0.013%
58	18.104	2549	2553	2562	rBV	97617	170542	5.69%	0.632%
59	18.180	2563	2566	2569	rVB	14246	18547	0.62%	0.069%
60	18.410	2601	2605	2610	rBV7	7842	15059	0.50%	0.056%
61	19.168	2730	2734	2736	rBV5	14793	20359	0.68%	0.075%
62	19.239	2743	2746	2749	rBV5	20911	30453	1.02%	0.113%
63	19.268	2749	2751	2758	rVB4	24984	38991	1.30%	0.145%
64	19.386	2767	2771	2780	rBV2	70811	115524	3.86%	0.428%
65	19.598	2801	2807	2820	rBV	1315755	1903067	63.52%	7.054%
66	21.103	3060	3063	3072	rBV	116945	174623	5.83%	0.647%
67	21.386	3106	3111	3120	rBV	2127593	2996080	100.00%	11.105%
68	23.574	3478	3483	3496	rVB2	1019160	2227549	74.35%	8.257%
69	23.721	3503	3508	3522	rVB	1368984	2948005	98.40%	10.927%




Sum of corrected areas: 26979179

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035508.D
Acq On : 17 Jun 2022 23:48
Operator : CG/JU
Sample : N3226-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

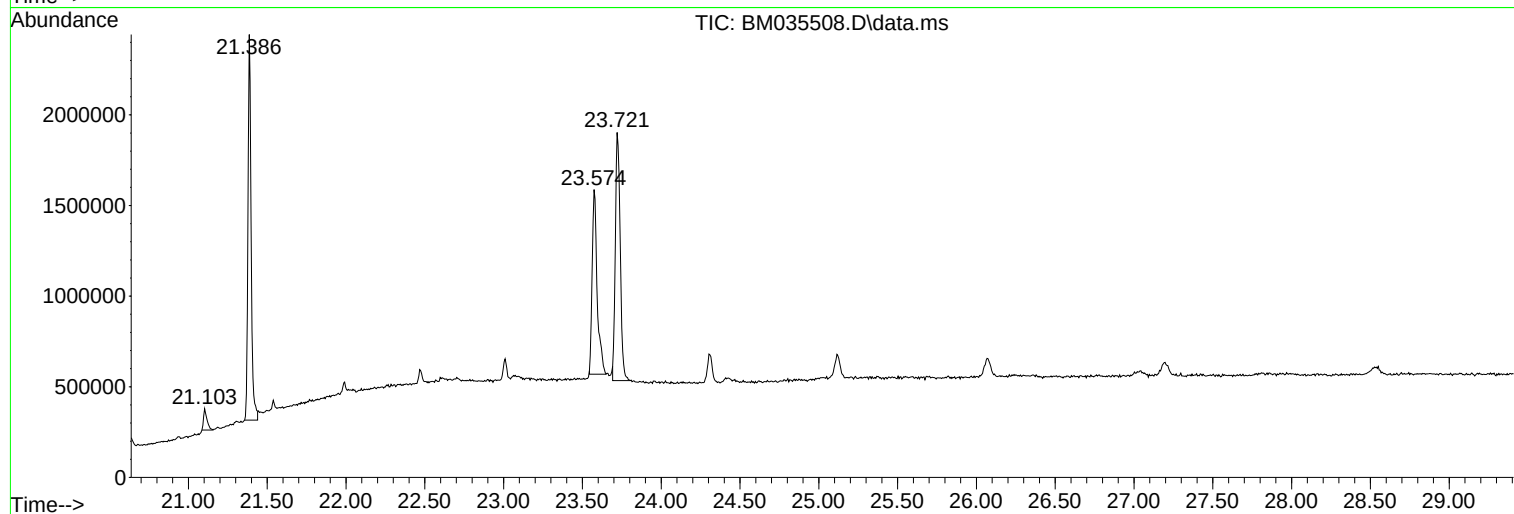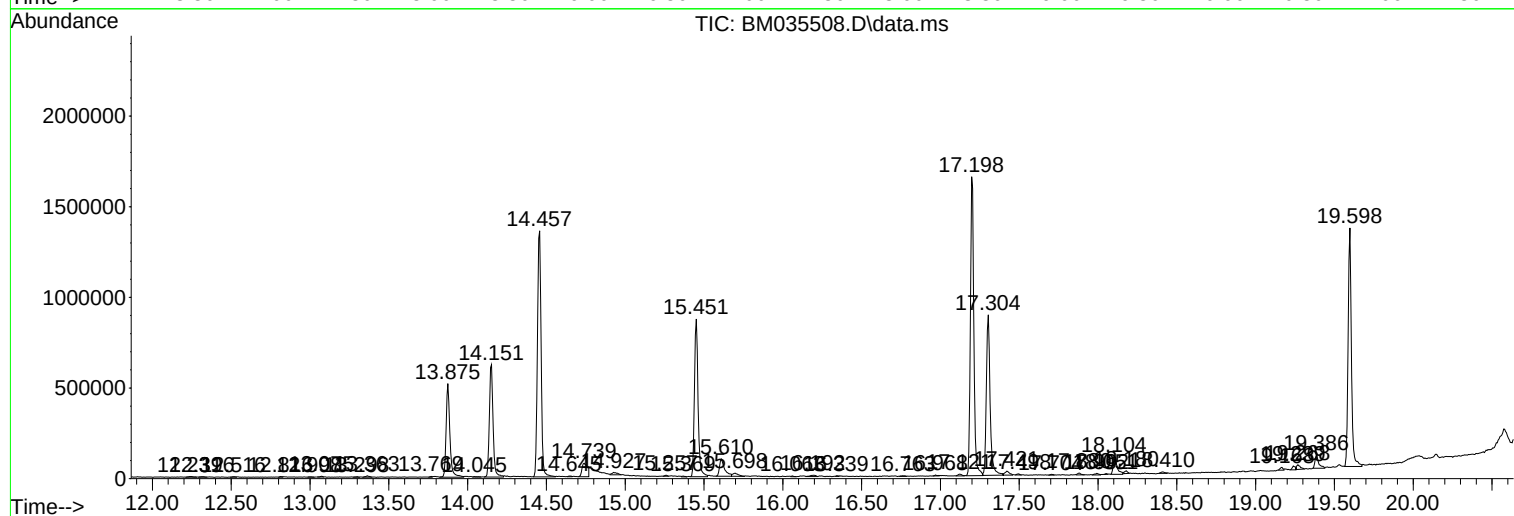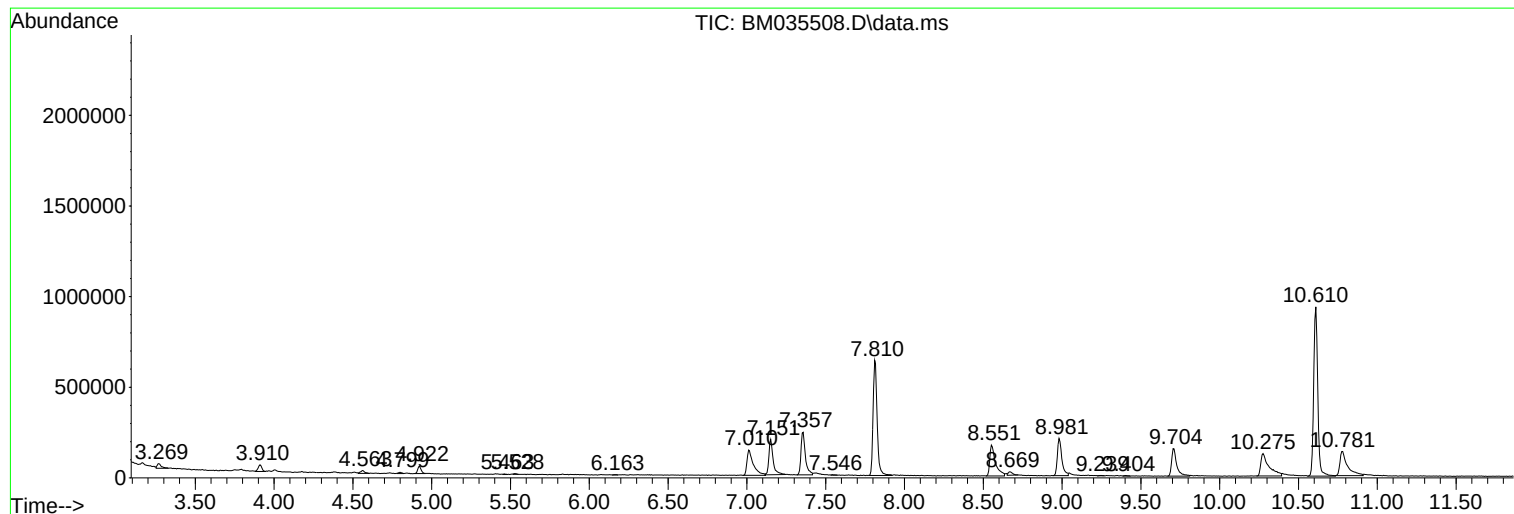

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035508.D
Acq On : 17 Jun 2022 23:48
Operator : CG/JU
Sample : N3226-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035508.D
Acq On : 17 Jun 2022 23:48
Operator : CG/JU
Sample : N3226-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------