

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035509.D
 Acq On : 18 Jun 2022 00:25
 Operator : CG/JU
 Sample : N3226-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035509.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	40	rVB	24480	40287	1.70%	0.164%
2	3.910	135	140	147	rBV3	34058	57577	2.43%	0.235%
3	4.004	154	156	161	rVB3	10120	13797	0.58%	0.056%
4	4.381	218	220	224	rVB5	5624	6998	0.30%	0.029%
5	4.563	247	251	258	rVB2	14796	22127	0.93%	0.090%
6	4.799	289	291	294	rVB3	7388	6563	0.28%	0.027%
7	4.922	308	312	319	rBV	40385	59521	2.51%	0.243%
8	5.528	412	415	420	rVB3	5137	7921	0.33%	0.032%
9	5.834	464	467	469	rBV4	2260	2805	0.12%	0.011%
10	6.687	608	612	614	rBV4	2096	3520	0.15%	0.014%
11	7.010	662	667	684	rBV	145447	403733	17.03%	1.646%
12	7.151	686	691	704	rVB	193777	347036	14.64%	1.415%
13	7.357	720	726	737	rBV	244510	478430	20.19%	1.951%
14	7.645	774	775	784	rVB9	2983	4753	0.20%	0.019%
15	7.810	797	803	821	rBV	536523	951883	40.16%	3.881%
16	7.975	830	831	836	rVB5	3119	3211	0.14%	0.013%
17	8.334	890	892	895	rBV4	2449	2440	0.10%	0.010%
18	8.551	923	929	944	rBV	182999	463805	19.57%	1.891%
19	8.663	945	948	957	rVB2	22248	49751	2.10%	0.203%
20	8.981	996	1002	1017	rBV	207238	439364	18.54%	1.791%
21	9.386	1067	1071	1072	rBV4	2235	2415	0.10%	0.010%
22	9.710	1119	1126	1142	rBV	150371	348245	14.69%	1.420%
23	10.275	1216	1222	1249	rBV	116964	475208	20.05%	1.938%
24	10.610	1271	1279	1297	rBV	821033	1452135	61.27%	5.921%
25	10.780	1301	1308	1329	rBV	118385	401741	16.95%	1.638%
26	12.175	1541	1545	1548	rBV6	1905	2515	0.11%	0.010%
27	12.251	1551	1558	1560	rBV7	4515	7862	0.33%	0.032%
28	12.827	1650	1656	1658	rBV7	2810	4706	0.20%	0.019%
29	13.074	1694	1698	1704	rVB6	6952	10902	0.46%	0.044%
30	13.298	1732	1736	1742	rVB8	3153	5820	0.25%	0.024%
31	13.363	1745	1747	1753	rVB6	2253	3865	0.16%	0.016%
32	13.810	1821	1823	1827	rVB5	2781	3740	0.16%	0.015%
33	13.874	1827	1834	1854	rBV	516540	896963	37.84%	3.657%
34	14.151	1874	1881	1894	rBV	644512	1061964	44.81%	4.330%
35	14.363	1914	1917	1921	rVB5	2992	4666	0.20%	0.019%
36	14.451	1926	1932	1942	rBV	1262477	1948402	82.21%	7.944%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035509.D
 Acq On : 18 Jun 2022 00:25
 Operator : CG/JU
 Sample : N3226-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4M9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

37	14.792	1980	1990	1991	rBV5	24538	36669	1.55%	0.150%
38	14.939	2008	2015	2029	rVB5	18095	56523	2.38%	0.230%
39	15.168	2053	2054	2057	rBV3	3346	2865	0.12%	0.012%
40	15.263	2063	2070	2073	rBV4	8658	16336	0.69%	0.067%
41	15.292	2073	2075	2084	rVB6	6491	12528	0.53%	0.051%
42	15.451	2096	2102	2114	rBV	903274	1425879	60.16%	5.814%
43	15.610	2123	2129	2141	rBV2	91359	213528	9.01%	0.871%
44	15.698	2141	2144	2151	rVB6	15503	28344	1.20%	0.116%
45	15.827	2162	2166	2170	rVB7	2888	4468	0.19%	0.018%
46	16.010	2193	2197	2200	rBV5	1998	3816	0.16%	0.016%
47	16.133	2214	2218	2219	rBV4	3018	3303	0.14%	0.013%
48	16.174	2222	2225	2227	rBV4	2906	3736	0.16%	0.015%
49	16.233	2233	2235	2236	rBV2	3379	3079	0.13%	0.013%
50	16.339	2250	2253	2255	rBV4	4095	5438	0.23%	0.022%
51	16.645	2303	2305	2307	rVB3	3236	2763	0.12%	0.011%
52	16.692	2310	2313	2319	rVB8	2594	5173	0.22%	0.021%
53	16.762	2321	2325	2329	rBV4	6868	11754	0.50%	0.048%
54	16.974	2357	2361	2363	rBV5	6725	8680	0.37%	0.035%
55	17.121	2383	2386	2391	rVB6	9150	11894	0.50%	0.048%
56	17.198	2393	2399	2411	rBV	1531288	2327051	98.18%	9.488%
57	17.304	2411	2417	2431	rVV	854752	1442255	60.85%	5.881%
58	17.421	2434	2437	2444	rVV7	21961	44826	1.89%	0.183%
59	17.498	2447	2450	2455	rVB4	8972	10989	0.46%	0.045%
60	17.709	2482	2486	2491	rBV7	3669	7570	0.32%	0.031%
61	17.880	2511	2515	2520	rVB6	12864	16756	0.71%	0.068%
62	17.992	2530	2534	2539	rBV8	9034	17502	0.74%	0.071%
63	18.051	2542	2544	2545	rVV2	5179	3771	0.16%	0.015%
64	18.104	2549	2553	2562	rVV2	86195	143016	6.03%	0.583%
65	18.180	2563	2566	2570	rVB	17772	22351	0.94%	0.091%
66	18.886	2684	2686	2687	rBV	5804	4420	0.19%	0.018%
67	19.168	2730	2734	2739	rBV6	15666	31737	1.34%	0.129%
68	19.239	2744	2746	2748	rVV2	17594	19641	0.83%	0.080%
69	19.268	2748	2751	2762	rVB	49873	81550	3.44%	0.333%
70	19.386	2767	2771	2778	rBV2	49965	77200	3.26%	0.315%
71	19.527	2793	2795	2801	rVB7	12290	10905	0.46%	0.044%
72	19.598	2801	2807	2820	rBV	1130742	1752161	73.93%	7.144%
73	21.103	3060	3063	3070	rBV4	105607	183104	7.73%	0.747%
74	21.392	3107	3112	3126	rBV	1533798	2350411	99.17%	9.583%
75	23.580	3478	3484	3498	rVB	797421	1754979	74.05%	7.156%
76	23.733	3503	3510	3526	rVB2	1122718	2370103	100.00%	9.664%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035509.D
Acq On : 18 Jun 2022 00:25
Operator : CG/JU
Sample : N3226-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4M9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Title : SVOA CALIBRATION




Sum of corrected areas: 24525745

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035509.D
Acq On : 18 Jun 2022 00:25
Operator : CG/JU
Sample : N3226-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4M9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

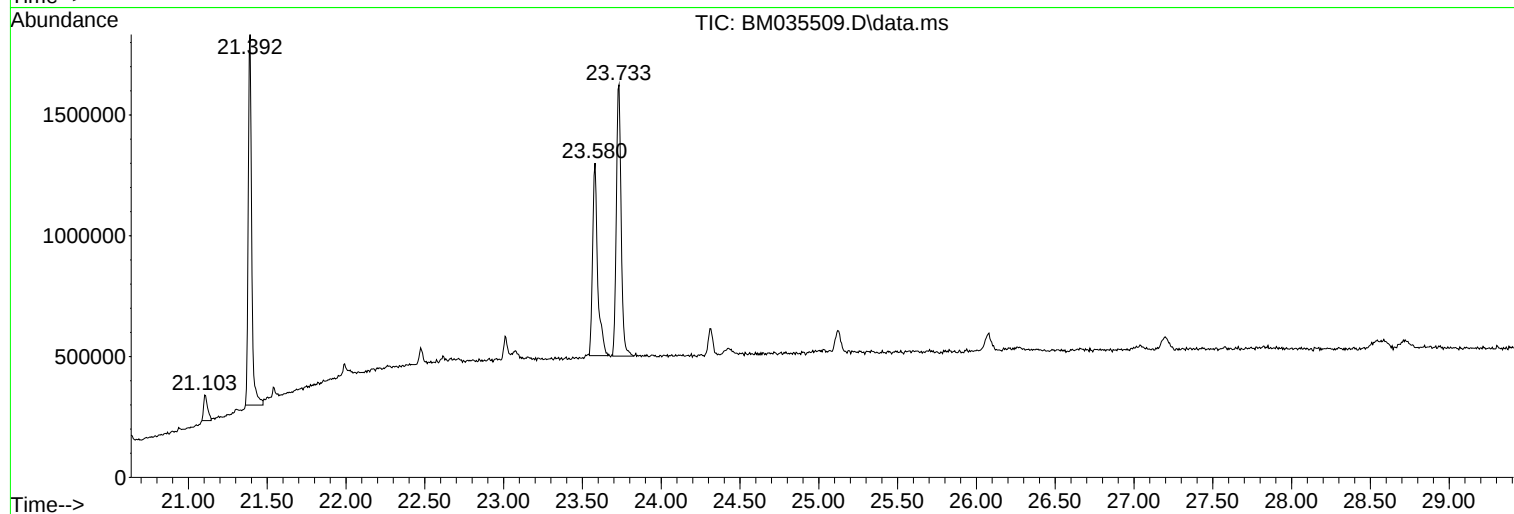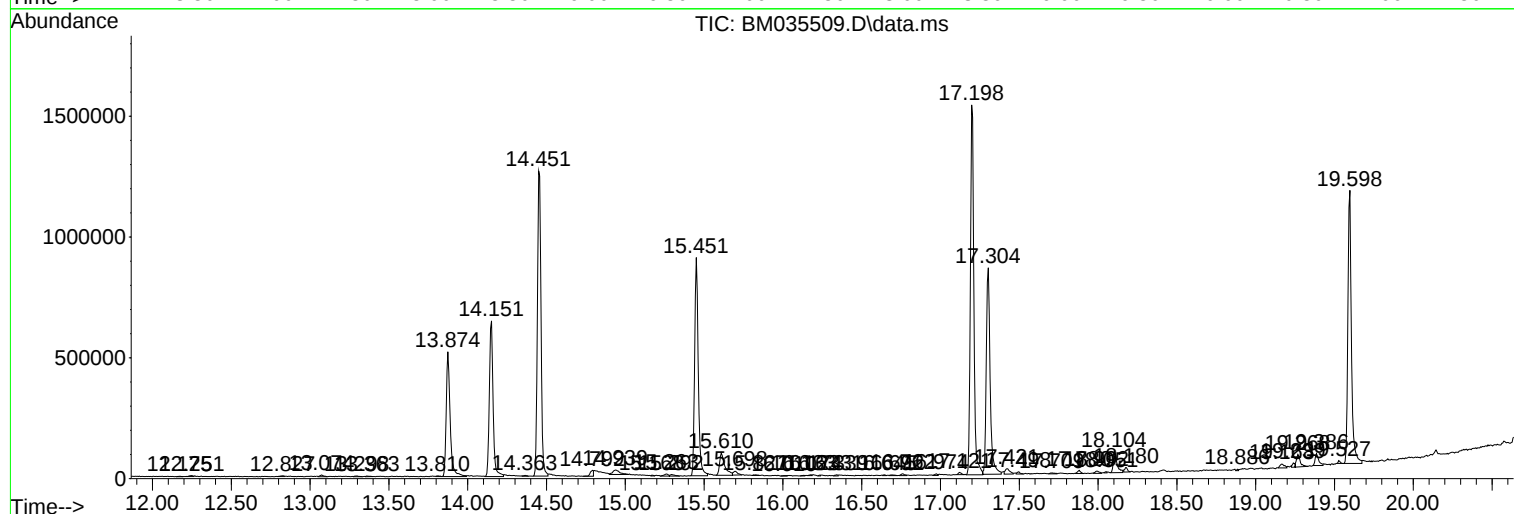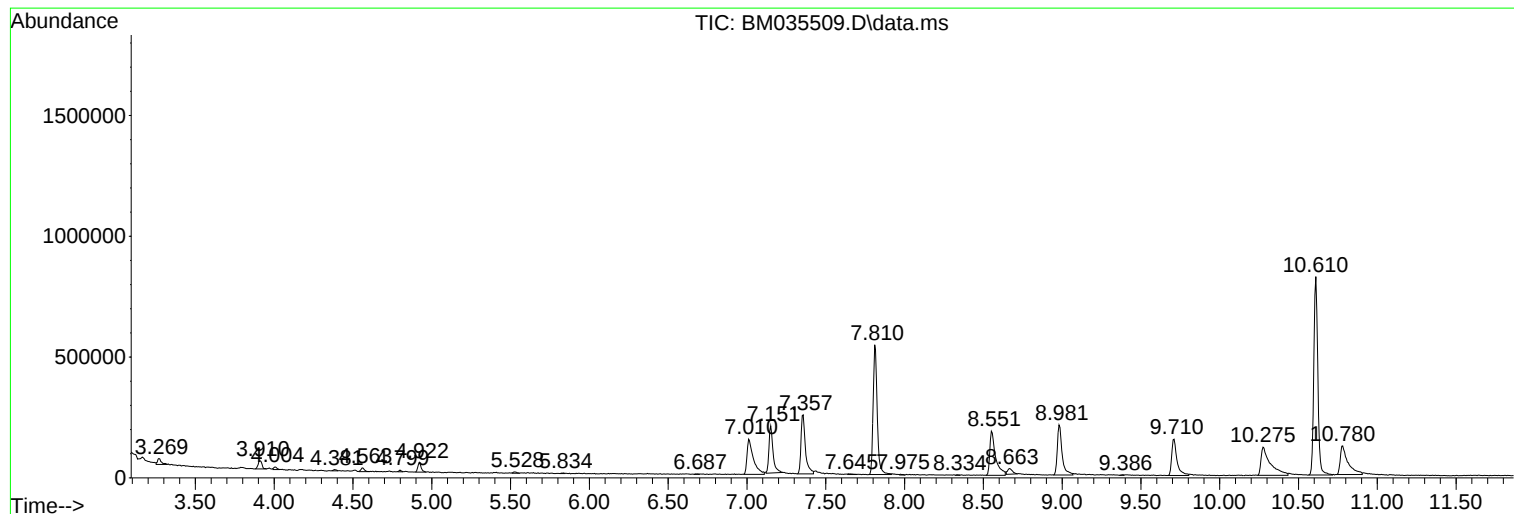

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035509.D
Acq On : 18 Jun 2022 00:25
Operator : CG/JU
Sample : N3226-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4M9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035509.D
Acq On : 18 Jun 2022 00:25
Operator : CG/JU
Sample : N3226-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4M9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------