

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035510.D
 Acq On : 18 Jun 2022 01:01
 Operator : CG/JU
 Sample : N3226-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035510.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	41	rVB	51370	82561	2.03%	0.187%
2	3.687	99	102	119	rBV	483993	861401	21.13%	1.946%
3	3.999	153	155	162	rVB2	13334	21761	0.53%	0.049%
4	4.557	248	250	256	rVB7	4972	8601	0.21%	0.019%
5	4.922	310	312	318	rVB2	9523	12343	0.30%	0.028%
6	6.998	660	665	684	rBV	452845	1015835	24.92%	2.295%
7	7.145	684	690	705	rVB	499934	853284	20.93%	1.928%
8	7.351	718	725	744	rBV	628127	1153673	28.30%	2.606%
9	7.810	797	803	818	rBV	654150	1144980	28.09%	2.586%
10	8.539	921	927	950	rBV	633582	1336343	32.78%	3.019%
11	8.975	993	1001	1019	rBV	566389	1051542	25.79%	2.375%
12	9.404	1070	1074	1079	rVB7	3495	6458	0.16%	0.015%
13	9.698	1118	1124	1141	rBV	435084	871199	21.37%	1.968%
14	10.257	1212	1219	1246	rBV	474419	1257032	30.83%	2.840%
15	10.610	1270	1279	1294	rBV	969894	1728040	42.39%	3.904%
16	10.763	1298	1305	1333	rBV	513478	1342691	32.94%	3.033%
17	12.245	1549	1557	1563	rVV3	9446	22173	0.54%	0.050%
18	13.080	1692	1699	1703	rBV6	4588	8470	0.21%	0.019%
19	13.369	1744	1748	1751	rVV4	5078	7745	0.19%	0.017%
20	13.527	1771	1775	1779	rBV6	2781	5985	0.15%	0.014%
21	13.868	1827	1833	1853	rBV	1320077	2109628	51.75%	4.766%
22	14.145	1873	1880	1897	rBV	1715787	2564156	62.90%	5.792%
23	14.363	1914	1917	1925	rVB9	4660	7075	0.17%	0.016%
24	14.451	1925	1932	1951	rBV	1540601	2235826	54.84%	5.051%
25	14.727	1974	1979	2005	rBV3	140723	692103	16.98%	1.563%
26	14.910	2008	2010	2018	rVB8	13035	28224	0.69%	0.064%
27	15.263	2065	2070	2073	rBV3	6286	10351	0.25%	0.023%
28	15.310	2076	2078	2082	rVB3	4991	5712	0.14%	0.013%
29	15.451	2095	2102	2116	rBV	1952294	3041364	74.60%	6.870%
30	15.592	2121	2126	2140	rVV	406864	812839	19.94%	1.836%
31	15.692	2140	2143	2154	rVB3	31544	64806	1.59%	0.146%
32	15.974	2187	2191	2193	rBV5	3120	4996	0.12%	0.011%
33	16.174	2221	2225	2231	rBV7	3946	7228	0.18%	0.016%
34	16.233	2233	2235	2241	rVB7	6523	8115	0.20%	0.018%
35	16.339	2249	2253	2255	rBV4	5299	5052	0.12%	0.011%
36	16.639	2300	2304	2307	rBV7	5301	7121	0.17%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035510.D
 Acq On : 18 Jun 2022 01:01
 Operator : CG/JU
 Sample : N3226-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

37	16.698	2311	2314	2318	rBV5	4439	5584	0.14%	0.013%
38	16.968	2356	2360	2363	rBV5	7056	11370	0.28%	0.026%
39	17.127	2384	2387	2390	rVB4	5898	7434	0.18%	0.017%
40	17.198	2393	2399	2410	rBV	1689011	2430665	59.62%	5.491%
41	17.298	2410	2416	2431	rVV	2108191	3214450	78.85%	7.261%
42	17.427	2435	2438	2443	rVB7	16597	27642	0.68%	0.062%
43	17.704	2482	2485	2488	rBV5	2899	4192	0.10%	0.009%
44	17.880	2511	2515	2522	rVB3	17477	21718	0.53%	0.049%
45	17.986	2529	2533	2538	rBV7	6766	13288	0.33%	0.030%
46	18.104	2549	2553	2562	rBV2	153593	246180	6.04%	0.556%
47	18.174	2563	2565	2570	rVB2	11988	17044	0.42%	0.039%
48	18.409	2602	2605	2609	rVB6	7014	9694	0.24%	0.022%
49	19.162	2730	2733	2742	rVB3	29363	40791	1.00%	0.092%
50	19.239	2742	2746	2749	rBV	33678	52417	1.29%	0.118%
51	19.386	2767	2771	2780	rBV3	75504	128062	3.14%	0.289%
52	19.533	2793	2796	2798	rVB2	12996	12662	0.31%	0.029%
53	19.592	2801	2806	2820	rVV	2562439	3735282	91.62%	8.438%
54	20.639	2982	2984	2989	rVB2	38053	33624	0.82%	0.076%
55	21.103	3059	3063	3071	rBV	237190	444926	10.91%	1.005%
56	21.386	3107	3111	3123	rBV2	1748184	2634712	64.63%	5.952%
57	23.574	3477	3483	3498	rVB	1915302	4076789	100.00%	9.209%
58	23.727	3503	3509	3522	rVB2	1305411	2702505	66.29%	6.105%




Sum of corrected areas: 44267744

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035510.D
Acq On : 18 Jun 2022 01:01
Operator : CG/JU
Sample : N3226-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

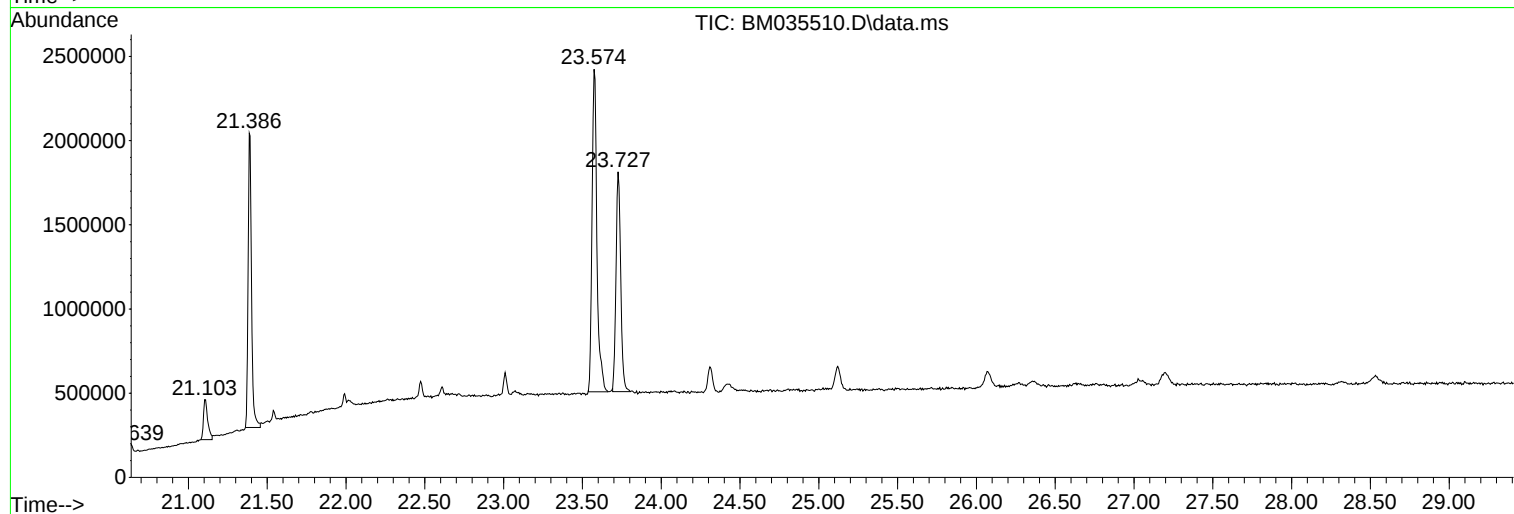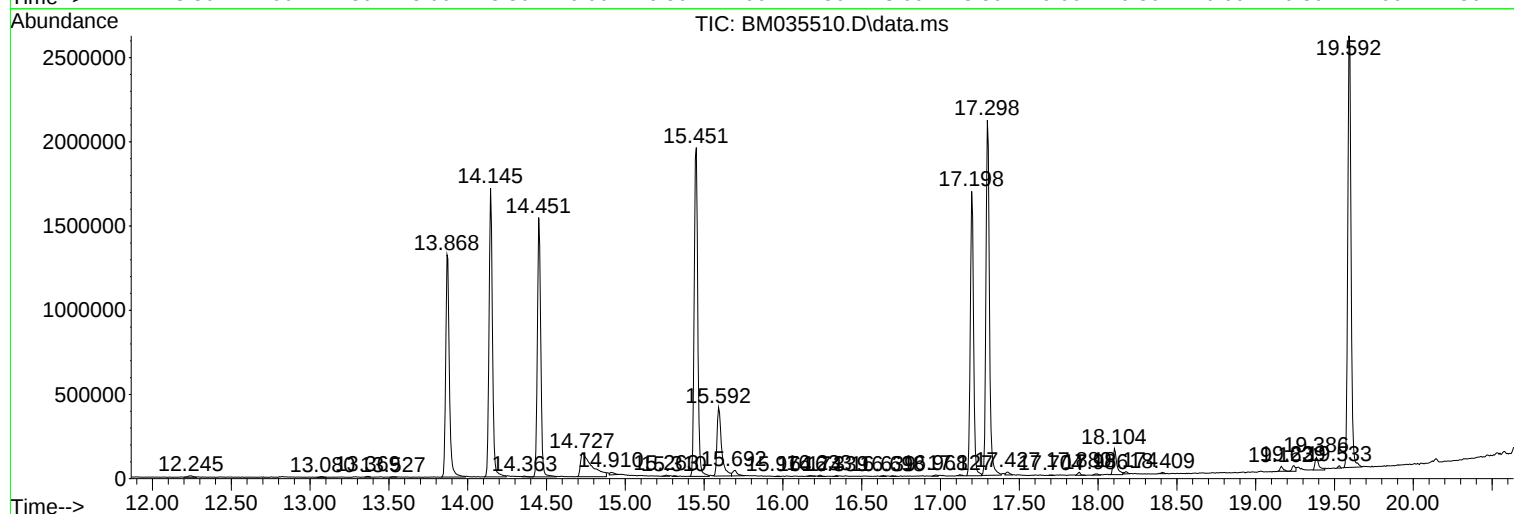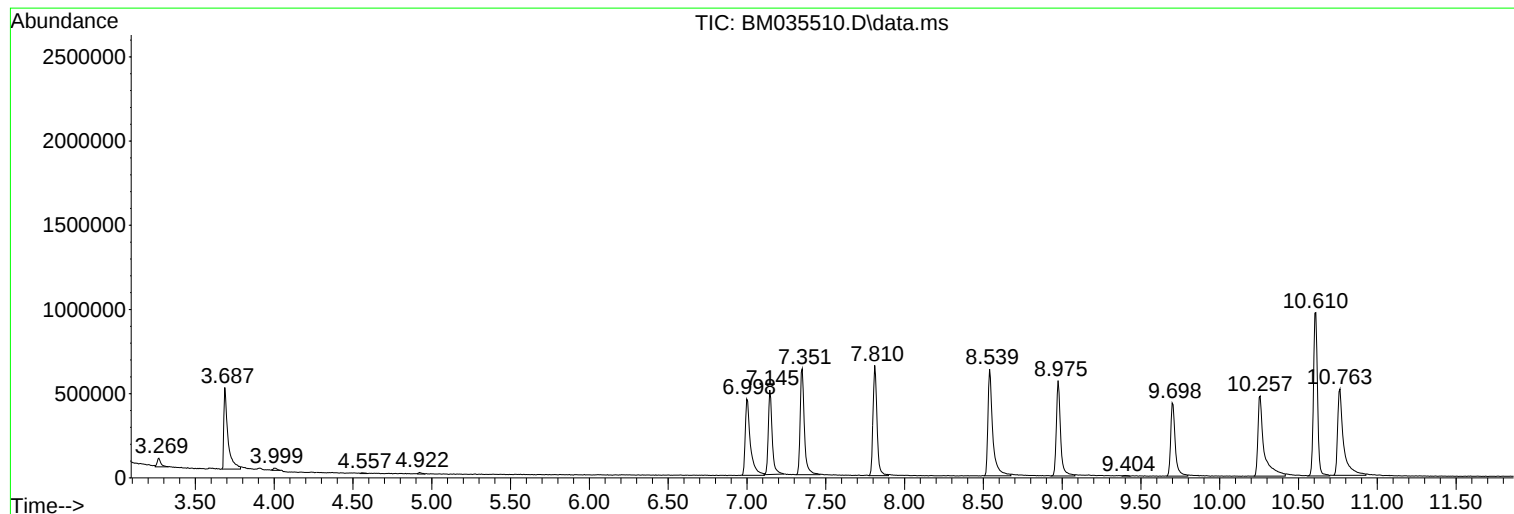

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035510.D
Acq On : 18 Jun 2022 01:01
Operator : CG/JU
Sample : N3226-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035510.D
Acq On : 18 Jun 2022 01:01
Operator : CG/JU
Sample : N3226-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc