

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035512.D
 Acq On : 18 Jun 2022 02:14
 Operator : CG/JU
 Sample : N3226-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	37	rVB	46603	60734	1.30%	0.126%
2	3.587	82	85	92	rBV3	7120	14531	0.31%	0.030%
3	3.687	99	102	125	rBV	430985	797350	17.04%	1.652%
4	4.005	152	156	167	rVB3	14820	27206	0.58%	0.056%
5	4.922	308	312	318	rBV3	9037	14749	0.32%	0.031%
6	6.998	659	665	684	rBV	429731	984580	21.04%	2.040%
7	7.145	684	690	709	rVB	503825	856143	18.30%	1.774%
8	7.351	718	725	737	rBV	609514	1103338	23.58%	2.286%
9	7.569	760	762	767	rVB6	3343	4718	0.10%	0.010%
10	7.810	796	803	816	rBV	676198	1189870	25.43%	2.465%
11	7.898	816	818	823	rVB6	4620	7028	0.15%	0.015%
12	8.540	921	927	947	rBV	635854	1323398	28.29%	2.742%
13	8.975	994	1001	1012	rBV	551921	1008749	21.56%	2.090%
14	9.151	1029	1031	1036	rVB6	3588	5895	0.13%	0.012%
15	9.404	1071	1074	1081	rVB6	3666	7790	0.17%	0.016%
16	9.698	1116	1124	1146	rBV	428866	861107	18.40%	1.784%
17	10.045	1179	1183	1189	rVB8	2458	5525	0.12%	0.011%
18	10.251	1212	1218	1250	rBV	468777	1223412	26.15%	2.534%
19	10.604	1270	1278	1292	rBV	1036450	1800882	38.49%	3.731%
20	10.757	1298	1304	1330	rBV	520585	1326212	28.35%	2.747%
21	11.145	1365	1370	1382	rVB9	10135	25962	0.55%	0.054%
22	11.645	1450	1455	1459	rVB4	5813	9723	0.21%	0.020%
23	12.045	1518	1523	1530	rBV3	12688	21105	0.45%	0.044%
24	12.233	1550	1555	1562	rBV4	9264	20254	0.43%	0.042%
25	12.998	1679	1685	1690	rVV8	6448	13104	0.28%	0.027%
26	13.063	1693	1696	1701	rVB7	4280	7667	0.16%	0.016%
27	13.286	1730	1734	1739	rVB	15298	21833	0.47%	0.045%
28	13.369	1743	1748	1753	rBV9	4565	8076	0.17%	0.017%
29	13.869	1827	1833	1849	rBV	1344289	2058164	43.99%	4.264%
30	14.145	1873	1880	1896	rBV	1665985	2504108	53.52%	5.188%
31	14.363	1913	1917	1922	rVB	19927	23807	0.51%	0.049%
32	14.451	1925	1932	1946	rBV	1591626	2377569	50.82%	4.926%
33	14.733	1974	1980	2006	rBV3	111368	563634	12.05%	1.168%
34	15.074	2036	2038	2045	rVB8	4032	7831	0.17%	0.016%
35	15.257	2065	2069	2072	rBV4	5803	9716	0.21%	0.020%
36	15.310	2075	2078	2083	rVB	14614	18674	0.40%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035512.D
 Acq On : 18 Jun 2022 02:14
 Operator : CG/JU
 Sample : N3226-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

37	15.445	2095	2101	2118	rBV	2073712	3237418	69.19%	6.707%
38	15.592	2121	2126	2139	rVV	353822	640402	13.69%	1.327%
39	15.698	2139	2144	2154	rVB3	32454	76273	1.63%	0.158%
40	16.174	2220	2225	2226	rBV2	15500	18956	0.41%	0.039%
41	16.198	2226	2229	2232	rVV	18342	24987	0.53%	0.052%
42	16.233	2232	2235	2242	rVB8	9832	17730	0.38%	0.037%
43	16.339	2248	2253	2254	rBV5	3341	4725	0.10%	0.010%
44	16.639	2299	2304	2305	rBV5	3586	5122	0.11%	0.011%
45	16.880	2342	2345	2347	rBV4	5041	5874	0.13%	0.012%
46	16.968	2356	2360	2364	rBV2	12815	20530	0.44%	0.043%
47	17.021	2364	2369	2373	rVB6	7479	14557	0.31%	0.030%
48	17.198	2392	2399	2410	rBV	1906433	2758781	58.96%	5.715%
49	17.298	2410	2416	2432	rVV	2335863	3514420	75.12%	7.281%
50	17.421	2434	2437	2443	rVV6	26945	58121	1.24%	0.120%
51	17.486	2446	2448	2456	rVV9	9520	20900	0.45%	0.043%
52	17.568	2458	2462	2465	rVV5	4286	6334	0.14%	0.013%
53	17.704	2482	2485	2491	rVB5	11200	12096	0.26%	0.025%
54	17.880	2512	2515	2519	rVB6	12364	15898	0.34%	0.033%
55	18.104	2548	2553	2563	rBV	252680	430678	9.21%	0.892%
56	18.398	2600	2603	2606	rBV2	12580	13391	0.29%	0.028%
57	19.033	2708	2711	2714	rBV3	10191	11360	0.24%	0.024%
58	19.162	2729	2733	2738	rBV3	33727	47910	1.02%	0.099%
59	19.239	2742	2746	2755	rBV2	35482	76127	1.63%	0.158%
60	19.386	2767	2771	2779	rBV	92194	144403	3.09%	0.299%
61	19.527	2793	2795	2799	rBV3	16660	17570	0.38%	0.036%
62	19.592	2801	2806	2814	rBV	2814364	4110489	87.86%	8.516%
63	20.145	2897	2900	2904	rVB	33894	38096	0.81%	0.079%
64	21.103	3059	3063	3074	rBV	635674	1150422	24.59%	2.383%
65	21.386	3106	3111	3123	rBV	2323553	3337153	71.33%	6.913%
66	23.574	3477	3483	3497	rVB2	2344798	4678688	100.00%	9.693%
67	23.727	3502	3509	3523	rVB	1640941	3446591	73.67%	7.140%




Sum of corrected areas: 48270446

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035512.D
Acq On : 18 Jun 2022 02:14
Operator : CG/JU
Sample : N3226-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

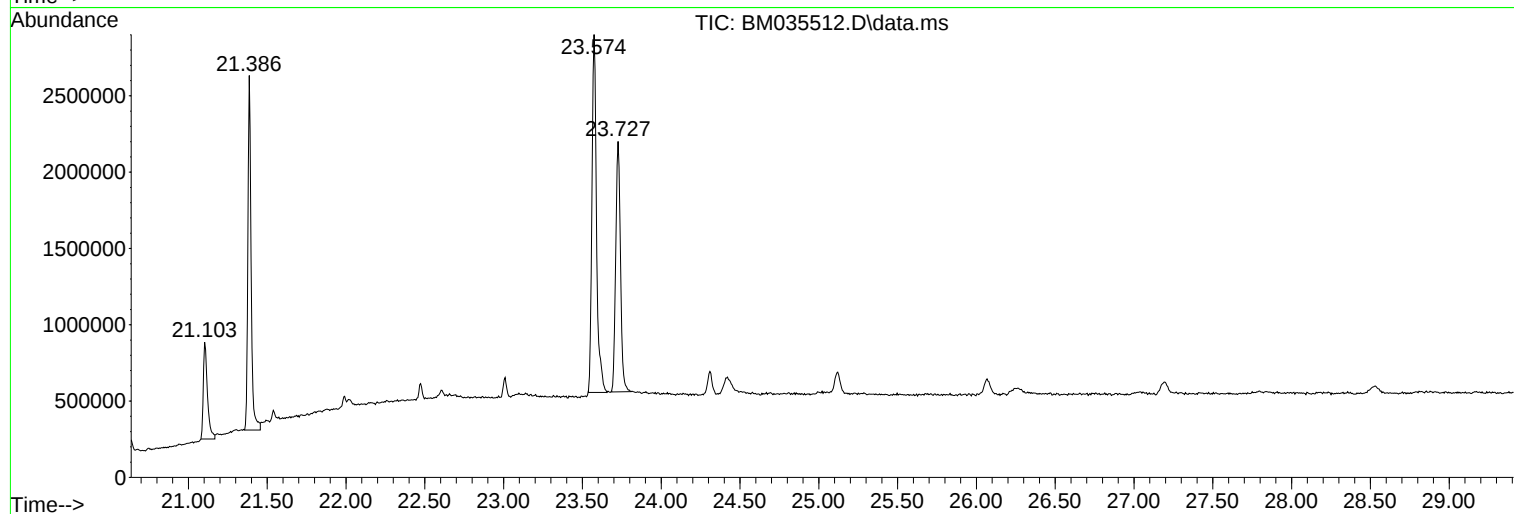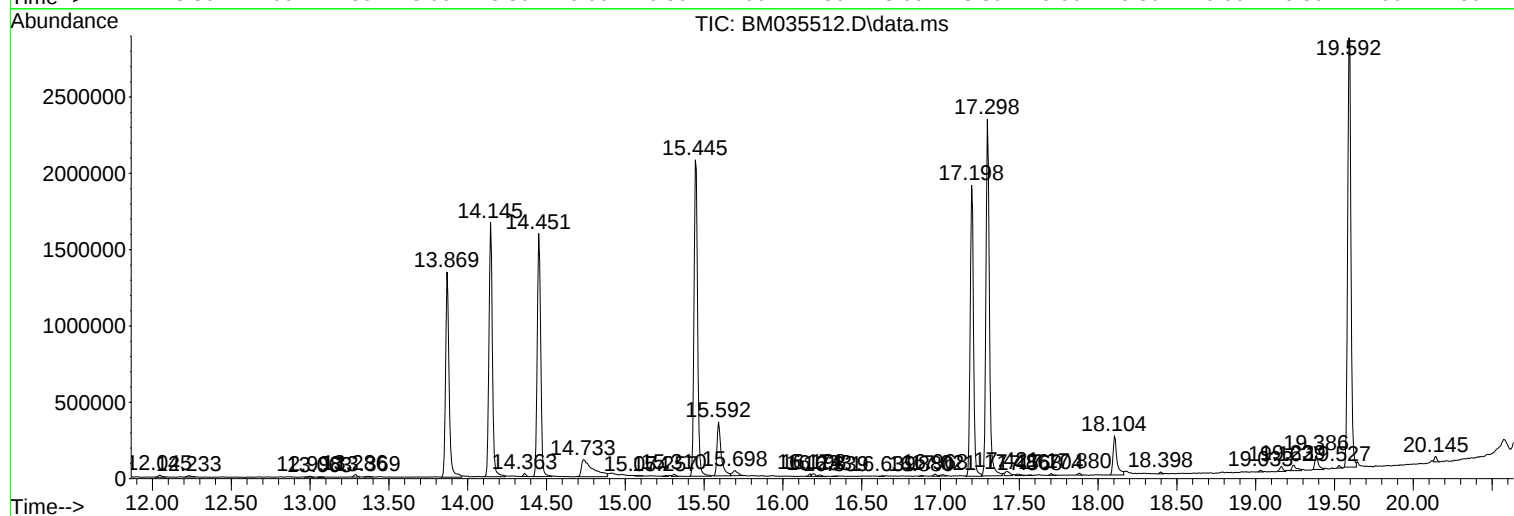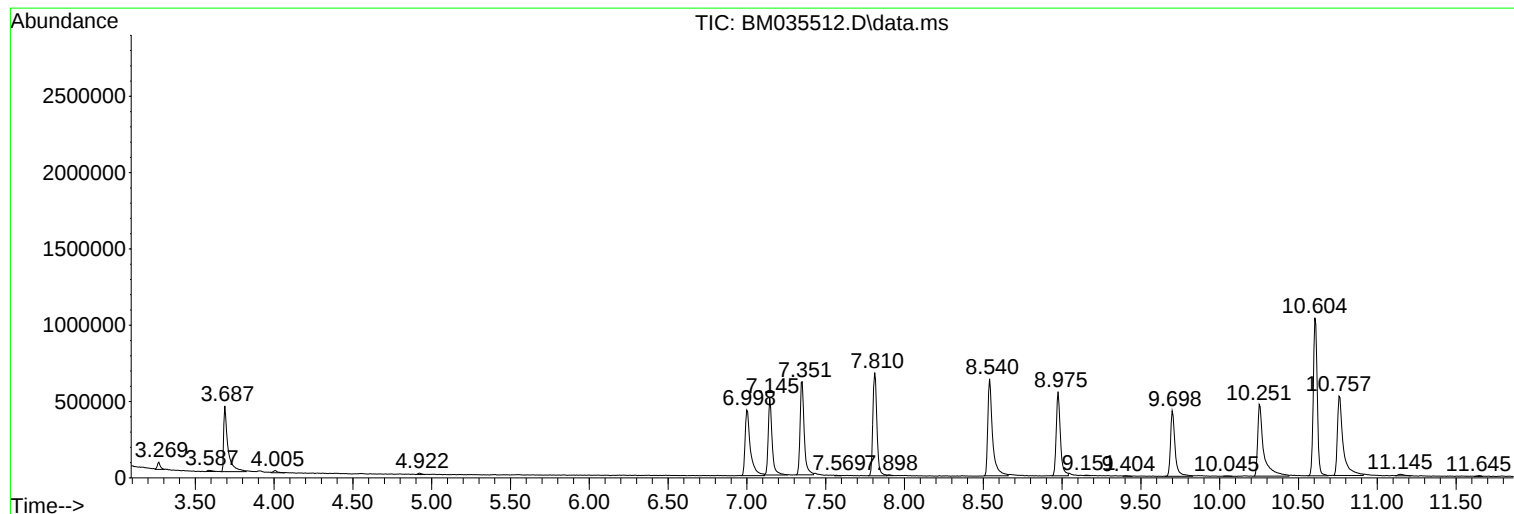

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035512.D
Acq On : 18 Jun 2022 02:14
Operator : CG/JU
Sample : N3226-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035512.D
Acq On : 18 Jun 2022 02:14
Operator : CG/JU
Sample : N3226-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc