

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035513.D
 Acq On : 18 Jun 2022 02:51
 Operator : CG/JU
 Sample : N3226-10
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	41	rVB3	25745	51548	1.55%	0.188%
2	3.910	135	140	147	rVB2	36510	60908	1.83%	0.222%
3	4.004	154	156	164	rVB2	15957	21618	0.65%	0.079%
4	4.557	246	250	257	rVB	14257	24516	0.74%	0.089%
5	4.734	278	280	284	rVB5	4585	4639	0.14%	0.017%
6	4.793	287	290	294	rBV4	8169	10236	0.31%	0.037%
7	4.922	307	312	323	rVB	40287	65951	1.98%	0.240%
8	5.528	412	415	417	rBV2	5613	4986	0.15%	0.018%
9	6.798	628	631	634	rBV4	2848	4240	0.13%	0.015%
10	6.957	655	658	661	rBV5	2323	3715	0.11%	0.014%
11	7.010	661	667	685	rVV	141474	398193	11.95%	1.451%
12	7.151	685	691	710	rVB	183362	357980	10.74%	1.304%
13	7.351	718	725	737	rBV	237343	457737	13.74%	1.668%
14	7.434	737	739	746	rVB5	12629	16846	0.51%	0.061%
15	7.810	797	803	823	rBV	661921	1137608	34.15%	4.145%
16	8.551	923	929	945	rBV	190795	473490	14.21%	1.725%
17	8.669	945	949	957	rVB2	19744	40554	1.22%	0.148%
18	8.980	994	1002	1017	rBV	195286	412847	12.39%	1.504%
19	9.704	1118	1125	1139	rBV	141142	321757	9.66%	1.172%
20	10.275	1216	1222	1249	rBV2	115520	457957	13.75%	1.668%
21	10.610	1272	1279	1296	rBV	923037	1702431	51.10%	6.202%
22	10.780	1299	1308	1329	rBV	125979	425610	12.77%	1.551%
23	12.239	1552	1556	1557	rBV4	3650	3725	0.11%	0.014%
24	12.816	1647	1654	1658	rBV8	3600	7676	0.23%	0.028%
25	13.080	1695	1699	1701	rVV4	3850	5305	0.16%	0.019%
26	13.874	1827	1834	1851	rBV	482316	823178	24.71%	2.999%
27	14.145	1873	1880	1899	rBV	593361	995455	29.88%	3.627%
28	14.451	1924	1932	1951	rBV	1468381	2278621	68.39%	8.302%
29	14.786	1984	1989	1991	rBV3	26899	45805	1.37%	0.167%
30	14.939	2009	2015	2021	rBV3	13472	31171	0.94%	0.114%
31	15.098	2040	2042	2049	rVB7	2503	4360	0.13%	0.016%
32	15.257	2065	2069	2073	rBV4	5582	8877	0.27%	0.032%
33	15.451	2096	2102	2115	rBV	822382	1323219	39.72%	4.821%
34	15.609	2123	2129	2141	rBV2	91499	200338	6.01%	0.730%
35	15.698	2141	2144	2149	rVV7	14084	26821	0.81%	0.098%
36	16.245	2233	2237	2239	rBV5	3589	4174	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035513.D
 Acq On : 18 Jun 2022 02:51
 Operator : CG/JU
 Sample : N3226-10
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

37	16.339	2248	2253	2259	rBV10	4373	8848	0.27%	0.032%
38	16.698	2312	2314	2318	rVB5	2745	3628	0.11%	0.013%
39	16.768	2321	2326	2329	rBV6	4516	8040	0.24%	0.029%
40	16.974	2356	2361	2363	rBV5	3788	6254	0.19%	0.023%
41	17.121	2383	2386	2392	rVB8	5959	10992	0.33%	0.040%
42	17.198	2392	2399	2411	rBV	1743326	2606222	78.23%	9.495%
43	17.303	2411	2417	2433	rVV2	851141	1461393	43.86%	5.324%
44	17.421	2433	2437	2444	rVV8	24530	49582	1.49%	0.181%
45	17.492	2447	2449	2456	rVB6	7519	9915	0.30%	0.036%
46	17.880	2511	2515	2519	rVB7	9678	12332	0.37%	0.045%
47	17.998	2533	2535	2539	rVB5	7741	7867	0.24%	0.029%
48	18.103	2548	2553	2562	rBV	94320	158807	4.77%	0.579%
49	18.180	2562	2566	2571	rVB	12987	23150	0.69%	0.084%
50	18.409	2602	2605	2610	rBV6	6528	11772	0.35%	0.043%
51	19.162	2730	2733	2736	rBV3	16468	21717	0.65%	0.079%
52	19.245	2744	2747	2748	rBV	13993	14103	0.42%	0.051%
53	19.268	2748	2751	2757	rVB2	38027	54055	1.62%	0.197%
54	19.386	2767	2771	2778	rBV3	52263	81405	2.44%	0.297%
55	19.533	2793	2796	2798	rVB4	13095	13667	0.41%	0.050%
56	19.597	2801	2807	2819	rBV	1189328	1804820	54.17%	6.575%
57	21.109	3060	3064	3073	rBV2	143053	268408	8.06%	0.978%
58	21.386	3106	3111	3122	rBV	2300381	3243936	97.37%	11.818%
59	23.574	3478	3483	3500	rVB	895323	2021616	60.68%	7.365%
60	23.727	3503	3509	3524	rVB2	1586494	3331663	100.00%	12.138%




Sum of corrected areas: 27448284

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035513.D
Acq On : 18 Jun 2022 02:51
Operator : CG/JU
Sample : N3226-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

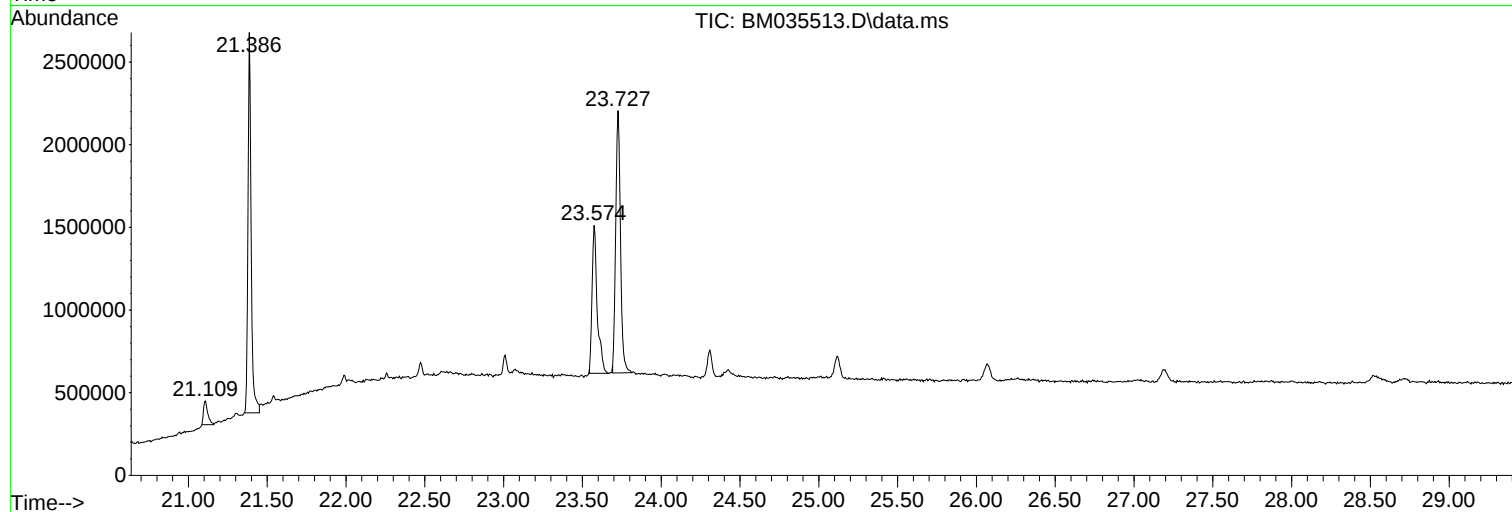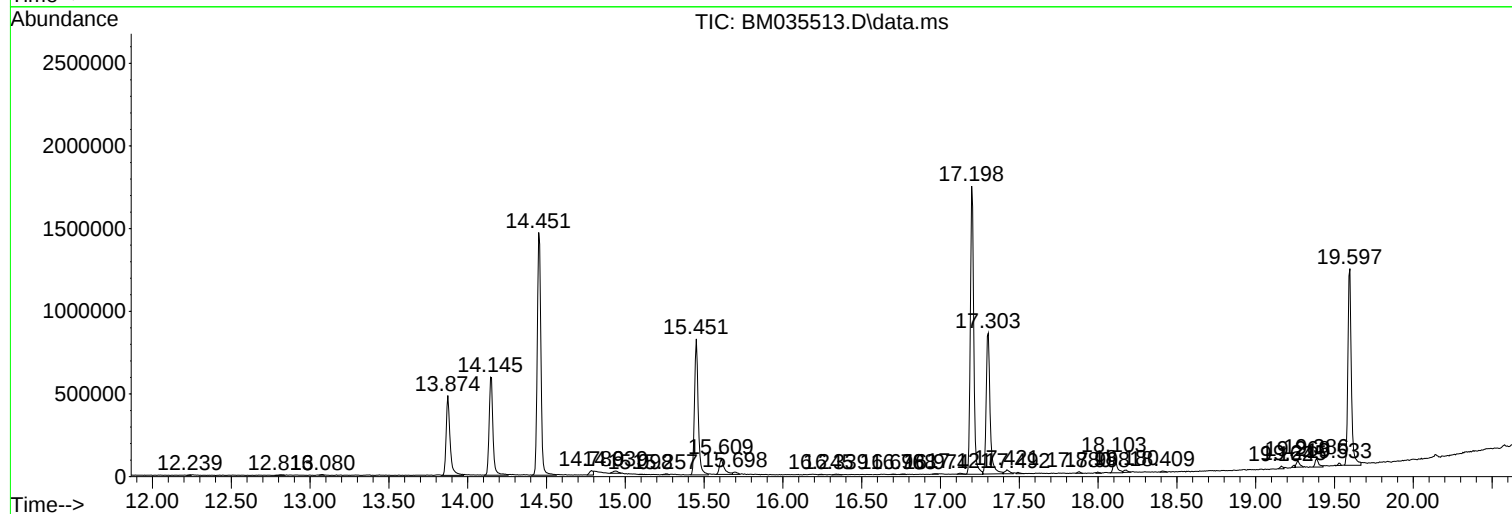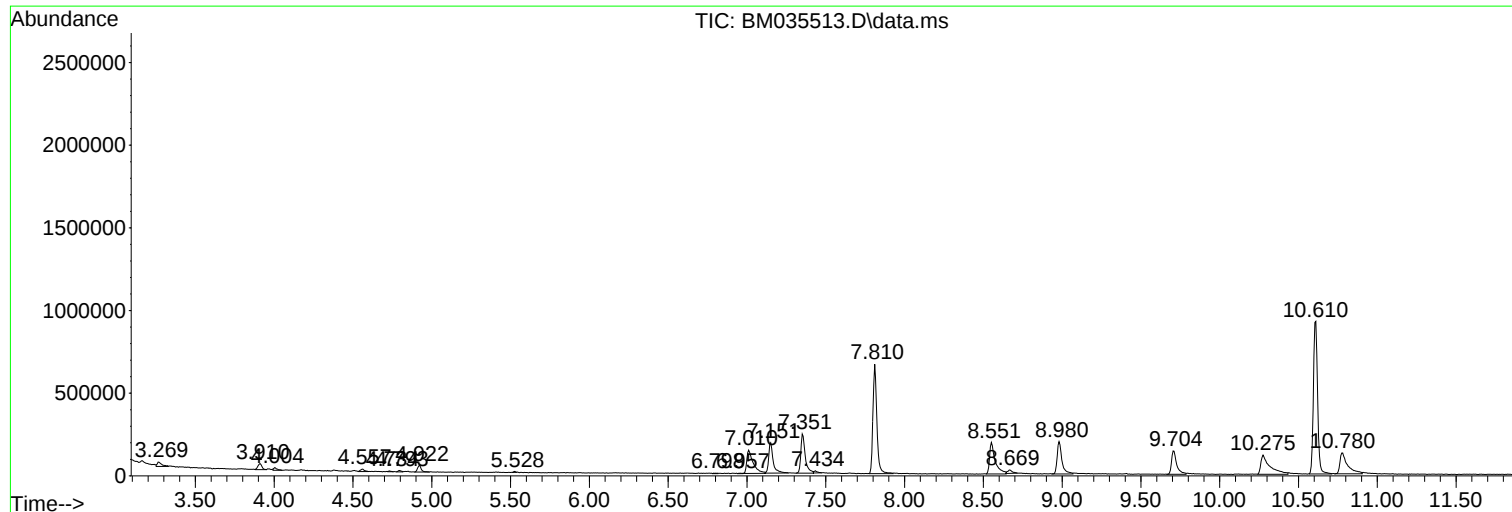

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035513.D
Acq On : 18 Jun 2022 02:51
Operator : CG/JU
Sample : N3226-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035513.D
Acq On : 18 Jun 2022 02:51
Operator : CG/JU
Sample : N3226-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------