

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030852.D
 Acq On : 07 Jul 2021 11:32
 Operator : CG/JU
 Sample : M2854-07
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDS9

Quant Time: Jul 07 12:30:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 06 14:32:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	94846	20.000	ng/ul	0.00
20) Naphthalene-d8	10.545	136	392815	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.392	164	241677	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.133	188	441314	20.000	ng/ul	0.00
79) Chrysene-d12	21.303	240	331819	20.000	ng/ul	0.00
88) Perylene-d12	23.550	264	349096	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.263	96	6265	2.581	ng/uL	0.00
4) Pyridine-d5	3.693	84	40622	6.400	ng/ul	0.02
7) Phenol-d5	6.934	99	117378	14.163	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.098	67	82268	15.411	ng/ul	0.00
11) 2-Chlorophenol-d4	7.298	132	97916	15.400	ng/ul	0.00
15) 4-Methylphenol-d8	8.463	113	92379	13.909	ng/ul	0.00
21) Nitrobenzene-d5	8.922	128	45467	15.562	ng/ul	0.00
24) 2-Nitrophenol-d4	9.639	143	49026	15.336	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.175	165	91553	14.882	ng/ul	0.00
31) 4-Chloroaniline-d4	10.686	131	115961	13.274	ng/ul	0.00
46) Dimethylphthalate-d6	13.804	166	300846	17.781	ng/ul	0.00
49) Acenaphthylene-d8	14.086	160	355486	16.633	ng/ul	0.00
54) 4-Nitrophenol-d4	14.610	143	22352	7.591	ng/ul	0.01
60) Fluorene-d10	15.386	176	255089	17.122	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.516	200	25188	8.901	ng/ul	0.00
73) Anthracene-d10	17.227	188	356871	17.353	ng/ul	0.00
81) Pyrene-d10	19.515	212	349017	19.071	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.403	264	291151	16.157	ng/ul	0.00


Target Compounds					Qvalue	
80) Fluoranthene	19.186	202	24067	1.067	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030852.D
Acq On : 07 Jul 2021 11:32
Operator : CG/JU
Sample : M2854-07
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDS9

Quant Time: Jul 07 12:30:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 06 14:32:50 2021
Response via : Initial Calibration

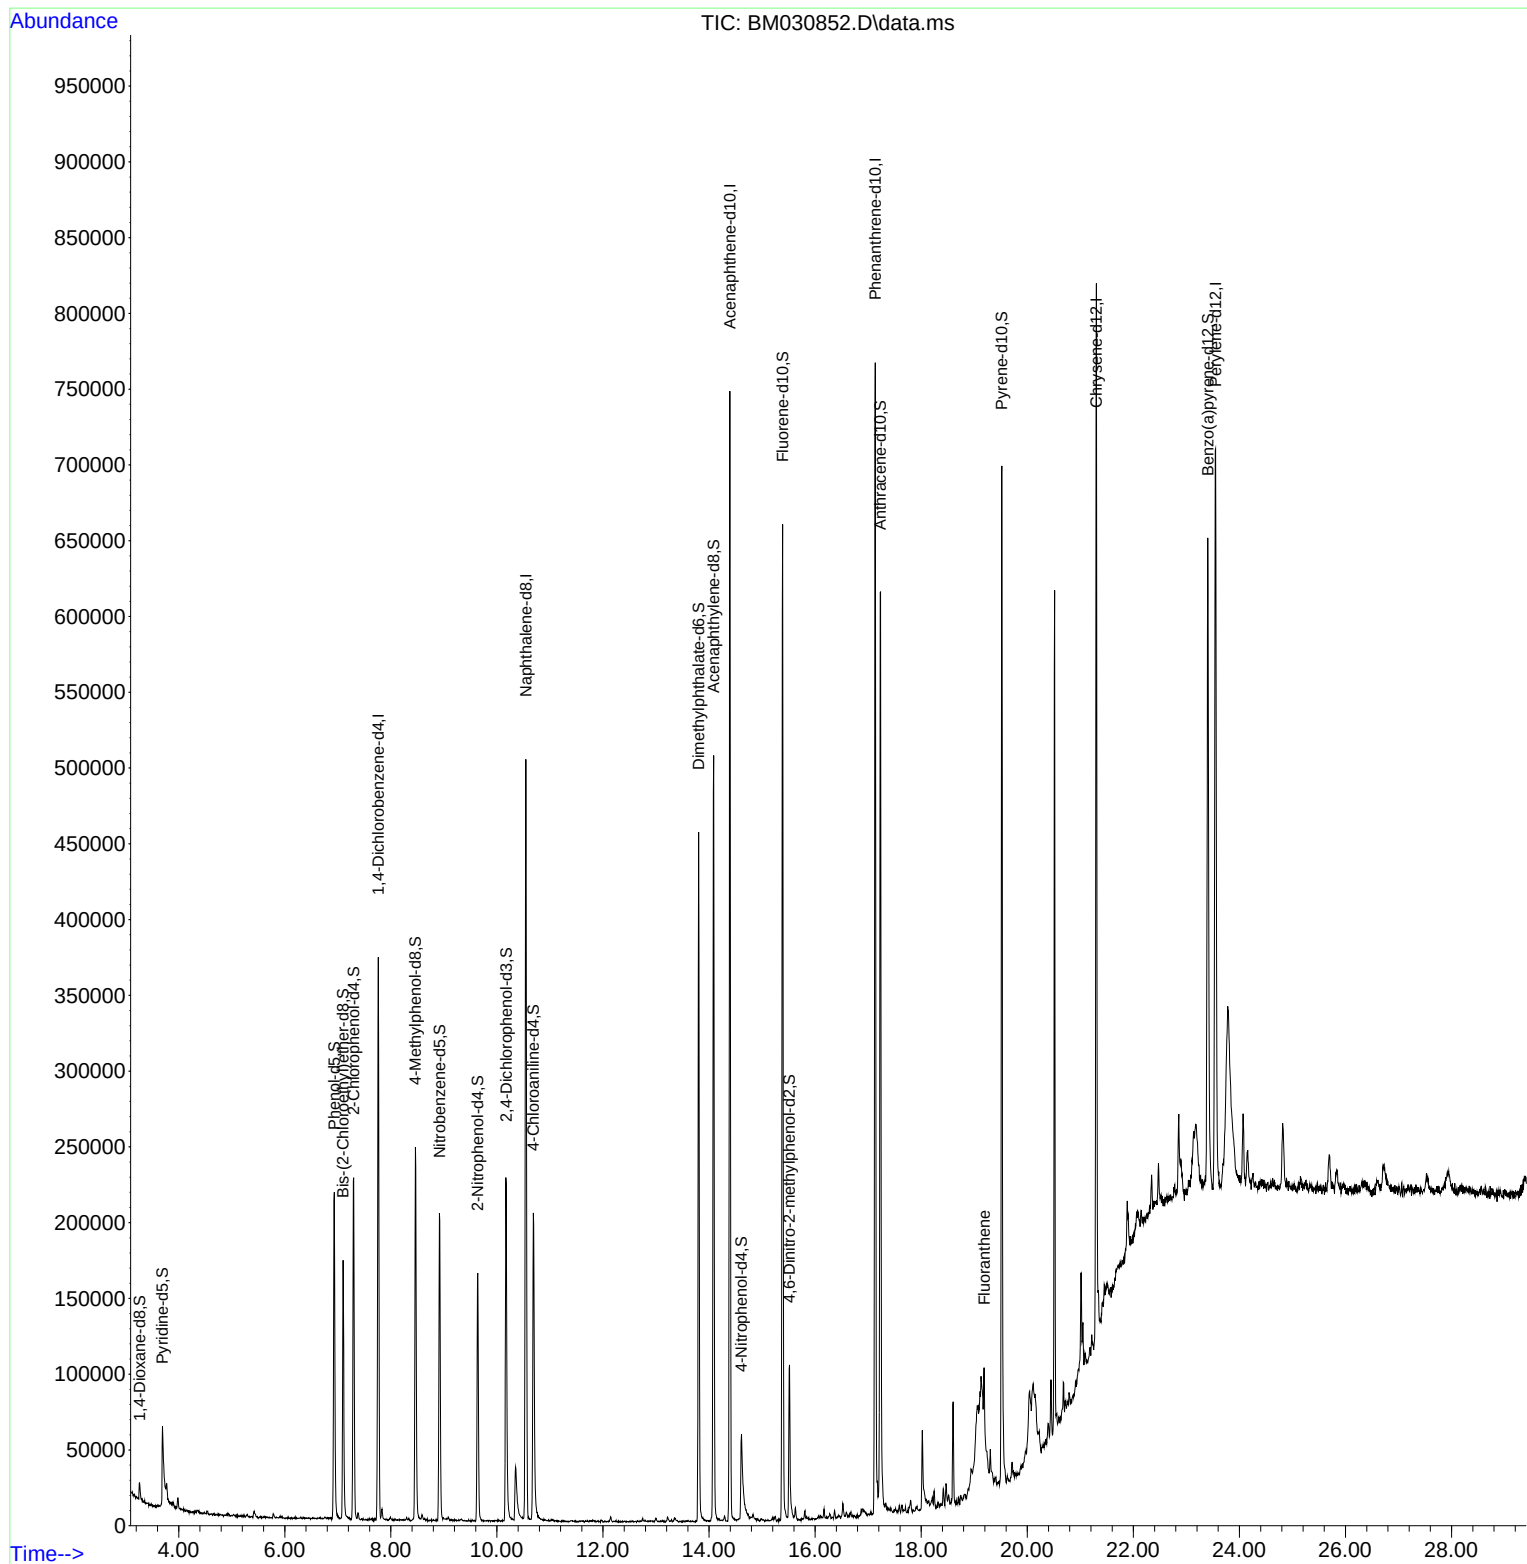

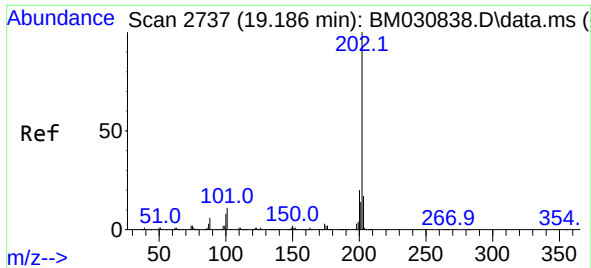

#80
Fluoranthene
Concen: 1.067 ng/ul
RT: 19.186 min Scan# 2737
Delta R.T. 0.000 min
Lab File: BM030852.D
Acq: 07 Jul 2021 11:32

Instrument :
BNA_M
ClientSampleId :
BGDS9

Tgt Ion	Ratio	Lower	Upper
202	100		
101	11.3	8.8	13.2
100	10.2	6.7	10.1

