

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030857.D
 Acq On : 07 Jul 2021 15:15
 Operator : CG/JU
 Sample : M2905-09DL 5X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK25DL

Quant Time: Jul 07 16:00:39 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 06 14:32:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	90701	20.000	ng/ul	0.00
20) Naphthalene-d8	10.545	136	372265	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.392	164	229258	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.133	188	428037	20.000	ng/ul	0.00
79) Chrysene-d12	21.303	240	338119	20.000	ng/ul	0.00
88) Perylene-d12	23.550	264	356736	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.940	99	4083	0.515	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.104	67	13271	2.600	ng/ul	0.00
11) 2-Chlorophenol-d4	7.298	132	11769	1.936	ng/ul	0.00
15) 4-Methylphenol-d8	8.475	113	7054	1.111	ng/ul	0.00
21) Nitrobenzene-d5	8.922	128	6226	2.249	ng/ul	0.00
24) 2-Nitrophenol-d4	9.639	143	6414	2.117	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.181	165	10982	1.884	ng/ul	0.00
31) 4-Chloroaniline-d4	10.698	131	13795	1.666	ng/ul	0.00
46) Dimethylphthalate-d6	13.810	166	55898	3.483	ng/ul	0.00
49) Acenaphthylene-d8	14.086	160	53539	2.641	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
60) Fluorene-d10	15.386	176	45545	3.223	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.521	200	11523	4.198	ng/ul	0.00
73) Anthracene-d10	17.233	188	73074	3.663	ng/ul	0.00
81) Pyrene-d10	19.521	212	69980	3.753	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.409	264	64238	3.489	ng/ul	0.00
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	15.027	232	6980	1.805	ng/ul#	94
71) Pentachlorophenol	16.786	266	69425	22.330	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030857.D
Acq On : 07 Jul 2021 15:15
Operator : CG/JU
Sample : M2905-09DL 5X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK25DL

Quant Time: Jul 07 16:00:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 06 14:32:50 2021
Response via : Initial Calibration

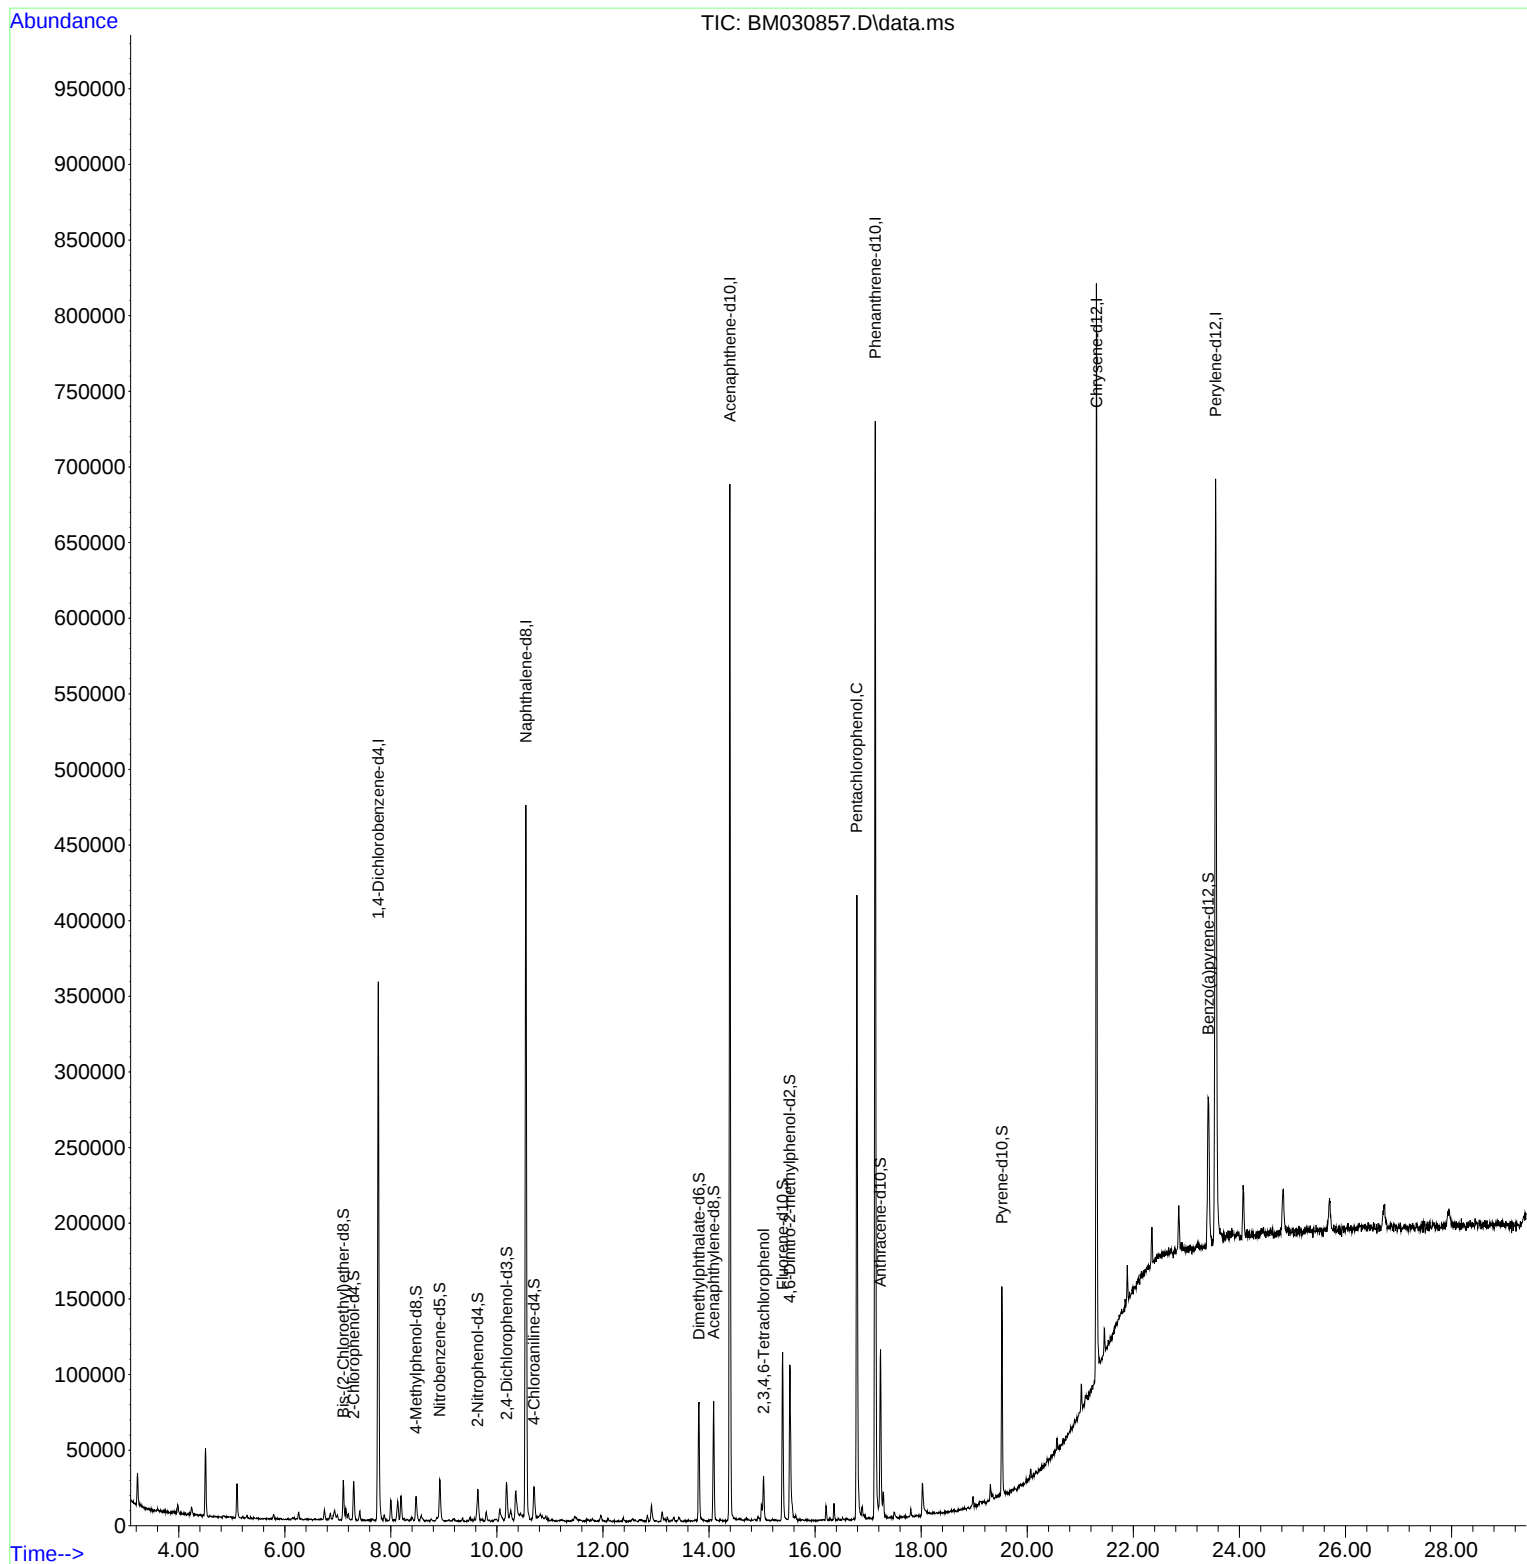




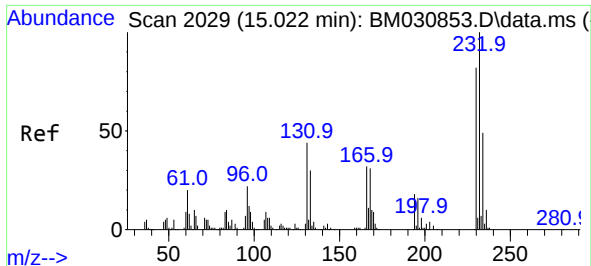


#58
2,3,4,6-Tetrachlorophenol
Concen: 1.805 ng/ul
RT: 15.027 min Scan# 2030
Delta R.T. 0.006 min
Lab File: BM030857.D
Acq: 07 Jul 2021 15:15

Instrument :
BNA_M
ClientSampleId :
DBK25DL

Tgt Ion:232 Resp: 6980

Ion	Ratio	Lower	Upper
232	100		
131	48.9	35.3	52.9
130	0.0	2.5	3.7#
166	28.2	24.3	36.5

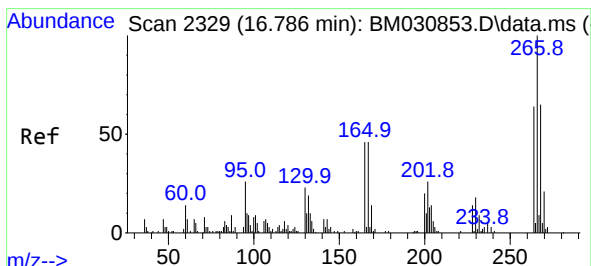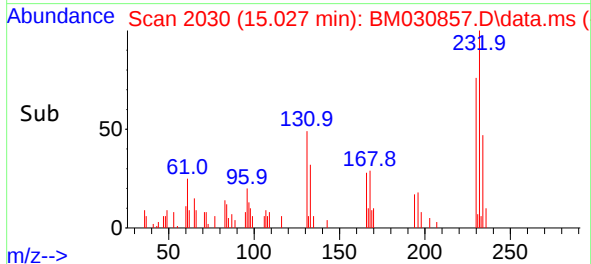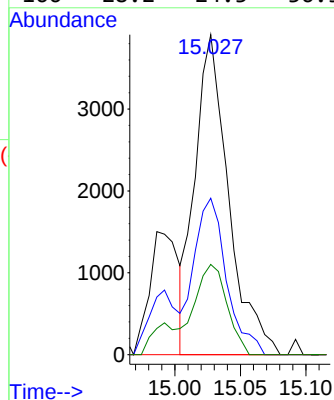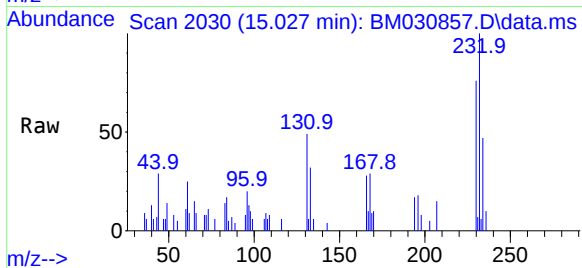

#71
Pentachlorophenol
Concen: 22.330 ng/ul
RT: 16.786 min Scan# 2329
Delta R.T. -0.006 min
Lab File: BM030857.D
Acq: 07 Jul 2021 15:15

Tgt Ion:266 Resp: 69425

Ion	Ratio	Lower	Upper
266	100		
264	64.7	48.5	72.7
268	64.4	49.3	73.9

