

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030866.D
 Acq On : 07 Jul 2021 20:52
 Operator : CG/JU
 Sample : M2877-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY9

Manual Integrations
 APPROVED

mohammad
 7/8/2021 12:38:12 PM

Quant Time: Jul 08 00:47:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 06 14:32:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	82086	20.000	ng/ul	0.00
20) Naphthalene-d8	10.545	136	336360	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.392	164	202676	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.133	188	363945	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	303128	20.000	ng/ul	0.00
88) Perylene-d12	23.544	264	324657	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.263	96	4157	1.979	ng/uL	0.00
4) Pyridine-d5	3.710	84	23288m	4.239	ng/ul	0.04
7) Phenol-d5	6.934	99	63166	8.807	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.098	67	47402	10.260	ng/ul	0.00
11) 2-Chlorophenol-d4	7.298	132	54578	9.918	ng/ul	0.00
15) 4-Methylphenol-d8	8.463	113	51095	8.889	ng/ul	0.00
21) Nitrobenzene-d5	8.922	128	23642	9.450	ng/ul	0.00
24) 2-Nitrophenol-d4	9.639	143	23742	8.674	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.175	165	43899	8.334	ng/ul	0.00
31) 4-Chloroaniline-d4	10.692	131	63869	8.538	ng/ul	0.00
46) Dimethylphthalate-d6	13.804	166	150380	10.598	ng/ul	0.00
49) Acenaphthylene-d8	14.086	160	175913	9.815	ng/ul	0.00
54) 4-Nitrophenol-d4	14.627	143	8891m	3.601	ng/ul	0.03
60) Fluorene-d10	15.386	176	127328	10.191	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.521	200	9611	4.118	ng/ul	0.00
73) Anthracene-d10	17.233	188	187274	11.042	ng/ul	0.00
81) Pyrene-d10	19.515	212	176099	10.533	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.403	264	152520	9.101	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.851	163	34541	2.485	ng/ul	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030866.D
Acq On : 07 Jul 2021 20:52
Operator : CG/JU
Sample : M2877-01
Misc :
ALS Vial : 43 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BGDY9

Manual Integrations
APPROVED

mohammad
7/8/2021 12:38:12 PM

Quant Time: Jul 08 00:47:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 06 14:32:50 2021
Response via : Initial Calibration

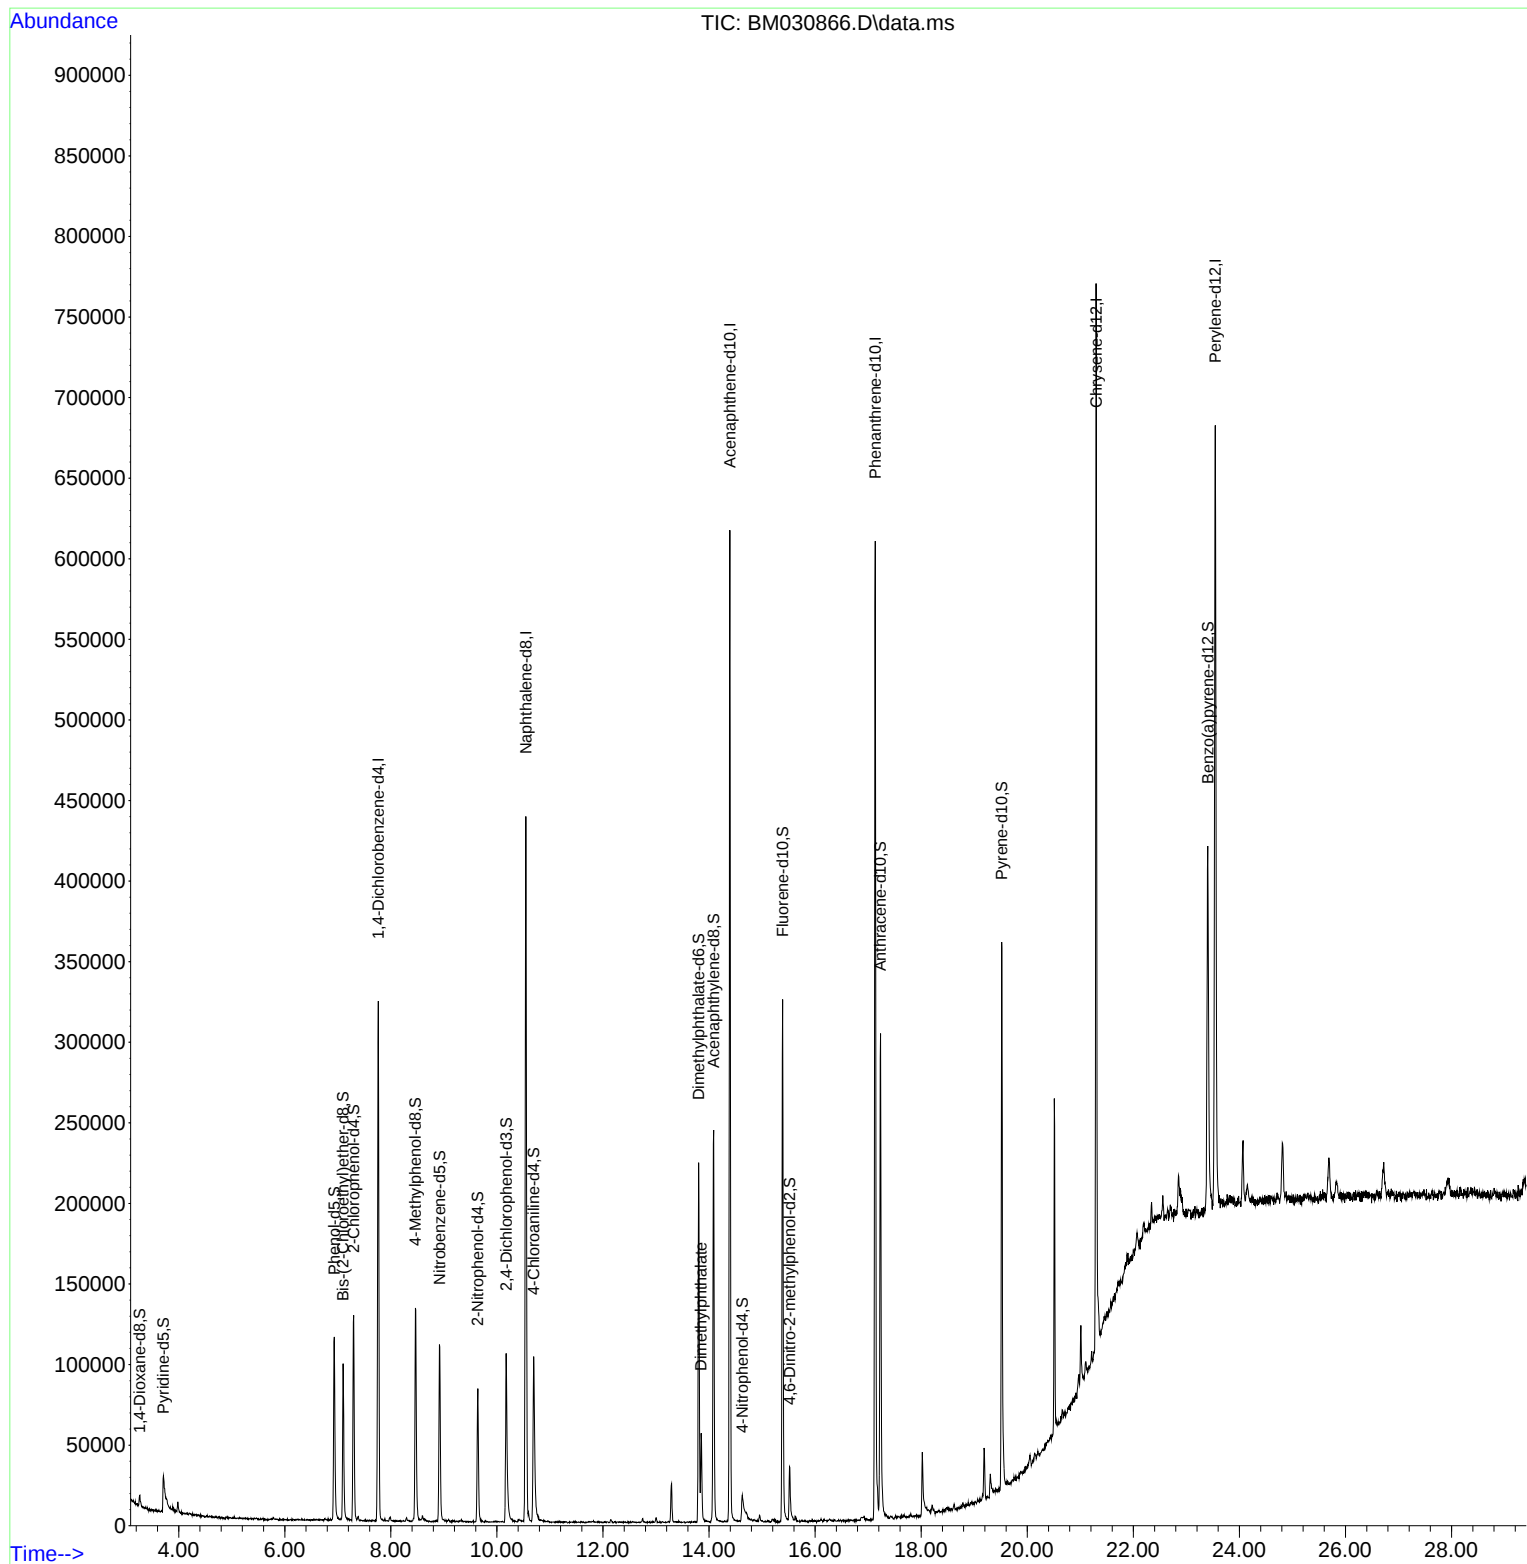

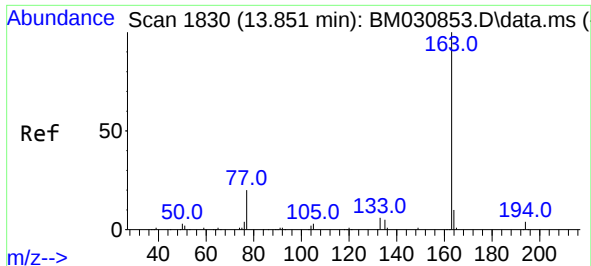

#47
Dimethylphthalate
Concen: 2.485 ng/ul
RT: 13.851 min Scan# 1830
Delta R.T. -0.006 min
Lab File: BM030866.D
Acq: 07 Jul 2021 20:52

Tgt Ion:	163	Resp:	34541
Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.2	4.8
164	9.3	7.8	11.8

Instrument :
BNA_M
ClientSampleId :
BGDY9

Manual Integrations
APPROVED

mohammad
7/8/2021 12:38:12 PM

