

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030822.D
 Acq On : 06 Jul 2021 15:31
 Operator : CG/JU
 Sample : PB137472BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK472

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030822.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	26	29	35	rVB	29334	36559	1.38%	0.139%
2	3.669	96	99	121	rBV	275844	549701	20.80%	2.090%
3	3.987	149	153	157	rVB	8378	11306	0.43%	0.043%
4	6.934	647	654	665	rBV	449212	718545	27.19%	2.732%
5	7.104	677	683	694	rBV	338153	555643	21.03%	2.112%
6	7.298	709	716	728	rVB	469608	754300	28.54%	2.868%
7	7.763	785	795	806	rBV	319994	519895	19.67%	1.977%
8	8.463	908	914	928	rBV	513656	869688	32.91%	3.306%
9	8.922	984	992	1006	rBV	427885	715505	27.08%	2.720%
10	9.639	1107	1114	1126	rBV	358848	600170	22.71%	2.282%
11	10.175	1197	1205	1226	rBV	470342	886166	33.53%	3.369%
12	10.551	1261	1269	1277	rBV	437562	737984	27.93%	2.806%
13	10.692	1285	1293	1315	rBV	466380	919967	34.81%	3.498%
14	12.157	1533	1542	1550	rBV3	6048	11529	0.44%	0.044%
15	13.810	1816	1823	1834	rBV	947861	1402216	53.06%	5.331%
16	14.086	1863	1870	1886	rBV	1126049	1646112	62.29%	6.258%
17	14.392	1916	1922	1931	rBV	688215	1029041	38.94%	3.912%
18	14.598	1950	1957	1982	rBV	280226	638014	24.14%	2.426%
19	15.386	2084	2091	2102	rBV	1440176	2085082	78.90%	7.927%
20	15.516	2107	2113	2128	rVV	381791	623614	23.60%	2.371%
21	15.627	2128	2132	2141	rVB2	19533	32917	1.25%	0.125%
22	16.168	2220	2224	2228	rVB3	3671	5553	0.21%	0.021%
23	16.921	2348	2352	2358	rVB2	3601	6333	0.24%	0.024%
24	17.133	2382	2388	2398	rBV	868264	1217128	46.06%	4.627%
25	17.233	2398	2405	2420	rVB2	1557829	2275737	86.12%	8.652%
26	18.033	2537	2541	2549	rBV6	18866	42914	1.62%	0.163%
27	18.104	2551	2553	2558	rVB3	3465	4912	0.19%	0.019%
28	19.162	2728	2733	2736	rBV	15264	22206	0.84%	0.084%
29	19.315	2756	2759	2762	rBV5	6883	11576	0.44%	0.044%
30	19.415	2773	2776	2779	rVB	11054	11771	0.45%	0.045%
31	19.521	2788	2794	2806	rBV	1922091	2642649	100.00%	10.047%
32	19.762	2832	2835	2840	rVB	12003	13718	0.52%	0.052%
33	21.039	3049	3052	3055	rBV	25226	28702	1.09%	0.109%
34	21.092	3058	3061	3067	rBV	54721	79393	3.00%	0.302%
35	21.309	3093	3098	3108	rBV	980517	1287530	48.72%	4.895%
36	23.415	3449	3456	3471	rVB	1065753	2193904	83.02%	8.341%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030822.D
Acq On : 06 Jul 2021 15:31
Operator : CG/JU
Sample : PB137472BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK472

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Title : SVOA CALIBRATION

37	23.556	3474	3480	3494	rVB2	546504	1115531	42.21%	4.241%
----	--------	------	------	------	------	--------	---------	--------	--------


Sum of corrected areas: 26303511

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030822.D
Acq On : 06 Jul 2021 15:31
Operator : CG/JU
Sample : PB137472BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK472

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

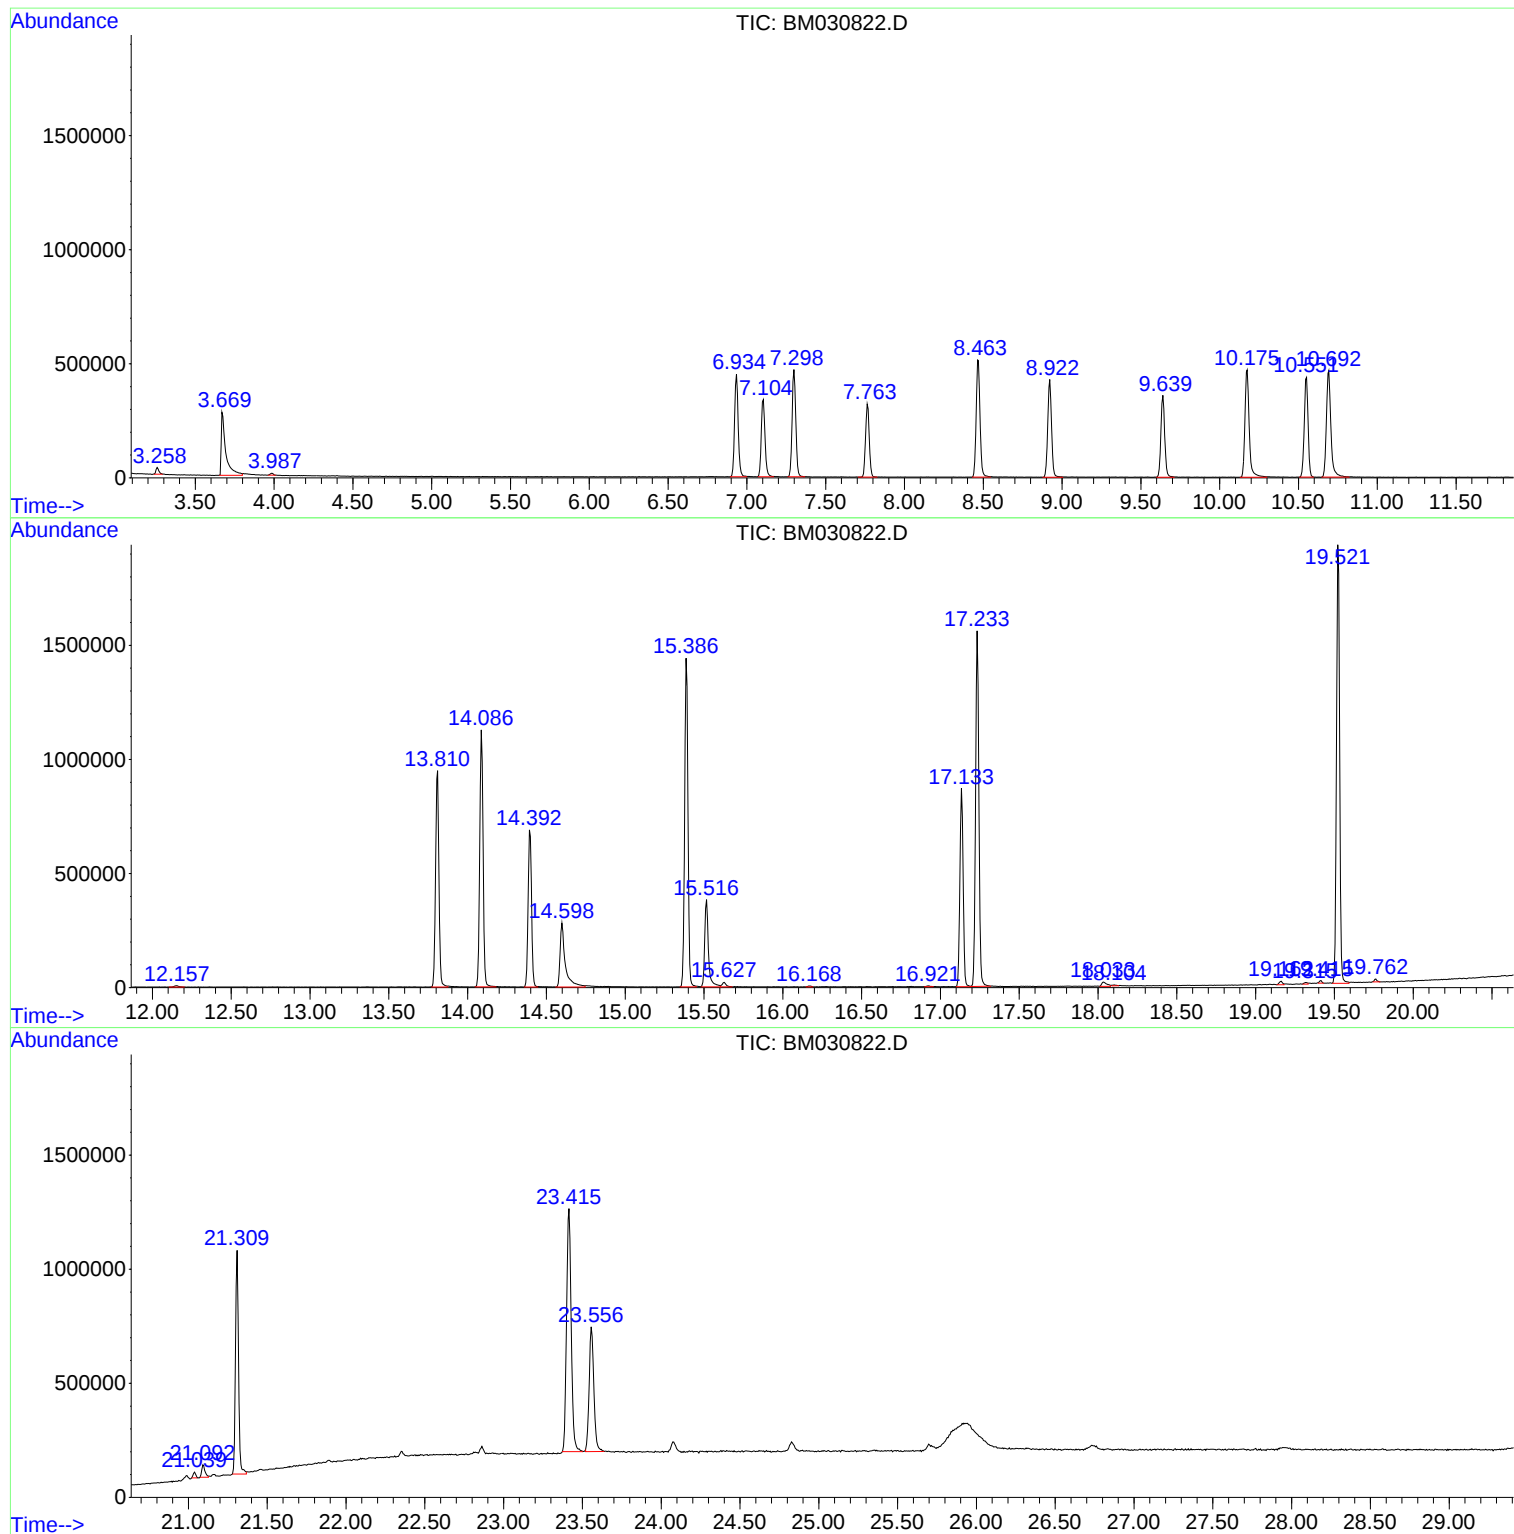

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030822.D
Acq On : 06 Jul 2021 15:31
Operator : CG/JU
Sample : PB137472BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK472

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030822.D
Acq On : 06 Jul 2021 15:31
Operator : CG/JU
Sample : PB137472BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK472

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
