

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030825.D
 Acq On : 06 Jul 2021 18:28
 Operator : CG/JU
 Sample : PB137437BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK437

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030825.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	26	29	36	rVB	30366	38157	1.70%	0.156%
2	3.669	96	99	122	rBV	286437	567933	25.31%	2.325%
3	3.987	149	153	158	rVB	9347	12956	0.58%	0.053%
4	6.934	647	654	667	rBV	461283	729978	32.53%	2.988%
5	7.105	676	683	697	rBV	348203	562797	25.08%	2.304%
6	7.299	709	716	728	rVB	477353	760660	33.90%	3.114%
7	7.763	787	795	803	rBV	326022	522240	23.27%	2.138%
8	8.469	907	915	933	rBV	520475	878109	39.13%	3.594%
9	8.922	985	992	1004	rBV	429611	723769	32.26%	2.963%
10	9.640	1106	1114	1127	rBV	361602	604528	26.94%	2.474%
11	10.175	1198	1205	1225	rBV	471659	878387	39.15%	3.595%
12	10.551	1261	1269	1276	rBV	435936	735989	32.80%	3.013%
13	10.687	1284	1292	1316	rBV	454829	921666	41.07%	3.773%
14	11.816	1478	1484	1486	rBV5	1556	2601	0.12%	0.011%
15	12.151	1536	1541	1546	rBV2	5807	11420	0.51%	0.047%
16	13.804	1816	1822	1834	rBV	884405	1323700	58.99%	5.418%
17	14.086	1862	1870	1885	rBV	1090525	1599889	71.30%	6.549%
18	14.392	1914	1922	1930	rBV	662784	992341	44.22%	4.062%
19	14.598	1951	1957	1992	rBV	239641	598936	26.69%	2.452%
20	15.386	2084	2091	2107	rBV	1350666	1982790	88.36%	8.116%
21	15.516	2107	2113	2128	rVV	340174	545902	24.33%	2.234%
22	15.627	2128	2132	2140	rVB	16466	28156	1.25%	0.115%
23	16.169	2220	2224	2229	rBV5	4607	5956	0.27%	0.024%
24	16.922	2347	2352	2359	rVB2	2993	5481	0.24%	0.022%
25	17.133	2382	2388	2398	rBV	776254	1116915	49.78%	4.572%
26	17.233	2398	2405	2420	rVB	1416554	2080724	92.73%	8.517%
27	17.810	2501	2503	2506	rBV4	1939	2598	0.12%	0.011%
28	18.033	2536	2541	2550	rBV4	19629	40431	1.80%	0.165%
29	18.568	2629	2632	2635	rBV4	1793	2383	0.11%	0.010%
30	19.157	2728	2732	2738	rBV	12329	18338	0.82%	0.075%
31	19.315	2756	2759	2763	rBV6	5928	8590	0.38%	0.035%
32	19.410	2771	2775	2781	rBV2	8851	13143	0.59%	0.054%
33	19.521	2788	2794	2803	rBV	1652587	2243896	100.00%	9.185%
34	21.092	3057	3061	3066	rBV	37156	59855	2.67%	0.245%
35	21.304	3092	3097	3106	rBV	800151	1025379	45.70%	4.197%
36	23.409	3448	3455	3468	rVB	938985	1869079	83.30%	7.651%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030825.D
Acq On : 06 Jul 2021 18:28
Operator : CG/JU
Sample : PB137437BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK437

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Title : SVOA CALIBRATION

37	23.551	3473	3479	3490	rVB	458938	914992	40.78%	3.745%
----	--------	------	------	------	-----	--------	--------	--------	--------




Sum of corrected areas: 24430664

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030825.D
Acq On : 06 Jul 2021 18:28
Operator : CG/JU
Sample : PB137437BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK437

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

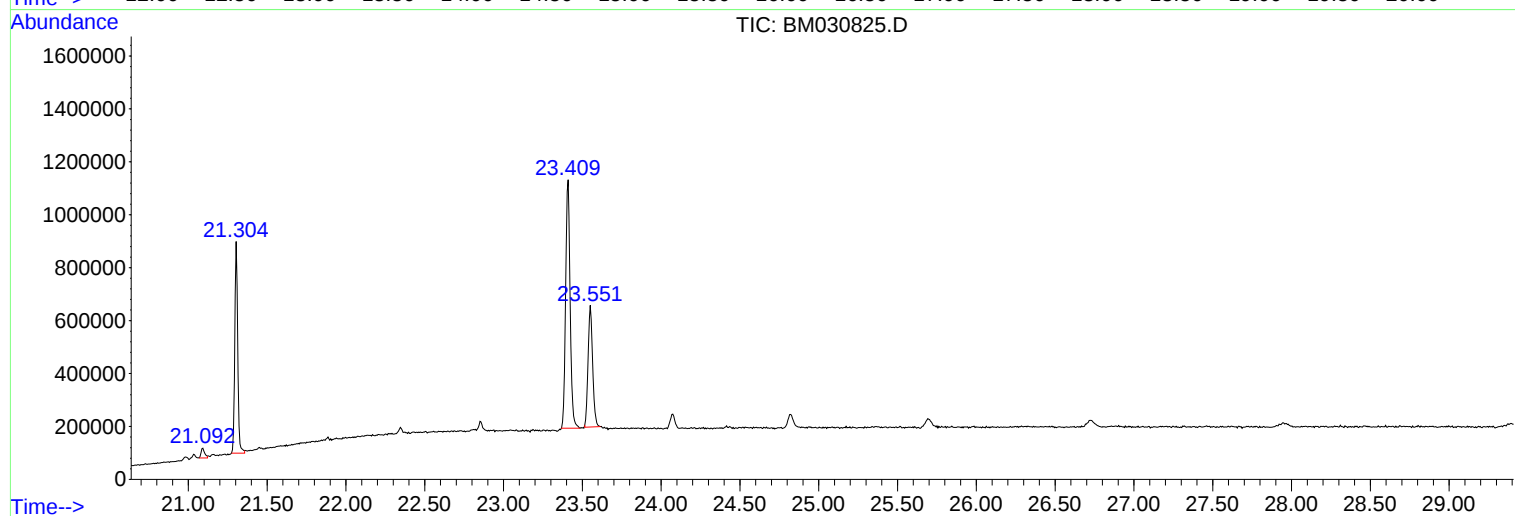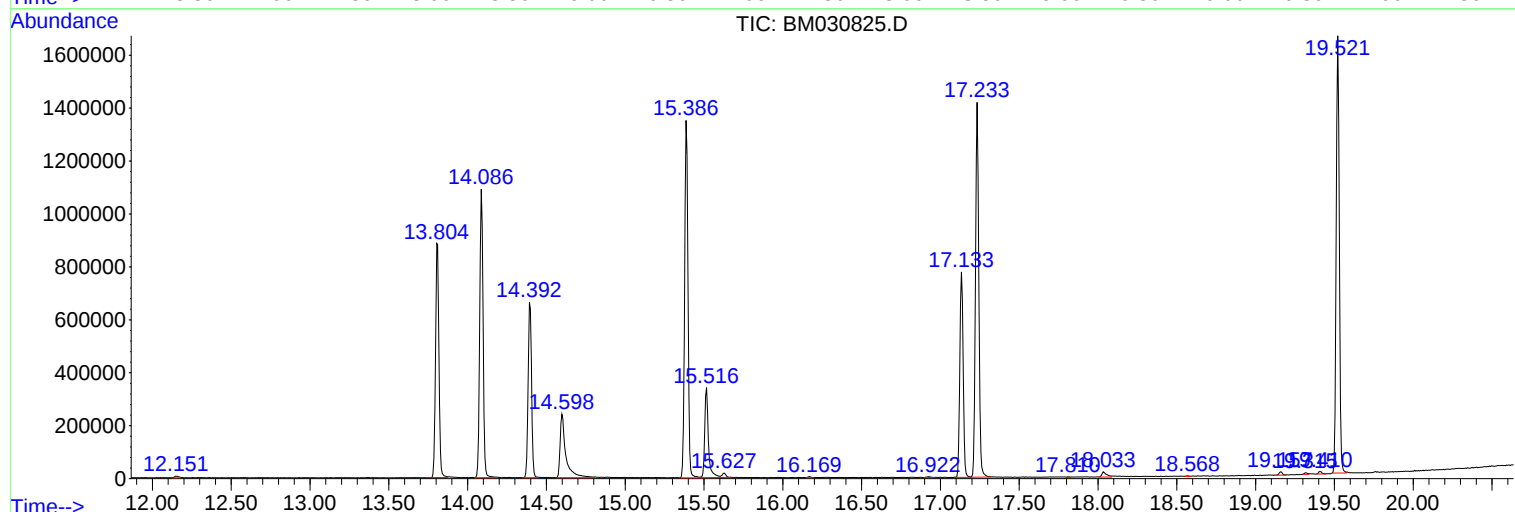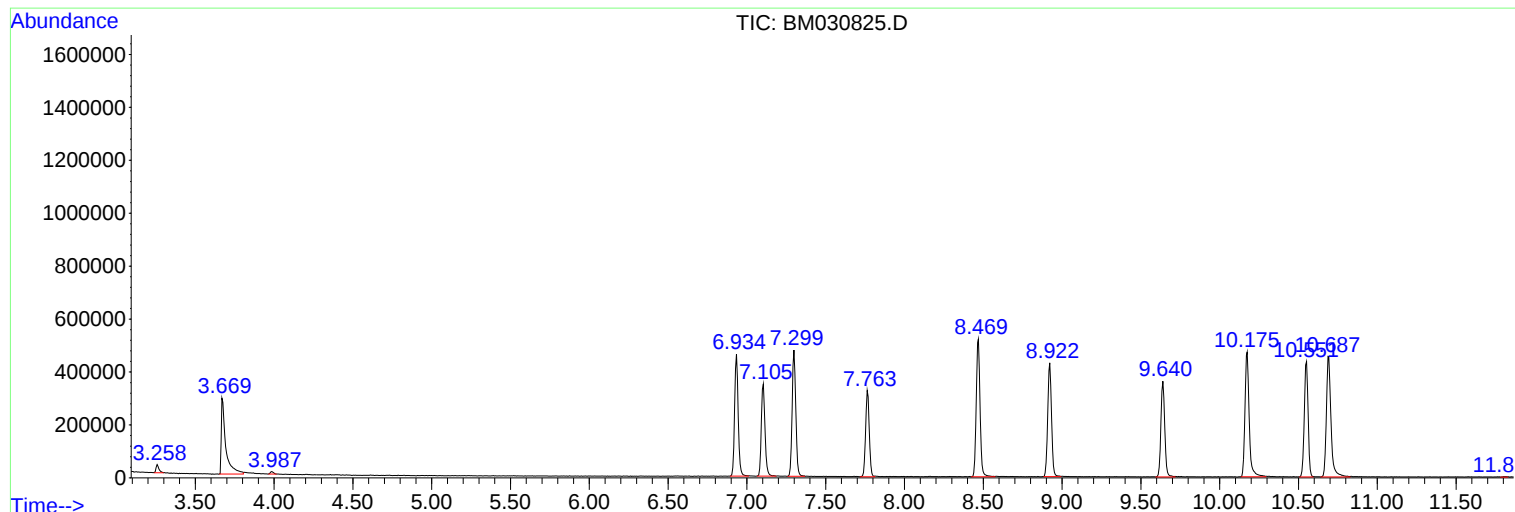

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030825.D
Acq On : 06 Jul 2021 18:28
Operator : CG/JU
Sample : PB137437BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK437

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030825.D
Acq On : 06 Jul 2021 18:28
Operator : CG/JU
Sample : PB137437BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK437

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
