

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030835.D
 Acq On : 07 Jul 2021 00:36
 Operator : CG/JU
 Sample : M2905-15DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK38DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030835.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.746	108	112	119	rBV4	5810	14642	0.98%	0.125%
2	3.987	149	153	158	rVB2	7590	11335	0.76%	0.097%
3	4.504	236	241	250	rVB	95545	142612	9.52%	1.214%
4	5.098	338	342	348	rVB2	8824	13066	0.87%	0.111%
5	6.940	649	655	664	rBV	15702	29230	1.95%	0.249%
6	7.104	678	683	696	rBV	68082	112908	7.54%	0.962%
7	7.298	710	716	725	rBV	69528	116694	7.79%	0.994%
8	7.763	788	795	805	rBV	415763	676187	45.16%	5.758%
9	8.116	850	855	864	rVB4	7535	14173	0.95%	0.121%
10	8.204	864	870	875	rVB6	2093	3662	0.24%	0.031%
11	8.469	909	915	926	rBV	47054	85790	5.73%	0.731%
12	8.922	986	992	1001	rBV	76039	134380	8.98%	1.144%
13	9.639	1105	1114	1126	rBV	57883	104806	7.00%	0.893%
14	10.180	1199	1206	1225	rBV	64960	147659	9.86%	1.257%
15	10.545	1261	1268	1277	rBV	546073	953179	63.66%	8.117%
16	10.698	1287	1294	1312	rBV2	61593	146075	9.76%	1.244%
17	11.192	1373	1378	1380	rBV3	1032	1596	0.11%	0.014%
18	11.510	1427	1432	1435	rBV5	1372	2263	0.15%	0.019%
19	11.810	1481	1483	1487	rVB5	1222	1778	0.12%	0.015%
20	12.157	1539	1542	1545	rVB4	1066	1562	0.10%	0.013%
21	13.810	1816	1823	1841	rBV	188620	297345	19.86%	2.532%
22	14.086	1864	1870	1878	rBV	212739	311324	20.79%	2.651%
23	14.392	1915	1922	1931	rBV	875556	1312557	87.66%	11.178%
24	14.663	1965	1968	1970	rBV3	1681	2171	0.14%	0.018%
25	14.874	2001	2004	2010	rVB3	1105	1834	0.12%	0.016%
26	14.951	2010	2017	2023	rBV7	6627	11528	0.77%	0.098%
27	15.033	2027	2031	2038	rVB6	5296	9401	0.63%	0.080%
28	15.386	2084	2091	2107	rBV	286164	432481	28.88%	3.683%
29	15.515	2107	2113	2129	rVV	41466	82656	5.52%	0.704%
30	15.627	2129	2132	2139	rVB7	3785	6296	0.42%	0.054%
31	16.204	2225	2230	2234	rBV6	1538	2252	0.15%	0.019%
32	16.786	2323	2329	2347	rBV	591874	891569	59.55%	7.593%
33	16.921	2350	2352	2358	rVB2	4643	6062	0.40%	0.052%
34	17.133	2381	2388	2399	rBV	1006986	1497261	100.00%	12.751%
35	17.233	2399	2405	2420	rVB	306247	501382	33.49%	4.270%
36	17.486	2447	2448	2452	rBV4	1312	1675	0.11%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030835.D
 Acq On : 07 Jul 2021 00:36
 Operator : CG/JU
 Sample : M2905-15DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK38DL

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

37	18.027	2536	2540	2549	rBV4	21260	42711	2.85%	0.364%
38	18.103	2551	2553	2555	rVV2	3777	3676	0.25%	0.031%
39	18.162	2559	2563	2566	rVV6	1293	1611	0.11%	0.014%
40	18.562	2629	2631	2634	rBV4	1687	1891	0.13%	0.016%
41	18.727	2655	2659	2661	rBV5	1603	2064	0.14%	0.018%
42	18.786	2667	2669	2672	rBV3	1745	1552	0.10%	0.013%
43	19.150	2729	2731	2734	rBV3	5606	7459	0.50%	0.064%
44	19.309	2754	2758	2764	rVB7	11109	20289	1.36%	0.173%
45	19.521	2788	2794	2801	rBV	414246	562419	37.56%	4.790%
46	21.303	3091	3097	3108	rBV	975881	1333858	89.09%	11.359%
47	23.403	3449	3454	3468	rVB	217196	460123	30.73%	3.918%
48	23.550	3472	3479	3490	rVV2	594921	1223455	81.71%	10.419%




Sum of corrected areas: 11742499

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030835.D
Acq On : 07 Jul 2021 00:36
Operator : CG/JU
Sample : M2905-15DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK38DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

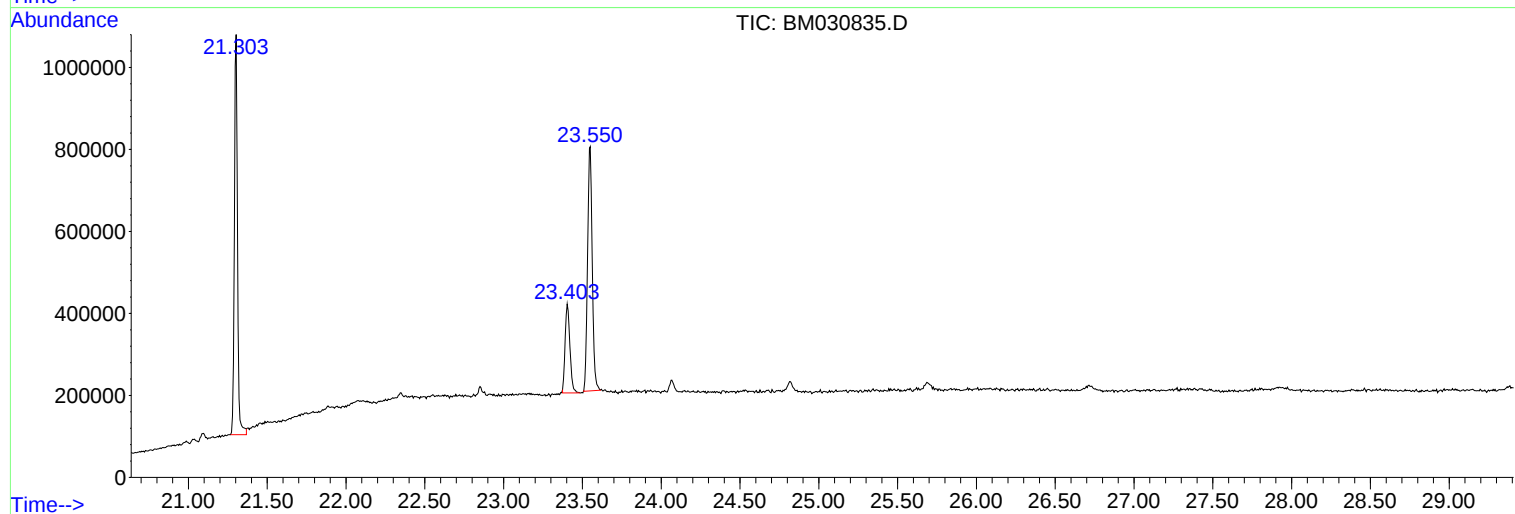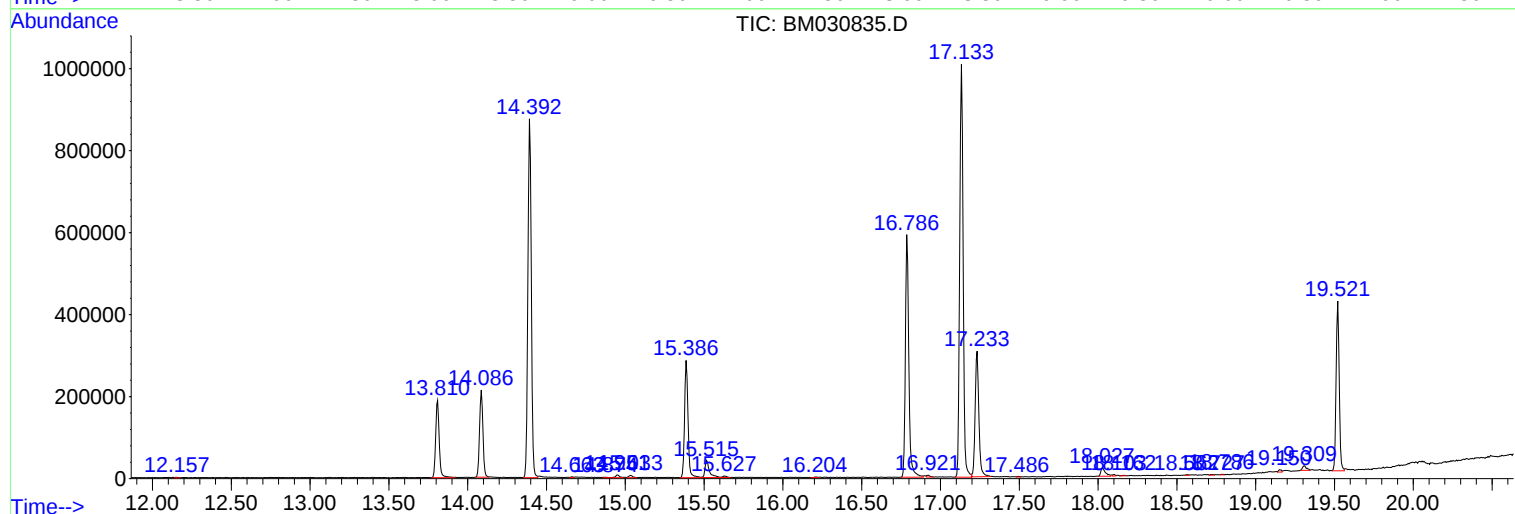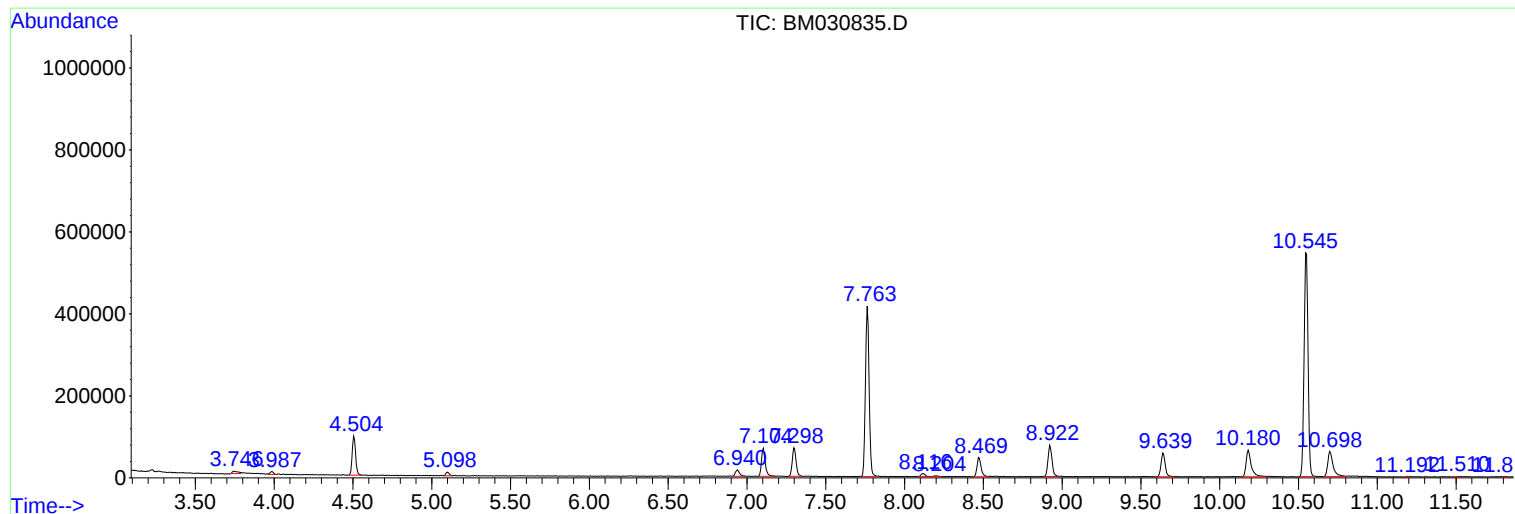

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030835.D
Acq On : 07 Jul 2021 00:36
Operator : CG/JU
Sample : M2905-15DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK38DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030835.D
Acq On : 07 Jul 2021 00:36
Operator : CG/JU
Sample : M2905-15DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK38DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
