

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030837.D
 Acq On : 07 Jul 2021 01:49
 Operator : CG/JU
 Sample : M2905-09DL 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK25DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030837.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	19	23	30	rVB3	22631	33957	2.97%	0.378%
2	3.822	122	125	128	rBV5	1526	2405	0.21%	0.027%
3	3.987	148	153	159	rVB	5984	10261	0.90%	0.114%
4	4.152	180	181	185	rBV3	1096	1622	0.14%	0.018%
5	4.246	194	197	202	rVB	5716	7162	0.63%	0.080%
6	4.505	236	241	247	rVB	51826	73725	6.44%	0.821%
7	4.852	297	300	304	rVB5	1892	2499	0.22%	0.028%
8	5.099	337	342	350	rBV	24759	38389	3.36%	0.428%
9	5.293	370	375	383	rVB3	3034	4595	0.40%	0.051%
10	5.787	455	459	463	rBV3	3957	4661	0.41%	0.052%
11	6.258	536	539	544	rVV2	5224	7030	0.61%	0.078%
12	6.752	618	623	627	rVB	7282	11216	0.98%	0.125%
13	6.857	635	641	646	rBV2	5537	8723	0.76%	0.097%
14	6.940	648	655	660	rVV4	6918	16904	1.48%	0.188%
15	6.987	660	663	668	rVB4	3371	5634	0.49%	0.063%
16	7.105	678	683	689	rBV	28882	48337	4.22%	0.538%
17	7.152	689	691	696	rVV3	5964	9185	0.80%	0.102%
18	7.205	696	700	706	rVB6	4370	6431	0.56%	0.072%
19	7.299	709	716	724	rBV	30062	51878	4.53%	0.578%
20	7.410	732	735	739	rVB2	6644	9917	0.87%	0.110%
21	7.652	774	776	780	rVB4	1214	1457	0.13%	0.016%
22	7.763	787	795	807	rBV	382878	627070	54.81%	6.986%
23	7.881	810	815	819	rVB3	3886	5843	0.51%	0.065%
24	7.999	827	835	842	rBV2	14928	24416	2.13%	0.272%
25	8.134	851	858	863	rBV3	13567	26971	2.36%	0.300%
26	8.193	863	868	876	rVV2	18197	31698	2.77%	0.353%
27	8.252	876	878	882	rVB3	2206	2991	0.26%	0.033%
28	8.375	893	899	901	rBV3	1054	1464	0.13%	0.016%
29	8.404	901	904	910	rVV6	2680	4582	0.40%	0.051%
30	8.475	910	916	925	rVV2	17875	34158	2.99%	0.381%
31	8.575	929	933	942	rVB6	3698	7986	0.70%	0.089%
32	8.757	961	964	966	rBV4	1532	1711	0.15%	0.019%
33	8.863	979	982	984	rBV3	2445	2961	0.26%	0.033%
34	8.922	987	992	1001	rVB	28975	53833	4.71%	0.600%
35	9.175	1027	1035	1040	rBV4	1692	4697	0.41%	0.052%
36	9.346	1059	1064	1071	rVB5	2344	4584	0.40%	0.051%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030837.D
 Acq On : 07 Jul 2021 01:49
 Operator : CG/JU
 Sample : M2905-09DL 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK25DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

37	9.440	1076	1080	1084	rBV4	1050	1675	0.15%	0.019%
38	9.493	1084	1089	1096	rVV3	2505	5061	0.44%	0.056%
39	9.581	1100	1104	1106	rBV5	1689	2500	0.22%	0.028%
40	9.640	1106	1114	1123	rVB3	21661	46638	4.08%	0.520%
41	9.798	1137	1141	1147	rVB3	6214	10099	0.88%	0.113%
42	9.857	1149	1151	1157	rVB5	1067	1527	0.13%	0.017%
43	9.963	1165	1169	1171	rBV5	1942	2299	0.20%	0.026%
44	9.993	1171	1174	1179	rVB4	1677	2687	0.23%	0.030%
45	10.057	1179	1185	1189	rBV2	9731	18898	1.65%	0.211%
46	10.087	1189	1190	1197	rVB4	3577	3573	0.31%	0.040%
47	10.181	1200	1206	1214	rBV	28889	54717	4.78%	0.610%
48	10.257	1214	1219	1227	rVB7	6368	13219	1.16%	0.147%
49	10.351	1230	1235	1248	rBV	21242	57504	5.03%	0.641%
50	10.440	1248	1250	1255	rVB4	2292	2518	0.22%	0.028%
51	10.545	1261	1268	1282	rVB	492803	852188	74.49%	9.493%
52	10.698	1285	1294	1301	rBV	25371	53154	4.65%	0.592%
53	10.816	1309	1314	1318	rBV6	2448	4616	0.40%	0.051%
54	10.928	1328	1333	1336	rVB6	2259	3603	0.31%	0.040%
55	11.034	1345	1351	1352	rBV4	1048	1572	0.14%	0.018%
56	11.422	1413	1417	1420	rBV5	1639	2429	0.21%	0.027%
57	11.469	1420	1425	1434	rVV6	4417	12496	1.09%	0.139%
58	11.598	1445	1447	1452	rVB6	1128	1471	0.13%	0.016%
59	11.792	1476	1480	1484	rBV5	1976	3208	0.28%	0.036%
60	11.963	1504	1509	1515	rVB5	4338	6646	0.58%	0.074%
61	12.092	1524	1531	1537	rBV8	2537	5934	0.52%	0.066%
62	12.140	1537	1539	1544	rVB4	1620	2343	0.20%	0.026%
63	12.381	1577	1580	1588	rVB5	2759	4486	0.39%	0.050%
64	12.569	1609	1612	1615	rVB4	1550	1994	0.17%	0.022%
65	12.834	1653	1657	1664	rBV6	4825	7776	0.68%	0.087%
66	12.916	1664	1671	1677	rBV3	13002	24295	2.12%	0.271%
67	13.116	1701	1705	1710	rVV3	6221	11000	0.96%	0.123%
68	13.216	1719	1722	1729	rVB7	2551	4611	0.40%	0.051%
69	13.339	1737	1743	1747	rVV6	2855	5719	0.50%	0.064%
70	13.434	1754	1759	1764	rBV6	3021	6615	0.58%	0.074%
71	13.810	1817	1823	1831	rVV	84877	130102	11.37%	1.449%
72	13.863	1831	1832	1836	rVV3	1560	1890	0.17%	0.021%
73	14.086	1864	1870	1880	rVB	83183	126038	11.02%	1.404%
74	14.392	1914	1922	1938	rBV	715911	1083499	94.70%	12.070%
75	14.710	1970	1976	1979	rVV5	1844	4246	0.37%	0.047%
76	14.922	2009	2012	2015	rBV2	3147	4785	0.42%	0.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030837.D
 Acq On : 07 Jul 2021 01:49
 Operator : CG/JU
 Sample : M2905-09DL 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK25DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

77	14.992	2020	2024	2026	rVV2	12529	18116	1.58%	0.202%
78	15.028	2026	2030	2042	rVB	30755	53463	4.67%	0.596%
79	15.192	2054	2058	2064	rBV6	1287	2393	0.21%	0.027%
80	15.386	2083	2091	2103	rBV	122226	186711	16.32%	2.080%
81	15.522	2108	2114	2128	rBV	112379	218898	19.13%	2.439%
82	16.204	2225	2230	2236	rBV	10861	16062	1.40%	0.179%
83	16.357	2251	2256	2262	rVB5	11207	15340	1.34%	0.171%
84	16.527	2282	2285	2288	rVB4	2010	2275	0.20%	0.025%
85	16.786	2323	2329	2342	rBV	453926	682038	59.61%	7.598%
86	16.886	2342	2346	2350	rVB6	6410	10267	0.90%	0.114%
87	17.133	2381	2388	2397	rBV	757875	1144099	100.00%	12.745%
88	17.233	2400	2405	2411	rVV	121833	200666	17.54%	2.235%
89	17.286	2411	2414	2422	rVB4	18297	27829	2.43%	0.310%
90	17.492	2446	2449	2454	rBV5	3987	5674	0.50%	0.063%
91	17.804	2498	2502	2507	rBV4	3907	6048	0.53%	0.067%
92	18.027	2535	2540	2547	rBV2	24650	43828	3.83%	0.488%
93	18.557	2628	2630	2634	rBV3	1416	2129	0.19%	0.024%
94	18.974	2695	2701	2706	rBV7	7268	11690	1.02%	0.130%
95	19.245	2745	2747	2749	rBV2	2004	1799	0.16%	0.020%
96	19.304	2753	2757	2766	rVV9	10961	23726	2.07%	0.264%
97	19.521	2789	2794	2803	rBV	150379	212950	18.61%	2.372%
98	21.304	3092	3097	3106	rBV	751023	1036297	90.58%	11.544%
99	23.403	3450	3454	3462	rVB2	97578	206931	18.09%	2.305%
100	23.545	3472	3478	3492	rVB2	527052	1066752	93.24%	11.884%


Sum of corrected areas: 8976565

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030837.D
Acq On : 07 Jul 2021 01:49
Operator : CG/JU
Sample : M2905-09DL 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
DBK25DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

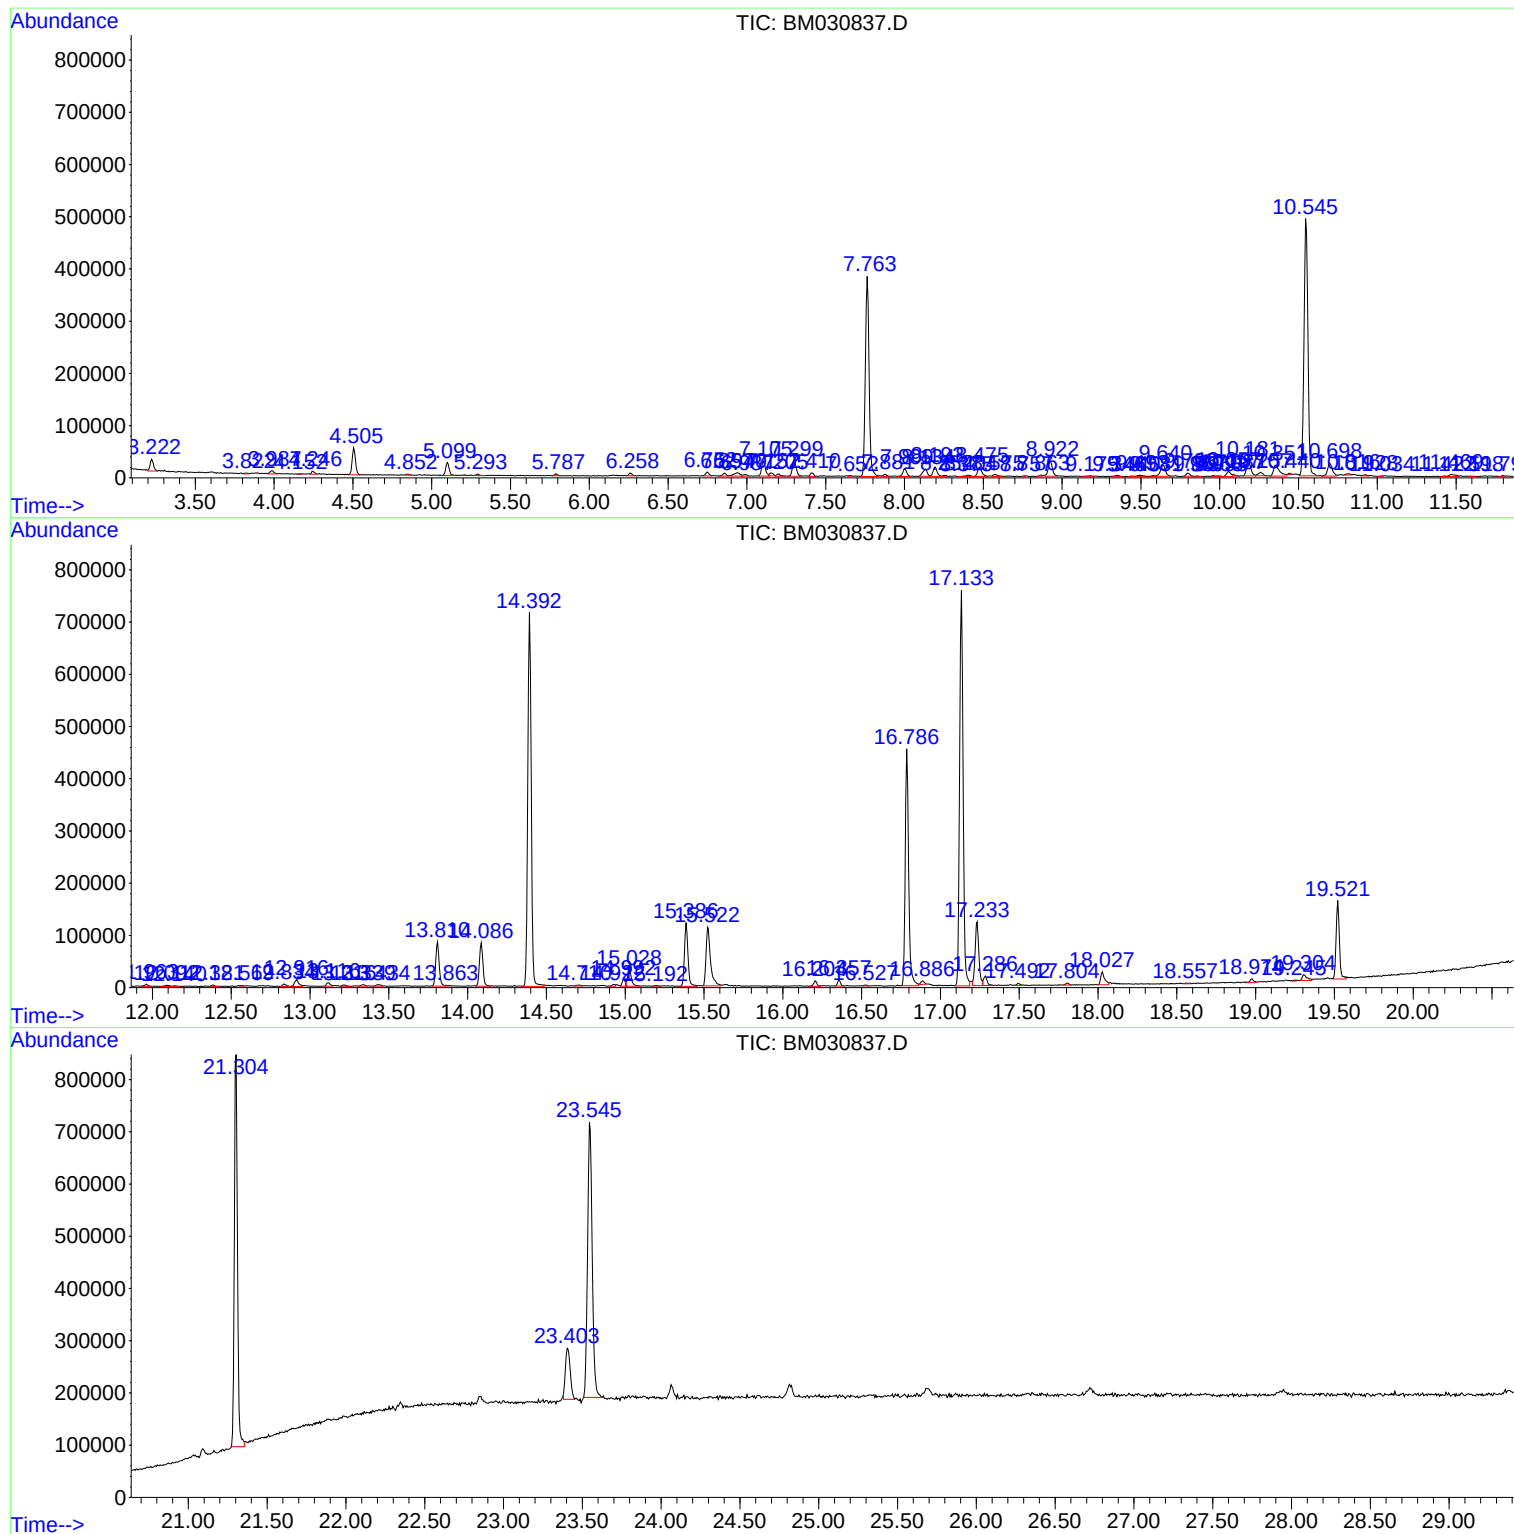

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030837.D
Acq On : 07 Jul 2021 01:49
Operator : CG/JU
Sample : M2905-09DL 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK25DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030837.D
Acq On : 07 Jul 2021 01:49
Operator : CG/JU
Sample : M2905-09DL 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK25DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc