

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030847.D
 Acq On : 07 Jul 2021 08:29
 Operator : CG/JU
 Sample : M2854-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030847.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	38	rVB2	10223	15917	1.22%	0.114%
2	3.716	104	107	115	rBV	14300	36176	2.77%	0.258%
3	3.987	149	153	159	rVB	7502	11031	0.84%	0.079%
4	4.346	211	214	215	rBV3	2126	2080	0.16%	0.015%
5	4.663	266	268	273	rVB5	1543	2334	0.18%	0.017%
6	5.416	390	396	401	rBV4	3188	5889	0.45%	0.042%
7	5.787	455	459	463	rBV6	2775	3981	0.30%	0.028%
8	6.757	619	624	632	rVB2	7579	12370	0.95%	0.088%
9	6.934	647	654	662	rBV	162768	277300	21.20%	1.980%
10	7.099	675	682	693	rBV	136089	227388	17.39%	1.623%
11	7.299	709	716	726	rVB	176659	296113	22.64%	2.114%
12	7.381	726	730	734	rBV3	3432	4681	0.36%	0.033%
13	7.604	764	768	772	rBV3	3708	4882	0.37%	0.035%
14	7.763	787	795	803	rVV	392061	641502	49.05%	4.580%
15	7.828	803	806	812	rVV3	3322	5820	0.45%	0.042%
16	7.887	812	816	821	rVB2	6331	10208	0.78%	0.073%
17	7.987	826	833	842	rBV2	24390	43896	3.36%	0.313%
18	8.169	861	864	868	rBV4	2090	2509	0.19%	0.018%
19	8.240	870	876	881	rBV4	5085	9431	0.72%	0.067%
20	8.293	881	885	889	rVV	15551	25772	1.97%	0.184%
21	8.328	889	891	897	rVB2	5347	7510	0.57%	0.054%
22	8.428	902	908	909	rBV	14616	18041	1.38%	0.129%
23	8.463	909	914	932	rVB	196835	337805	25.83%	2.412%
24	8.634	938	943	947	rBV2	6477	12153	0.93%	0.087%
25	8.663	947	948	955	rVB3	4856	5001	0.38%	0.036%
26	8.787	966	969	971	rBV3	1864	2557	0.20%	0.018%
27	8.804	971	972	978	rVB3	2074	1939	0.15%	0.014%
28	8.869	978	983	985	rBV4	1618	2471	0.19%	0.018%
29	8.922	985	992	1001	rBV	151641	269849	20.63%	1.926%
30	9.093	1016	1021	1024	rVB5	1728	2447	0.19%	0.017%
31	9.328	1055	1061	1065	rVB7	2214	3393	0.26%	0.024%
32	9.640	1107	1114	1123	rBV	119952	212310	16.23%	1.516%
33	10.175	1197	1205	1221	rBV	165936	329907	25.23%	2.355%
34	10.392	1236	1242	1243	rBV4	3277	4982	0.38%	0.036%
35	10.545	1260	1268	1277	rBV	518393	872352	66.71%	6.228%
36	10.692	1285	1293	1313	rBV	142834	309048	23.63%	2.206%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030847.D
 Acq On : 07 Jul 2021 08:29
 Operator : CG/JU
 Sample : M2854-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGD7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

37	11.804	1479	1482	1491	rVB5	733	1869	0.14%	0.013%
38	11.969	1507	1510	1515	rVB4	1169	1718	0.13%	0.012%
39	12.139	1535	1539	1546	rVB3	2446	4055	0.31%	0.029%
40	12.745	1637	1642	1647	rBV4	2166	3192	0.24%	0.023%
41	13.004	1680	1686	1689	rBV4	3171	5401	0.41%	0.039%
42	13.216	1719	1722	1728	rBV5	1875	3876	0.30%	0.028%
43	13.580	1779	1784	1786	rBV3	937	1733	0.13%	0.012%
44	13.804	1815	1822	1834	rBV	330841	500543	38.27%	3.573%
45	13.992	1850	1854	1856	rVB3	1100	1357	0.10%	0.010%
46	14.086	1860	1870	1885	rVV	371938	593155	45.36%	4.235%
47	14.180	1885	1886	1892	rVB6	1699	1476	0.11%	0.011%
48	14.292	1902	1905	1909	rVB4	1973	2809	0.21%	0.020%
49	14.392	1915	1922	1936	rBV	769830	1169875	89.46%	8.352%
50	14.616	1953	1960	1978	rBV2	38083	123905	9.47%	0.885%
51	14.833	1993	1997	2000	rVB5	2358	2550	0.19%	0.018%
52	15.192	2054	2058	2060	rBV3	1965	3049	0.23%	0.022%
53	15.245	2064	2067	2073	rVB4	2795	4292	0.33%	0.031%
54	15.386	2084	2091	2100	rBV	511123	775525	59.30%	5.536%
55	15.516	2107	2113	2126	rBV	60714	110979	8.49%	0.792%
56	15.627	2128	2132	2135	rVB4	4431	5039	0.39%	0.036%
57	15.804	2157	2162	2167	rVB3	4896	6604	0.50%	0.047%
58	16.057	2199	2205	2206	rBV5	2041	3301	0.25%	0.024%
59	16.169	2219	2224	2227	rVB4	5288	6737	0.52%	0.048%
60	16.227	2231	2234	2236	rBV3	1221	1399	0.11%	0.010%
61	16.274	2239	2242	2246	rVB5	1865	3149	0.24%	0.022%
62	16.369	2254	2258	2262	rBV3	4363	6397	0.49%	0.046%
63	16.527	2278	2285	2287	rBV4	6544	9950	0.76%	0.071%
64	16.592	2292	2296	2301	rVV6	3345	4520	0.35%	0.032%
65	16.663	2304	2308	2312	rVV7	2112	4302	0.33%	0.031%
66	16.698	2312	2314	2316	rVV3	2201	1980	0.15%	0.014%
67	16.733	2316	2320	2321	rVV4	1383	1635	0.13%	0.012%
68	16.757	2321	2324	2327	rVB3	1363	1628	0.12%	0.012%
69	16.845	2336	2339	2340	rBV2	1548	1766	0.14%	0.013%
70	16.869	2340	2343	2346	rVV3	4498	5936	0.45%	0.042%
71	16.892	2346	2347	2350	rVV2	3388	4018	0.31%	0.029%
72	16.921	2350	2352	2356	rVB3	1969	2536	0.19%	0.018%
73	17.127	2381	2387	2396	rBV	878130	1307769	100.00%	9.336%
74	17.227	2396	2404	2419	rVB	522132	813207	62.18%	5.805%
75	17.427	2433	2438	2443	rVB6	1712	3833	0.29%	0.027%
76	17.498	2447	2450	2452	rBV3	1323	1971	0.15%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030847.D
 Acq On : 07 Jul 2021 08:29
 Operator : CG/JU
 Sample : M2854-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGD7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

77	17.627	2471	2472	2476	rVB4	1548	1325	0.10%	0.009%
78	17.668	2476	2479	2483	rVV5	1686	2705	0.21%	0.019%
79	17.804	2498	2502	2506	rVB3	4776	5698	0.44%	0.041%
80	17.904	2515	2519	2521	rBV3	3423	3638	0.28%	0.026%
81	18.021	2534	2539	2547	rBV	34155	60415	4.62%	0.431%
82	18.098	2550	2552	2557	rVV2	6630	8728	0.67%	0.062%
83	18.133	2557	2558	2560	rVV2	2514	1921	0.15%	0.014%
84	18.157	2560	2562	2564	rVB2	1659	1345	0.10%	0.010%
85	18.321	2586	2590	2592	rBV4	1795	2044	0.16%	0.015%
86	18.368	2596	2598	2603	rBV4	1964	2586	0.20%	0.018%
87	18.468	2612	2615	2620	rBV2	6230	10674	0.82%	0.076%
88	18.580	2629	2634	2640	rBV7	11650	18275	1.40%	0.130%
89	18.951	2694	2697	2702	rBV5	4764	8215	0.63%	0.059%
90	19.010	2705	2707	2708	rBV2	2326	1638	0.13%	0.012%
91	19.157	2729	2732	2734	rBV2	6197	8342	0.64%	0.060%
92	19.186	2734	2737	2744	rVB2	9188	16547	1.27%	0.118%
93	19.304	2753	2757	2763	rBV6	13748	24126	1.84%	0.172%
94	19.515	2788	2793	2804	rBV	565711	819442	62.66%	5.850%
95	20.509	2958	2962	2967	rBV	407473	474211	36.26%	3.385%
96	21.009	3044	3047	3053	rBV4	39792	61398	4.69%	0.438%
97	21.304	3091	3097	3103	rBV	815412	1108856	84.79%	7.916%
98	22.474	3292	3296	3302	rVB	96015	128245	9.81%	0.916%
99	23.403	3448	3454	3468	rVB	287560	637531	48.75%	4.551%
100	23.545	3472	3478	3490	rVB2	537883	1059636	81.03%	7.565%




Sum of corrected areas: 14007622

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030847.D
Acq On : 07 Jul 2021 08:29
Operator : CG/JU
Sample : M2854-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDT7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

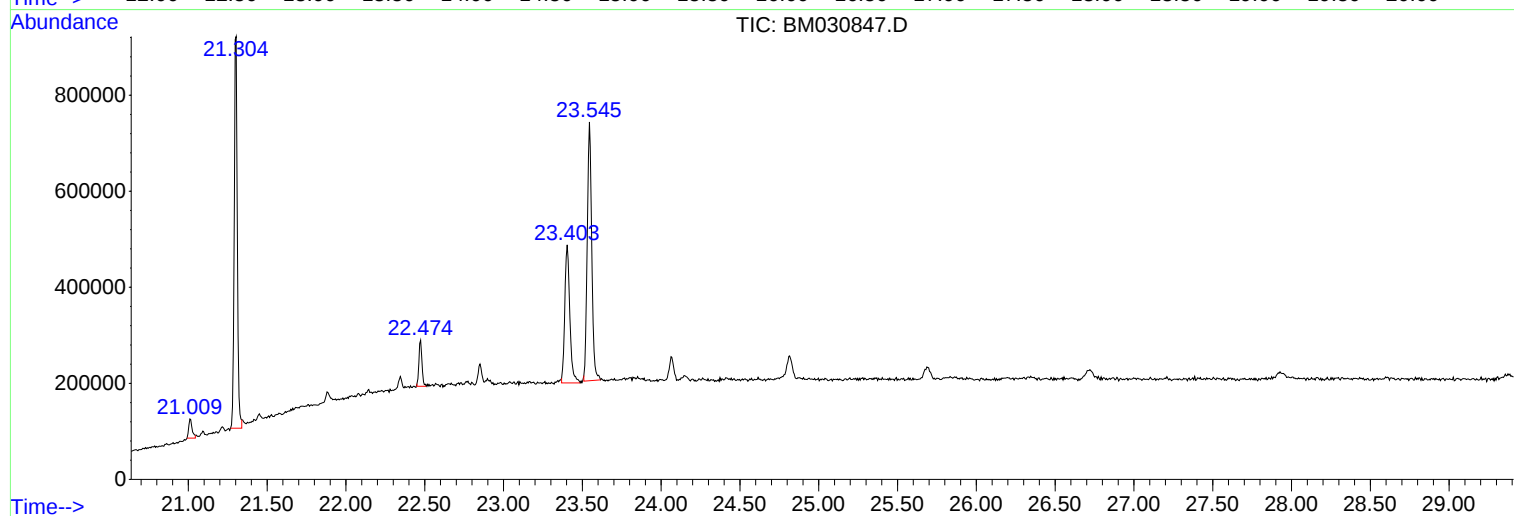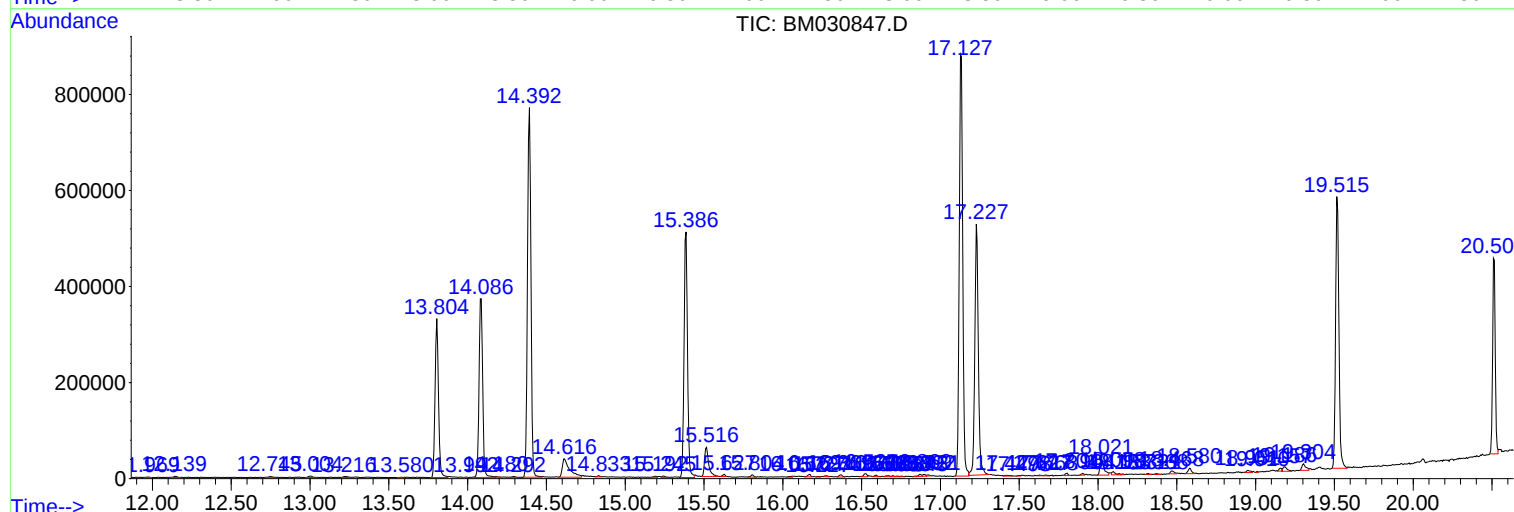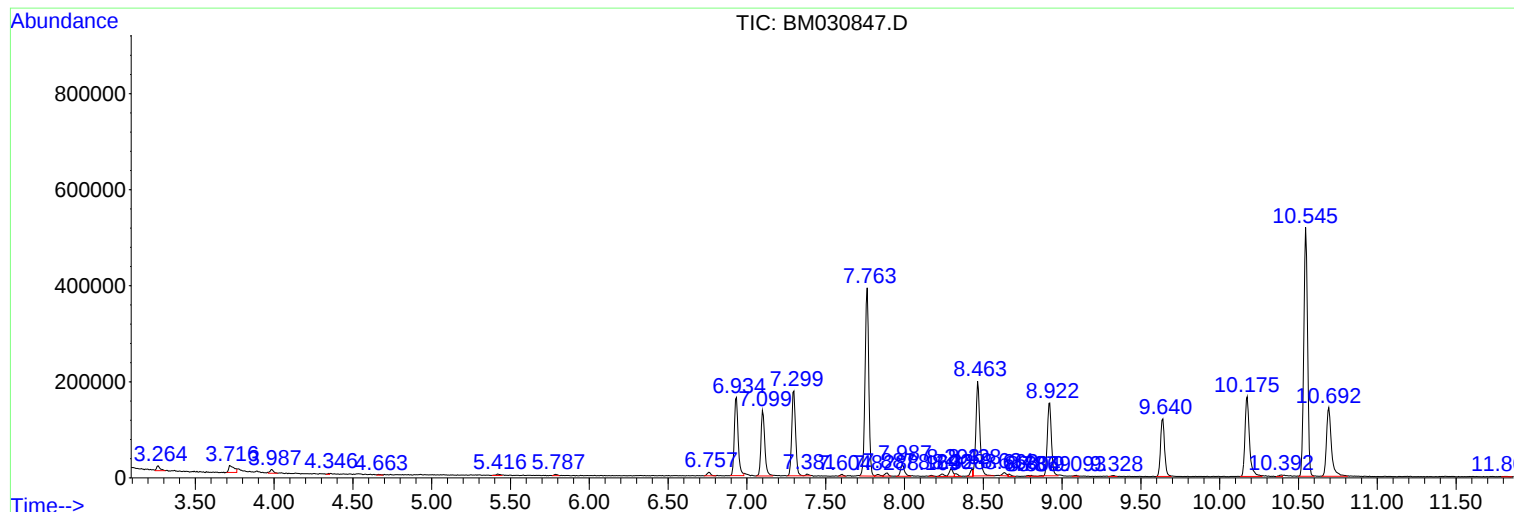

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030847.D
Acq On : 07 Jul 2021 08:29
Operator : CG/JU
Sample : M2854-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDT7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030847.D
Acq On : 07 Jul 2021 08:29
Operator : CG/JU
Sample : M2854-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDT7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
