

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030850.D
 Acq On : 07 Jul 2021 10:19
 Operator : CG/JU
 Sample : M2854-18
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDW2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030850.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	27	29	37	rVB3	6114	10045	0.76%	0.086%
2	3.734	106	110	112	rBV	9067	13070	0.99%	0.111%
3	3.887	134	136	142	rVB5	3234	5318	0.40%	0.045%
4	3.981	149	152	158	rVB	7321	10990	0.83%	0.094%
5	4.304	205	207	211	rBV5	1426	2005	0.15%	0.017%
6	4.346	211	214	216	rVV3	1796	2084	0.16%	0.018%
7	4.369	216	218	222	rVB4	1188	1336	0.10%	0.011%
8	4.540	244	247	250	rVB4	1778	2184	0.17%	0.019%
9	5.410	393	395	396	rBV	2170	1422	0.11%	0.012%
10	5.793	456	460	463	rVB3	2572	3355	0.25%	0.029%
11	6.757	620	624	631	rVB	4760	7786	0.59%	0.066%
12	6.934	648	654	668	rBV	111820	195297	14.84%	1.665%
13	7.098	676	682	693	rBV	87468	148222	11.26%	1.264%
14	7.298	709	716	725	rBV	119423	199647	15.17%	1.702%
15	7.387	727	731	736	rVB6	3227	5038	0.38%	0.043%
16	7.604	763	768	773	rBV2	2097	3428	0.26%	0.029%
17	7.763	786	795	804	rBV	362423	596461	45.32%	5.085%
18	7.828	804	806	810	rVB5	1947	2207	0.17%	0.019%
19	7.887	811	816	820	rVB4	2885	4911	0.37%	0.042%
20	7.987	828	833	839	rBV	11885	19565	1.49%	0.167%
21	8.175	862	865	868	rVB3	1223	1561	0.12%	0.013%
22	8.245	871	877	881	rVV7	2198	3939	0.30%	0.034%
23	8.298	881	886	889	rVV2	7060	11743	0.89%	0.100%
24	8.328	889	891	895	rVB4	2484	3146	0.24%	0.027%
25	8.428	902	908	909	rBV2	6914	8371	0.64%	0.071%
26	8.469	909	915	925	rVB	127591	226404	17.20%	1.930%
27	8.592	934	936	939	rBV3	1522	1428	0.11%	0.012%
28	8.628	939	942	946	rVV6	2406	3496	0.27%	0.030%
29	8.781	964	968	971	rBV5	921	1539	0.12%	0.013%
30	8.922	985	992	1002	rVV	100436	181956	13.82%	1.551%
31	8.986	1002	1003	1008	rVB2	1797	1751	0.13%	0.015%
32	9.092	1015	1021	1024	rBV5	1829	3213	0.24%	0.027%
33	9.328	1056	1061	1066	rVB5	1842	3437	0.26%	0.029%
34	9.639	1107	1114	1124	rVB	77258	135819	10.32%	1.158%
35	10.175	1199	1205	1220	rBV	106462	220096	16.72%	1.876%
36	10.380	1236	1240	1243	rBV5	5718	8805	0.67%	0.075%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030850.D
 Acq On : 07 Jul 2021 10:19
 Operator : CG/JU
 Sample : M2854-18
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDW2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

37	10.545	1261	1268	1279	rBV	497219	835193	63.45%	7.120%
38	10.692	1286	1293	1307	rBV	104465	228171	17.33%	1.945%
39	10.998	1343	1345	1348	rVB3	1246	1411	0.11%	0.012%
40	12.145	1537	1540	1545	rVB3	1777	2771	0.21%	0.024%

41	12.751	1639	1643	1646	rBV3	1592	2020	0.15%	0.017%
42	13.004	1682	1686	1690	rBV4	3521	5943	0.45%	0.051%
43	13.227	1718	1724	1727	rBV6	1904	3363	0.26%	0.029%
44	13.804	1816	1822	1833	rBV	257911	392365	29.81%	3.345%
45	14.086	1861	1870	1883	rBV	279690	429003	32.59%	3.657%

46	14.292	1902	1905	1910	rVB5	2625	3311	0.25%	0.028%
47	14.392	1915	1922	1940	rBV	755197	1139619	86.58%	9.715%
48	14.621	1955	1961	1988	rBV3	25582	91165	6.93%	0.777%
49	14.904	2008	2009	2016	rVB5	1225	1516	0.12%	0.013%
50	14.980	2018	2022	2025	rBV3	939	1586	0.12%	0.014%

51	15.198	2054	2059	2060	rBV3	1647	2646	0.20%	0.023%
52	15.239	2065	2066	2072	rVB4	2527	3125	0.24%	0.027%
53	15.386	2085	2091	2103	rBV	382849	577725	43.89%	4.925%
54	15.515	2108	2113	2124	rVV	43649	83421	6.34%	0.711%
55	15.627	2128	2132	2139	rVB5	3786	7062	0.54%	0.060%

56	15.810	2157	2163	2168	rVB7	4815	7416	0.56%	0.063%
57	15.857	2168	2171	2176	rBV4	1445	2390	0.18%	0.020%
58	16.045	2200	2203	2205	rBV4	1354	1481	0.11%	0.013%
59	16.162	2221	2223	2228	rVB4	3565	4575	0.35%	0.039%
60	16.274	2237	2242	2245	rVB4	2250	3622	0.28%	0.031%

61	16.368	2253	2258	2261	rVB4	4123	5543	0.42%	0.047%
62	16.521	2280	2284	2289	rVB4	4852	7237	0.55%	0.062%
63	16.592	2292	2296	2298	rBV4	2086	2302	0.17%	0.020%
64	16.792	2327	2330	2333	rBV4	1434	1424	0.11%	0.012%
65	16.827	2333	2336	2339	rBV5	996	1517	0.12%	0.013%

66	16.874	2339	2344	2345	rBV4	3002	3878	0.29%	0.033%
67	17.057	2370	2375	2379	rBV9	1787	3242	0.25%	0.028%
68	17.133	2381	2388	2396	rVV	902739	1316248	100.00%	11.221%
69	17.233	2398	2405	2416	rVV	404439	658772	50.05%	5.616%
70	17.339	2420	2423	2426	rVV4	4523	6063	0.46%	0.052%

71	17.380	2429	2430	2434	rVB3	1339	1620	0.12%	0.014%
72	17.633	2470	2473	2477	rVB5	1199	1895	0.14%	0.016%
73	17.668	2477	2479	2487	rBV7	2018	3268	0.25%	0.028%
74	17.798	2499	2501	2506	rVB4	3727	5088	0.39%	0.043%
75	17.904	2517	2519	2520	rBV2	1599	1367	0.10%	0.012%

76	18.021	2535	2539	2548	rBV2	30136	57543	4.37%	0.491%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030850.D
 Acq On : 07 Jul 2021 10:19
 Operator : CG/JU
 Sample : M2854-18
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDW2

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

77	18.315	2588	2589	2593	rVB4	1852	1341	0.10%	0.011%
78	18.768	2663	2666	2667	rBV3	2074	2326	0.18%	0.020%
79	18.951	2693	2697	2698	rBV4	2858	3859	0.29%	0.033%
80	19.156	2729	2732	2734	rBV3	6301	7418	0.56%	0.063%
81	19.186	2734	2737	2741	rVB2	9155	10265	0.78%	0.088%
82	19.303	2754	2757	2768	rVB7	14462	21051	1.60%	0.179%
83	19.521	2788	2794	2804	rBV	500966	701154	53.27%	5.977%
84	20.515	2959	2963	2966	rBV	95780	104462	7.94%	0.891%
85	21.009	3044	3047	3052	rBV3	41918	60689	4.61%	0.517%
86	21.303	3092	3097	3107	rBV	956142	1272105	96.65%	10.844%
87	23.403	3449	3454	3464	rVB2	222850	495136	37.62%	4.221%
88	23.550	3472	3479	3491	rVB2	537154	1091701	82.94%	9.307%


Sum of corrected areas: 11730489

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030850.D
Acq On : 07 Jul 2021 10:19
Operator : CG/JU
Sample : M2854-18
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDW2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

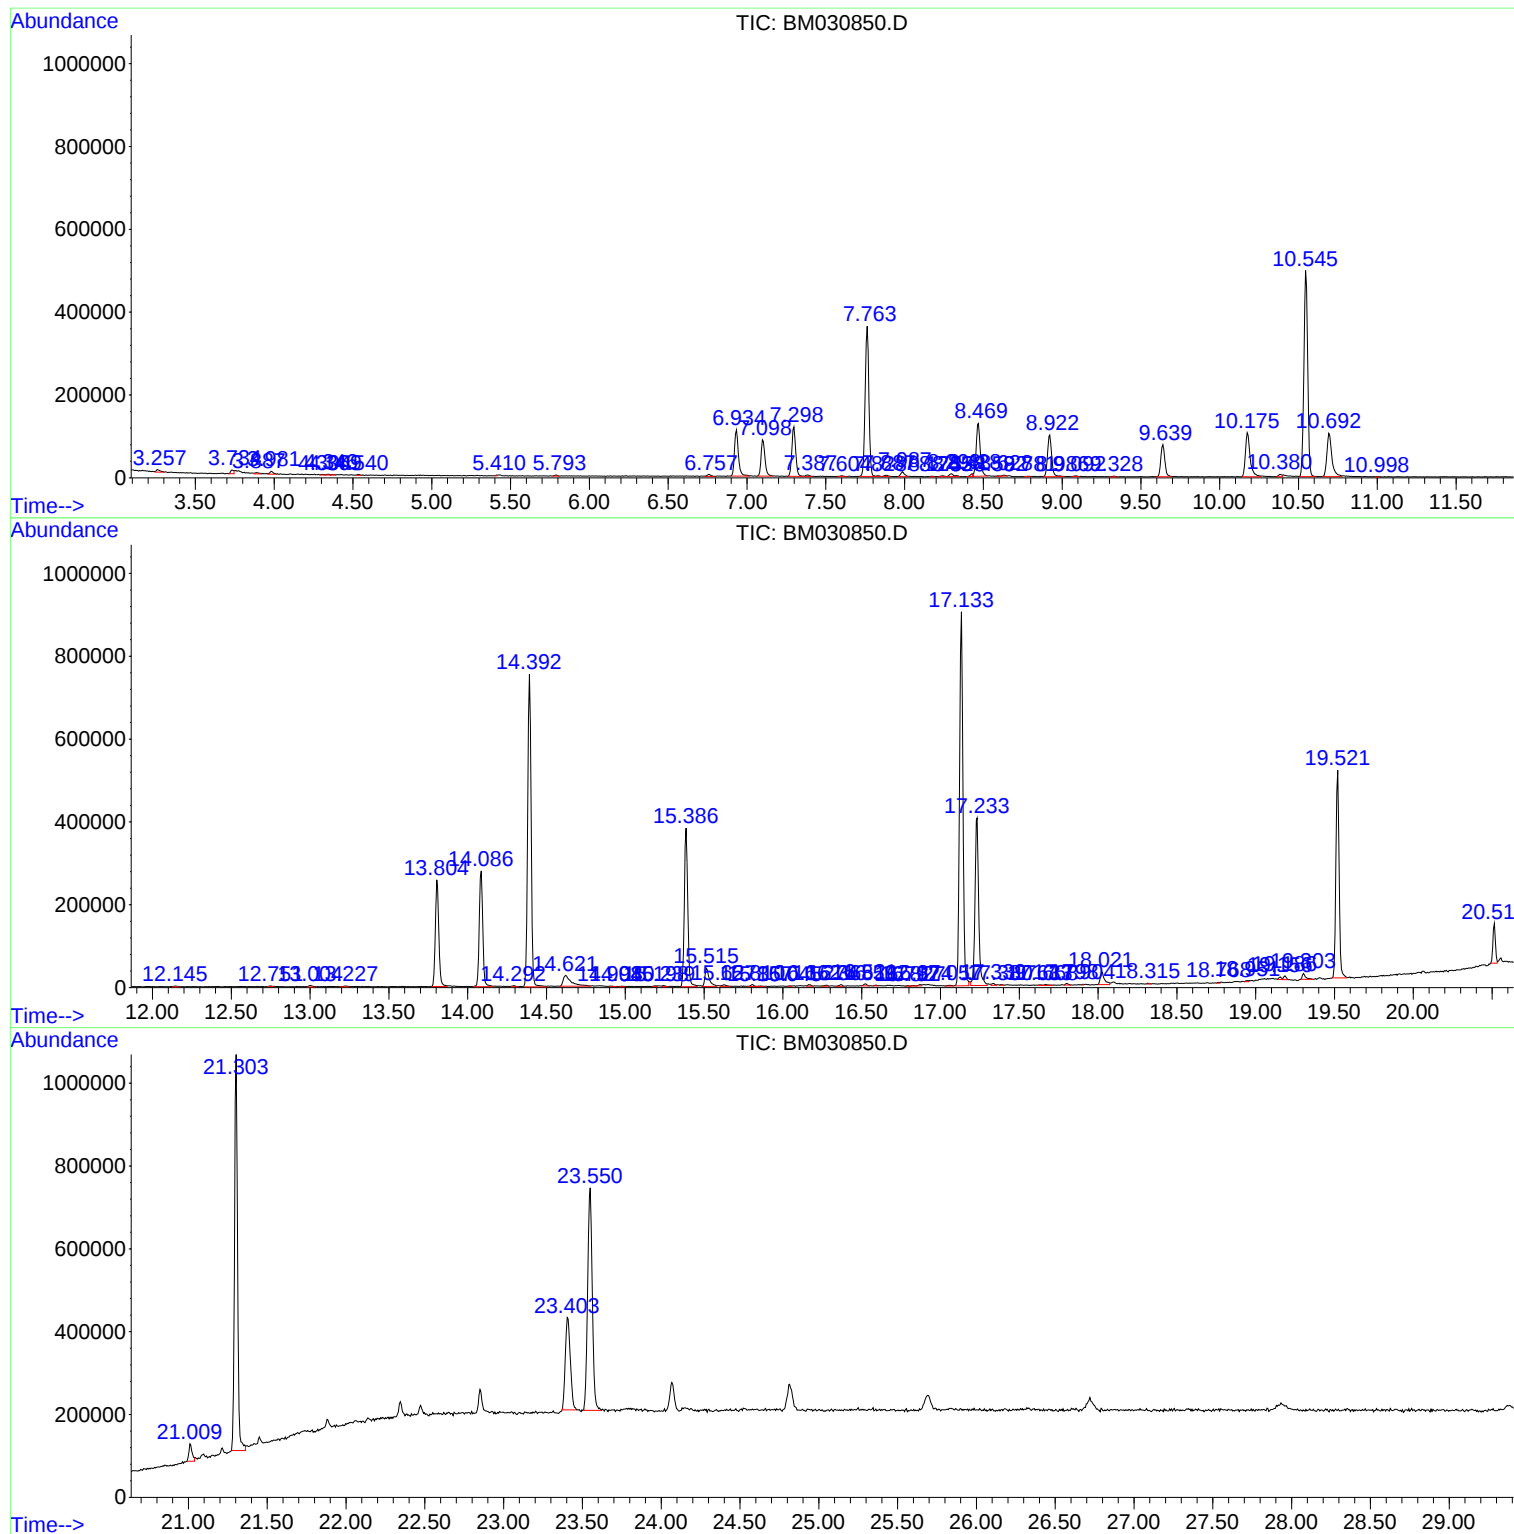

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030850.D
Acq On : 07 Jul 2021 10:19
Operator : CG/JU
Sample : M2854-18
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDW2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030850.D
Acq On : 07 Jul 2021 10:19
Operator : CG/JU
Sample : M2854-18
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDW2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------