

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030854.D
 Acq On : 07 Jul 2021 13:23
 Operator : CG/JU
 Sample : PB137514BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK514

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030854.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	25	29	42	rVB	34822	51379	2.39%	0.198%
2	3.669	96	99	127	rBV	333143	637602	29.69%	2.457%
3	3.981	150	152	162	rVB2	5915	9382	0.44%	0.036%
4	6.934	647	654	666	rBV	521436	850180	39.59%	3.276%
5	7.098	676	682	693	rBV	405161	650196	30.28%	2.505%
6	7.298	709	716	727	rBV	547705	882363	41.09%	3.400%
7	7.763	789	795	808	rVB	348555	552501	25.73%	2.129%
8	8.463	907	914	924	rBV	622525	1018538	47.44%	3.924%
9	8.916	984	991	1002	rBV	496374	835680	38.92%	3.220%
10	9.639	1107	1114	1126	rBV	401994	695194	32.38%	2.678%
11	10.169	1197	1204	1224	rBV	565826	1041098	48.49%	4.011%
12	10.545	1260	1268	1277	rBV	476681	804174	37.45%	3.098%
13	10.686	1285	1292	1309	rBV	540157	1050164	48.91%	4.046%
14	12.145	1536	1540	1545	rBV3	7924	13289	0.62%	0.051%
15	13.369	1742	1748	1753	rBV3	1683	2880	0.13%	0.011%
16	13.804	1816	1822	1833	rBV	1033709	1438861	67.01%	5.544%
17	14.086	1863	1870	1886	rBV	1198142	1785656	83.16%	6.880%
18	14.392	1915	1922	1929	rBV	694114	1037095	48.30%	3.996%
19	14.598	1950	1957	1983	rBV	237354	577073	26.88%	2.223%
20	15.386	2084	2091	2107	rBV	1503193	2147214	100.00%	8.273%
21	15.510	2107	2112	2127	rVV	309636	508398	23.68%	1.959%
22	15.621	2127	2131	2136	rVB	15321	24339	1.13%	0.094%
23	16.163	2217	2223	2227	rVB5	4040	5630	0.26%	0.022%
24	16.921	2349	2352	2359	rBV4	3324	5075	0.24%	0.020%
25	17.133	2381	2388	2397	rBV	735081	1083193	50.45%	4.173%
26	17.233	2398	2405	2426	rVB	1433248	2092621	97.46%	8.063%
27	18.027	2536	2540	2549	rBV4	15474	29175	1.36%	0.112%
28	19.156	2728	2732	2738	rBV	12763	18793	0.88%	0.072%
29	19.309	2754	2758	2763	rBV7	6747	11961	0.56%	0.046%
30	19.409	2771	2775	2778	rVB	9639	10794	0.50%	0.042%
31	19.521	2788	2794	2802	rBV	1529882	2116812	98.58%	8.156%
32	21.303	3092	3097	3106	rBV	718337	937426	43.66%	3.612%
33	23.403	3448	3454	3468	rVB	1032376	2070728	96.44%	7.978%
34	23.550	3473	3479	3488	rVB2	488690	959459	44.68%	3.697%

Sum of corrected areas: 25954923

Instrument :

BNA_M

ClientSampleId :


SBLK514

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030854.D
Acq On : 07 Jul 2021 13:23
Operator : CG/JU
Sample : PB137514BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK514

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

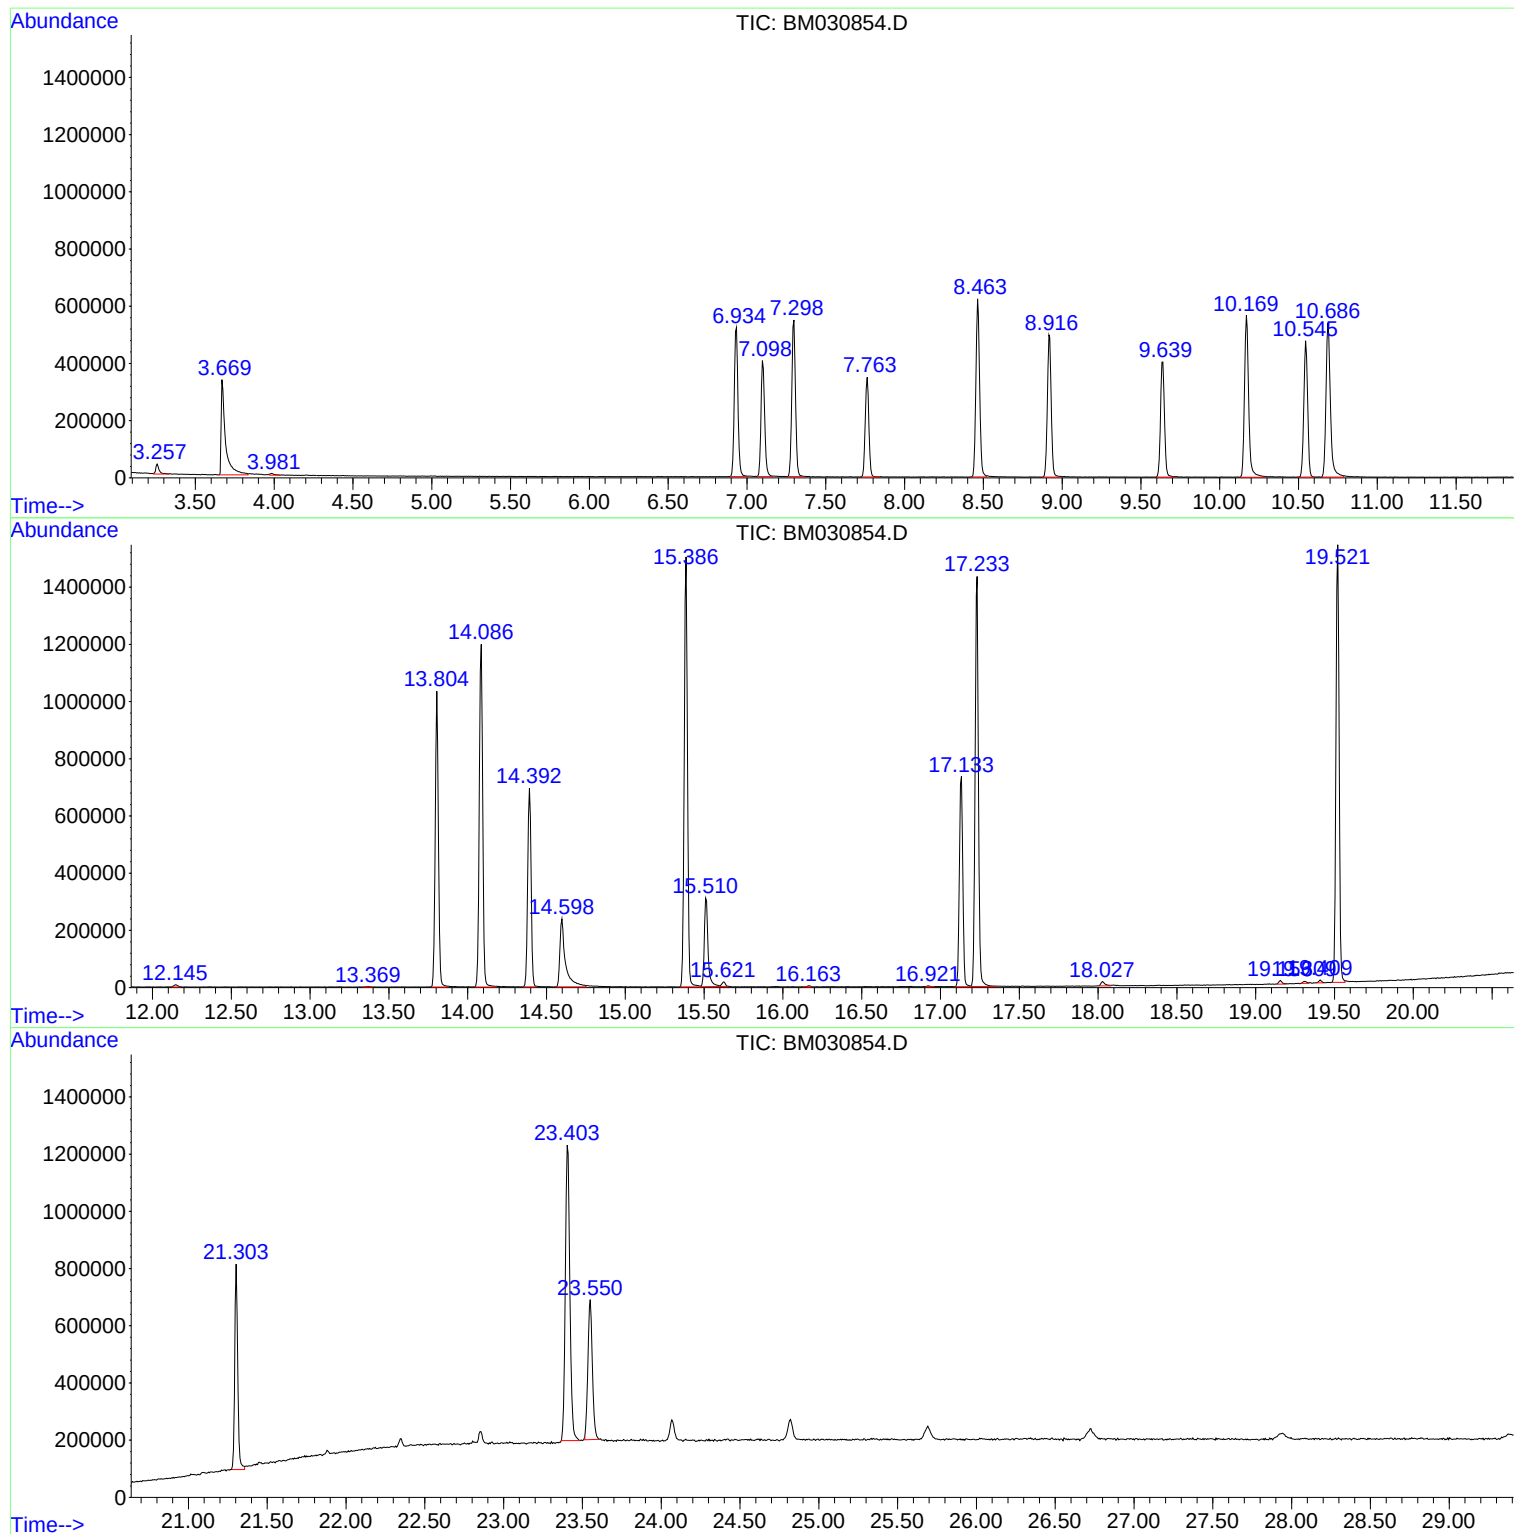

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030854.D
Acq On : 07 Jul 2021 13:23
Operator : CG/JU
Sample : PB137514BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK514

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030854.D
Acq On : 07 Jul 2021 13:23
Operator : CG/JU
Sample : PB137514BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK514

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
