

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030855.D
 Acq On : 07 Jul 2021 14:00
 Operator : CG/JU
 Sample : M2905-15DL 5X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK38DL

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030855.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	20	23	26	rVB4	5564	6261	0.66%	0.072%
2	3.416	53	56	62	rVB4	4098	5918	0.62%	0.068%
3	3.752	109	113	116	rBV2	4697	8830	0.93%	0.102%
4	3.981	149	152	160	rVB	6739	10639	1.12%	0.123%
5	4.181	184	186	189	rBV3	1223	1368	0.14%	0.016%
6	4.246	195	197	200	rVB4	1895	1735	0.18%	0.020%
7	4.328	208	211	216	rBV4	1834	2750	0.29%	0.032%
8	4.505	236	241	253	rVB	85902	129247	13.58%	1.489%
9	4.846	297	299	304	rBV3	827	1349	0.14%	0.016%
10	4.916	308	311	314	rBV4	1415	1953	0.21%	0.022%
11	4.975	317	321	322	rVB3	1261	1413	0.15%	0.016%
12	5.099	338	342	348	rBV2	8393	11013	1.16%	0.127%
13	5.287	373	374	376	rBV2	1136	1063	0.11%	0.012%
14	5.469	403	405	409	rBV5	834	1152	0.12%	0.013%
15	5.987	491	493	497	rVB5	816	1017	0.11%	0.012%
16	6.398	560	563	567	rBV5	629	1079	0.11%	0.012%
17	6.940	649	655	661	rVV	13764	24612	2.59%	0.284%
18	7.104	677	683	702	rBV2	65975	152247	15.99%	1.754%
19	7.298	709	716	725	rVV	61632	103547	10.88%	1.193%
20	7.387	729	731	737	rVB4	1250	1721	0.18%	0.020%
21	7.763	786	795	804	rBV	321500	515366	54.14%	5.937%
22	8.004	835	836	844	rVB6	1474	1638	0.17%	0.019%
23	8.116	849	855	861	rBV2	7768	13389	1.41%	0.154%
24	8.192	865	868	869	rBV2	2035	2209	0.23%	0.025%
25	8.469	910	915	924	rBV2	37876	70451	7.40%	0.812%
26	8.575	930	933	935	rBV3	1495	1325	0.14%	0.015%
27	8.592	935	936	944	rVB4	2244	3327	0.35%	0.038%
28	8.657	944	947	949	rBV2	980	1197	0.13%	0.014%
29	8.922	984	992	1001	rBV	68690	119955	12.60%	1.382%
30	9.087	1017	1020	1023	rVB3	1036	1155	0.12%	0.013%
31	9.122	1023	1026	1028	rBV2	953	1027	0.11%	0.012%
32	9.175	1031	1035	1036	rVV2	889	988	0.10%	0.011%
33	9.522	1093	1094	1098	rVB2	1405	1138	0.12%	0.013%
34	9.639	1107	1114	1126	rVB	47561	87516	9.19%	1.008%
35	9.828	1143	1146	1149	rBV4	1087	1424	0.15%	0.016%
36	9.934	1159	1164	1165	rBV4	1110	1218	0.13%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030855.D
 Acq On : 07 Jul 2021 14:00
 Operator : CG/JU
 Sample : M2905-15DL 5X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK38DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

37	9.945	1165	1166	1171	rVB3	1782	2116	0.22%	0.024%
38	10.086	1186	1190	1192	rBV3	818	1349	0.14%	0.016%
39	10.181	1199	1206	1220	rBV2	51241	119003	12.50%	1.371%
40	10.545	1261	1268	1277	rBV	424884	715993	75.21%	8.248%
41	10.698	1288	1294	1309	rBV2	50876	120504	12.66%	1.388%
42	10.792	1309	1310	1314	rVB4	1177	992	0.10%	0.011%
43	11.416	1412	1416	1421	rVB4	1373	2213	0.23%	0.025%
44	11.822	1482	1485	1487	rVB2	921	1062	0.11%	0.012%
45	11.922	1494	1502	1505	rBV5	1702	2410	0.25%	0.028%
46	11.963	1505	1509	1512	rBV5	953	1627	0.17%	0.019%
47	12.145	1538	1540	1547	rVB4	1340	2345	0.25%	0.027%
48	12.733	1635	1640	1644	rVB3	840	1458	0.15%	0.017%
49	13.292	1732	1735	1737	rBV	984	996	0.10%	0.011%
50	13.327	1740	1741	1745	rBV4	677	1049	0.11%	0.012%
51	13.539	1773	1777	1779	rBV3	867	1069	0.11%	0.012%
52	13.810	1817	1823	1832	rBV	149257	230416	24.20%	2.654%
53	14.027	1859	1860	1864	rVB4	893	993	0.10%	0.011%
54	14.086	1864	1870	1878	rBV	164889	250527	26.32%	2.886%
55	14.392	1915	1922	1934	rBV	608421	924023	97.07%	10.644%
56	14.469	1934	1935	1941	rVV4	2039	3418	0.36%	0.039%
57	14.527	1943	1945	1948	rVV4	1437	1422	0.15%	0.016%
58	14.674	1969	1970	1975	rVV4	1337	1746	0.18%	0.020%
59	14.827	1993	1996	2000	rVV2	696	1252	0.13%	0.014%
60	14.951	2010	2017	2022	rVV6	3094	5620	0.59%	0.065%
61	15.033	2027	2031	2037	rVB3	3837	5628	0.59%	0.065%
62	15.121	2042	2046	2049	rVB3	886	1157	0.12%	0.013%
63	15.227	2062	2064	2067	rBV3	1136	1296	0.14%	0.015%
64	15.269	2067	2071	2073	rVV4	707	1033	0.11%	0.012%
65	15.386	2084	2091	2107	rBV	218756	368270	38.69%	4.242%
66	15.521	2109	2114	2121	rVV	24949	49848	5.24%	0.574%
67	15.568	2121	2122	2127	rVV4	4388	4022	0.42%	0.046%
68	15.627	2130	2132	2133	rVV2	2139	2009	0.21%	0.023%
69	15.639	2133	2134	2137	rVB3	2472	1535	0.16%	0.018%
70	16.098	2210	2212	2215	rVV3	903	1284	0.13%	0.015%
71	16.133	2215	2218	2221	rVB4	889	1279	0.13%	0.015%
72	16.216	2227	2232	2235	rBV5	1334	1750	0.18%	0.020%
73	16.445	2268	2271	2275	rBV4	1312	1575	0.17%	0.018%
74	16.786	2324	2329	2345	rBV	408007	630925	66.28%	7.268%
75	16.892	2345	2347	2349	rVV2	2705	2863	0.30%	0.033%
76	16.915	2349	2351	2357	rVB4	2630	4908	0.52%	0.057%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030855.D
 Acq On : 07 Jul 2021 14:00
 Operator : CG/JU
 Sample : M2905-15DL 5X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK38DL

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

77	17.027	2368	2370	2371	rBV2	1811	1092	0.11%	0.013%
78	17.133	2381	2388	2399	rBV	616630	951945	100.00%	10.966%
79	17.233	2399	2405	2424	rVB	224310	366654	38.52%	4.224%
80	17.498	2446	2450	2452	rBV4	1846	2257	0.24%	0.026%
81	17.539	2454	2457	2460	rVB4	1072	1194	0.13%	0.014%
82	17.568	2460	2462	2465	rBV4	1238	1084	0.11%	0.012%
83	17.592	2465	2466	2469	rBV2	1500	1006	0.11%	0.012%
84	17.621	2469	2471	2474	rBV3	1291	1586	0.17%	0.018%
85	18.027	2533	2540	2547	rBV4	19837	37813	3.97%	0.436%
86	18.074	2547	2548	2550	rVV2	2285	1897	0.20%	0.022%
87	18.098	2550	2552	2554	rVB2	1941	1910	0.20%	0.022%
88	18.151	2560	2561	2565	rVB4	1424	1391	0.15%	0.016%
89	18.427	2606	2608	2611	rBV4	1288	1209	0.13%	0.014%
90	18.521	2621	2624	2626	rBV2	2012	2329	0.24%	0.027%
91	18.686	2651	2652	2655	rBV3	1365	1534	0.16%	0.018%
92	18.739	2659	2661	2664	rBV4	2324	2467	0.26%	0.028%
93	18.915	2689	2691	2693	rBV3	2088	1791	0.19%	0.021%
94	19.115	2723	2725	2726	rBV2	2074	1191	0.13%	0.014%
95	19.239	2744	2746	2748	rBV3	1966	1527	0.16%	0.018%
96	19.309	2754	2758	2763	rBV5	8773	14781	1.55%	0.170%
97	19.521	2788	2794	2803	rBV	282089	403518	42.39%	4.648%
98	21.303	3092	3097	3104	rBV	648068	852507	89.55%	9.820%
99	23.409	3450	3455	3466	rVB	187353	382803	40.21%	4.410%
100	23.550	3473	3479	3495	rVB2	437882	880475	92.49%	10.142%


Sum of corrected areas: 8681183

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030855.D
Acq On : 07 Jul 2021 14:00
Operator : CG/JU
Sample : M2905-15DL 5X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK38DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

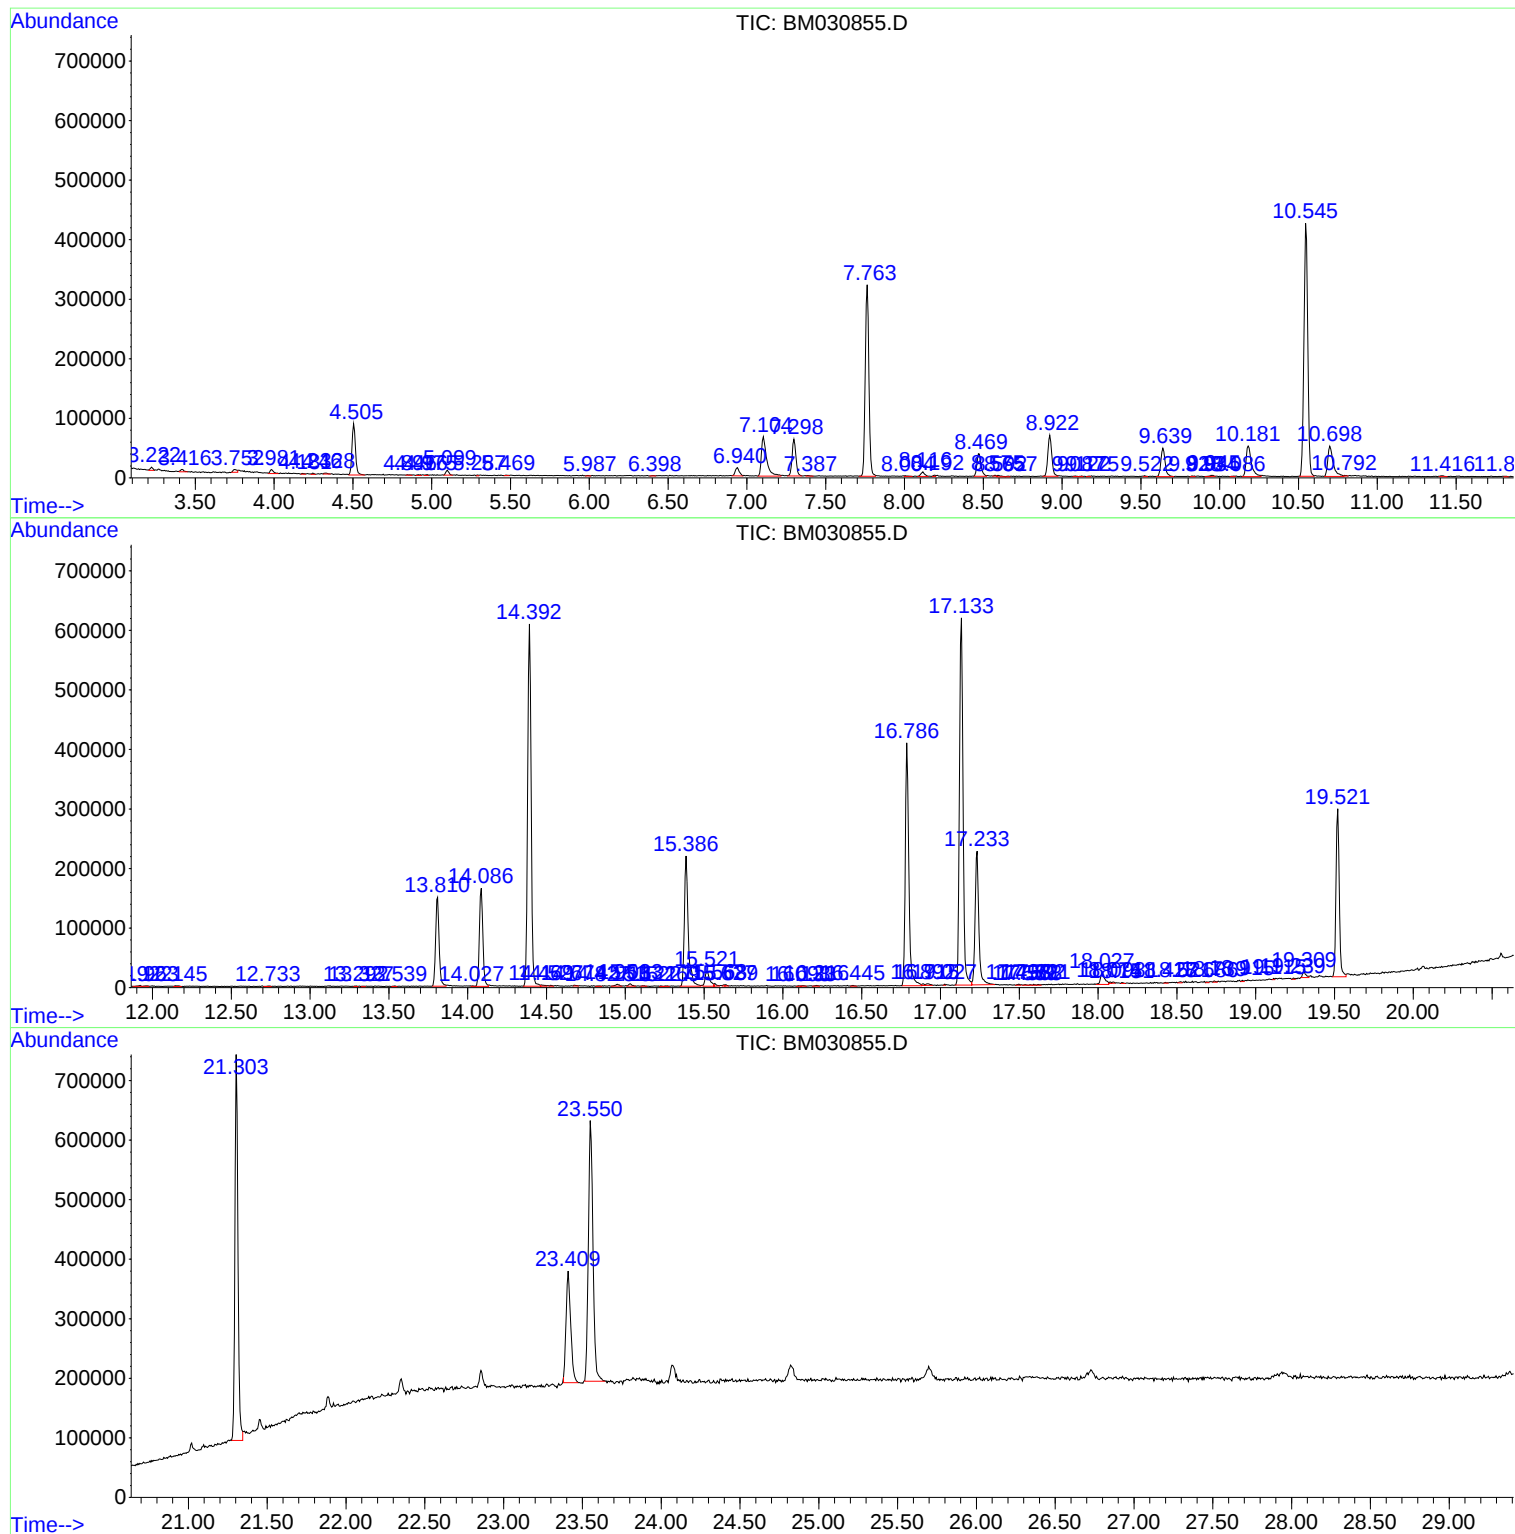

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030855.D
Acq On : 07 Jul 2021 14:00
Operator : CG/JU
Sample : M2905-15DL 5X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK38DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030855.D
Acq On : 07 Jul 2021 14:00
Operator : CG/JU
Sample : M2905-15DL 5X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK38DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
