

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030856.D
 Acq On : 07 Jul 2021 14:38
 Operator : CG/JU
 Sample : M2905-08DL 5X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK24DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030856.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	18	23	30	rVB	24917	38989	3.43%	0.422%
2	3.987	148	153	158	rVB2	7579	11227	0.99%	0.121%
3	4.246	194	197	201	rBV2	7199	8819	0.78%	0.095%
4	4.505	235	241	247	rBV	60981	87606	7.72%	0.948%
5	4.710	274	276	281	rVB3	1883	2353	0.21%	0.025%
6	4.846	296	299	305	rVB5	2226	4277	0.38%	0.046%
7	5.099	337	342	348	rBV	29075	42186	3.72%	0.457%
8	5.293	371	375	379	rBV2	3895	5523	0.49%	0.060%
9	5.787	453	459	463	rBV4	4840	7534	0.66%	0.082%
10	6.134	512	518	521	rBV5	2219	4015	0.35%	0.043%
11	6.263	534	540	546	rVB	6925	12206	1.08%	0.132%
12	6.746	616	622	627	rVB	9013	13567	1.20%	0.147%
13	6.851	637	640	646	rVB	6736	9782	0.86%	0.106%
14	6.934	646	654	659	rBV5	6321	18000	1.59%	0.195%
15	6.993	661	664	667	rVB3	4273	5725	0.50%	0.062%
16	7.104	678	683	688	rVV	27989	51368	4.53%	0.556%
17	7.157	688	692	695	rVV	12574	23079	2.03%	0.250%
18	7.193	695	698	706	rVV2	6191	11898	1.05%	0.129%
19	7.299	709	716	723	rBV2	27569	48299	4.26%	0.523%
20	7.410	730	735	742	rVB2	9882	15414	1.36%	0.167%
21	7.634	767	773	776	rBV7	2043	3334	0.29%	0.036%
22	7.763	788	795	810	rBV	370869	593501	52.29%	6.423%
23	7.875	810	814	819	rVV3	4942	8024	0.71%	0.087%
24	7.998	830	835	842	rBV2	20307	32646	2.88%	0.353%
25	8.128	849	857	863	rBV2	16683	35624	3.14%	0.386%
26	8.193	863	868	875	rVV	26428	43614	3.84%	0.472%
27	8.251	875	878	882	rVB6	2609	4053	0.36%	0.044%
28	8.310	886	888	893	rVV5	1636	2392	0.21%	0.026%
29	8.398	895	903	910	rVV7	3803	8040	0.71%	0.087%
30	8.475	910	916	925	rVV	16658	33784	2.98%	0.366%
31	8.569	927	932	942	rVV7	5206	11955	1.05%	0.129%
32	8.757	959	964	970	rBV7	1943	4497	0.40%	0.049%
33	8.869	976	983	984	rBV5	3767	6019	0.53%	0.065%
34	8.922	987	992	1002	rVV	29751	57707	5.08%	0.624%
35	9.351	1061	1065	1073	rVB5	3529	4482	0.39%	0.049%
36	9.445	1078	1081	1084	rBV4	1626	2333	0.21%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030856.D
 Acq On : 07 Jul 2021 14:38
 Operator : CG/JU
 Sample : M2905-08DL 5X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK24DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

37	9.492	1084	1089	1092	rVV2	3650	5314	0.47%	0.058%
38	9.575	1097	1103	1107	rVV5	1715	3081	0.27%	0.033%
39	9.640	1107	1114	1120	rVV6	20290	45094	3.97%	0.488%
40	9.722	1124	1128	1131	rVB3	2047	2948	0.26%	0.032%

41	9.792	1134	1140	1146	rBV4	8268	16013	1.41%	0.173%
42	9.851	1148	1150	1155	rVB3	1697	2258	0.20%	0.024%
43	9.957	1163	1168	1171	rBV4	2325	3187	0.28%	0.034%
44	10.057	1178	1185	1189	rBV2	10241	21241	1.87%	0.230%
45	10.181	1201	1206	1213	rBV	26737	50642	4.46%	0.548%

46	10.257	1213	1219	1229	rVB6	9136	22143	1.95%	0.240%
47	10.363	1232	1237	1245	rBV5	5850	14849	1.31%	0.161%
48	10.445	1247	1251	1254	rBV6	3687	5826	0.51%	0.063%
49	10.545	1261	1268	1283	rVB	487978	831515	73.26%	8.998%
50	10.698	1288	1294	1302	rBV2	22575	45807	4.04%	0.496%

51	10.763	1302	1305	1308	rBV5	1990	2241	0.20%	0.024%
52	10.816	1308	1314	1318	rBV7	3363	8771	0.77%	0.095%
53	10.916	1330	1331	1337	rVB5	2361	2790	0.25%	0.030%
54	11.028	1344	1350	1352	rBV3	2001	3653	0.32%	0.040%
55	11.463	1418	1424	1428	rVV5	7254	13450	1.18%	0.146%

56	11.498	1428	1430	1437	rVV5	3143	5444	0.48%	0.059%
57	11.957	1502	1508	1515	rVB7	6551	13094	1.15%	0.142%
58	12.086	1526	1530	1537	rVV5	3269	6347	0.56%	0.069%
59	12.222	1548	1553	1555	rBV4	1489	2380	0.21%	0.026%
60	12.381	1576	1580	1586	rVV4	4363	7282	0.64%	0.079%

61	12.539	1604	1607	1608	rBV3	2517	2913	0.26%	0.032%
62	12.675	1626	1630	1631	rBV2	2401	2614	0.23%	0.028%
63	12.692	1631	1633	1635	rVV2	2390	2522	0.22%	0.027%
64	12.833	1651	1657	1664	rBV4	6245	10629	0.94%	0.115%
65	12.910	1664	1670	1678	rBV2	17180	32645	2.88%	0.353%

66	13.110	1700	1704	1709	rBV5	10900	17827	1.57%	0.193%
67	13.204	1718	1720	1728	rVB6	2800	5229	0.46%	0.057%
68	13.339	1737	1743	1749	rBV5	4376	8049	0.71%	0.087%
69	13.422	1754	1757	1766	rVB5	5650	12821	1.13%	0.139%
70	13.804	1817	1822	1832	rBV	81491	125320	11.04%	1.356%

71	14.086	1863	1870	1877	rVV	77108	116755	10.29%	1.263%
72	14.392	1915	1922	1936	rBV	734272	1074201	94.64%	11.625%
73	14.710	1971	1976	1980	rVB4	2849	5351	0.47%	0.058%
74	14.922	2005	2012	2019	rBV8	5722	13746	1.21%	0.149%
75	14.992	2019	2024	2026	rVV3	15609	23516	2.07%	0.254%

76	15.027	2026	2030	2037	rVB	43482	65290	5.75%	0.707%
----	--------	------	------	------	-----	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030856.D
 Acq On : 07 Jul 2021 14:38
 Operator : CG/JU
 Sample : M2905-08DL 5X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK24DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

77	15.186	2054	2057	2062	rVV4	1363	2843	0.25%	0.031%
78	15.386	2083	2091	2104	rBV	115657	189182	16.67%	2.047%
79	15.522	2108	2114	2128	rVV	156911	288885	25.45%	3.126%
80	15.639	2131	2134	2139	rVB6	4722	7235	0.64%	0.078%
81	16.204	2225	2230	2236	rVB3	15215	21350	1.88%	0.231%
82	16.351	2252	2255	2263	rVB5	13724	20129	1.77%	0.218%
83	16.786	2323	2329	2342	rBV	612066	932227	82.13%	10.088%
84	16.880	2342	2345	2350	rVV5	11168	19622	1.73%	0.212%
85	16.921	2350	2352	2356	rVB2	2684	3425	0.30%	0.037%
86	17.133	2381	2388	2399	rVV	770703	1135067	100.00%	12.283%
87	17.233	2399	2405	2410	rVV	119404	190449	16.78%	2.061%
88	17.286	2410	2414	2420	rVB3	23462	37609	3.31%	0.407%
89	17.492	2444	2449	2452	rBV3	5840	8490	0.75%	0.092%
90	17.621	2469	2471	2475	rBV5	1865	2468	0.22%	0.027%
91	17.798	2498	2501	2505	rVB5	2840	4688	0.41%	0.051%
92	18.021	2533	2539	2549	rBV6	23577	49528	4.36%	0.536%
93	19.115	2721	2725	2726	rBV4	2553	2628	0.23%	0.028%
94	19.304	2754	2757	2763	rBV6	10933	18985	1.67%	0.205%
95	19.521	2789	2794	2803	rBV	142468	200023	17.62%	2.165%
96	20.556	2968	2970	2974	rVB4	11408	10969	0.97%	0.119%
97	21.021	3046	3049	3055	rVB4	19103	23863	2.10%	0.258%
98	21.303	3092	3097	3106	rBV	715704	977570	86.12%	10.579%
99	23.409	3451	3455	3466	rVB3	89947	193279	17.03%	2.092%
100	23.550	3473	3479	3492	rVB2	470955	971532	85.59%	10.514%


Sum of corrected areas: 9240716

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030856.D
Acq On : 07 Jul 2021 14:38
Operator : CG/JU
Sample : M2905-08DL 5X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK24DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

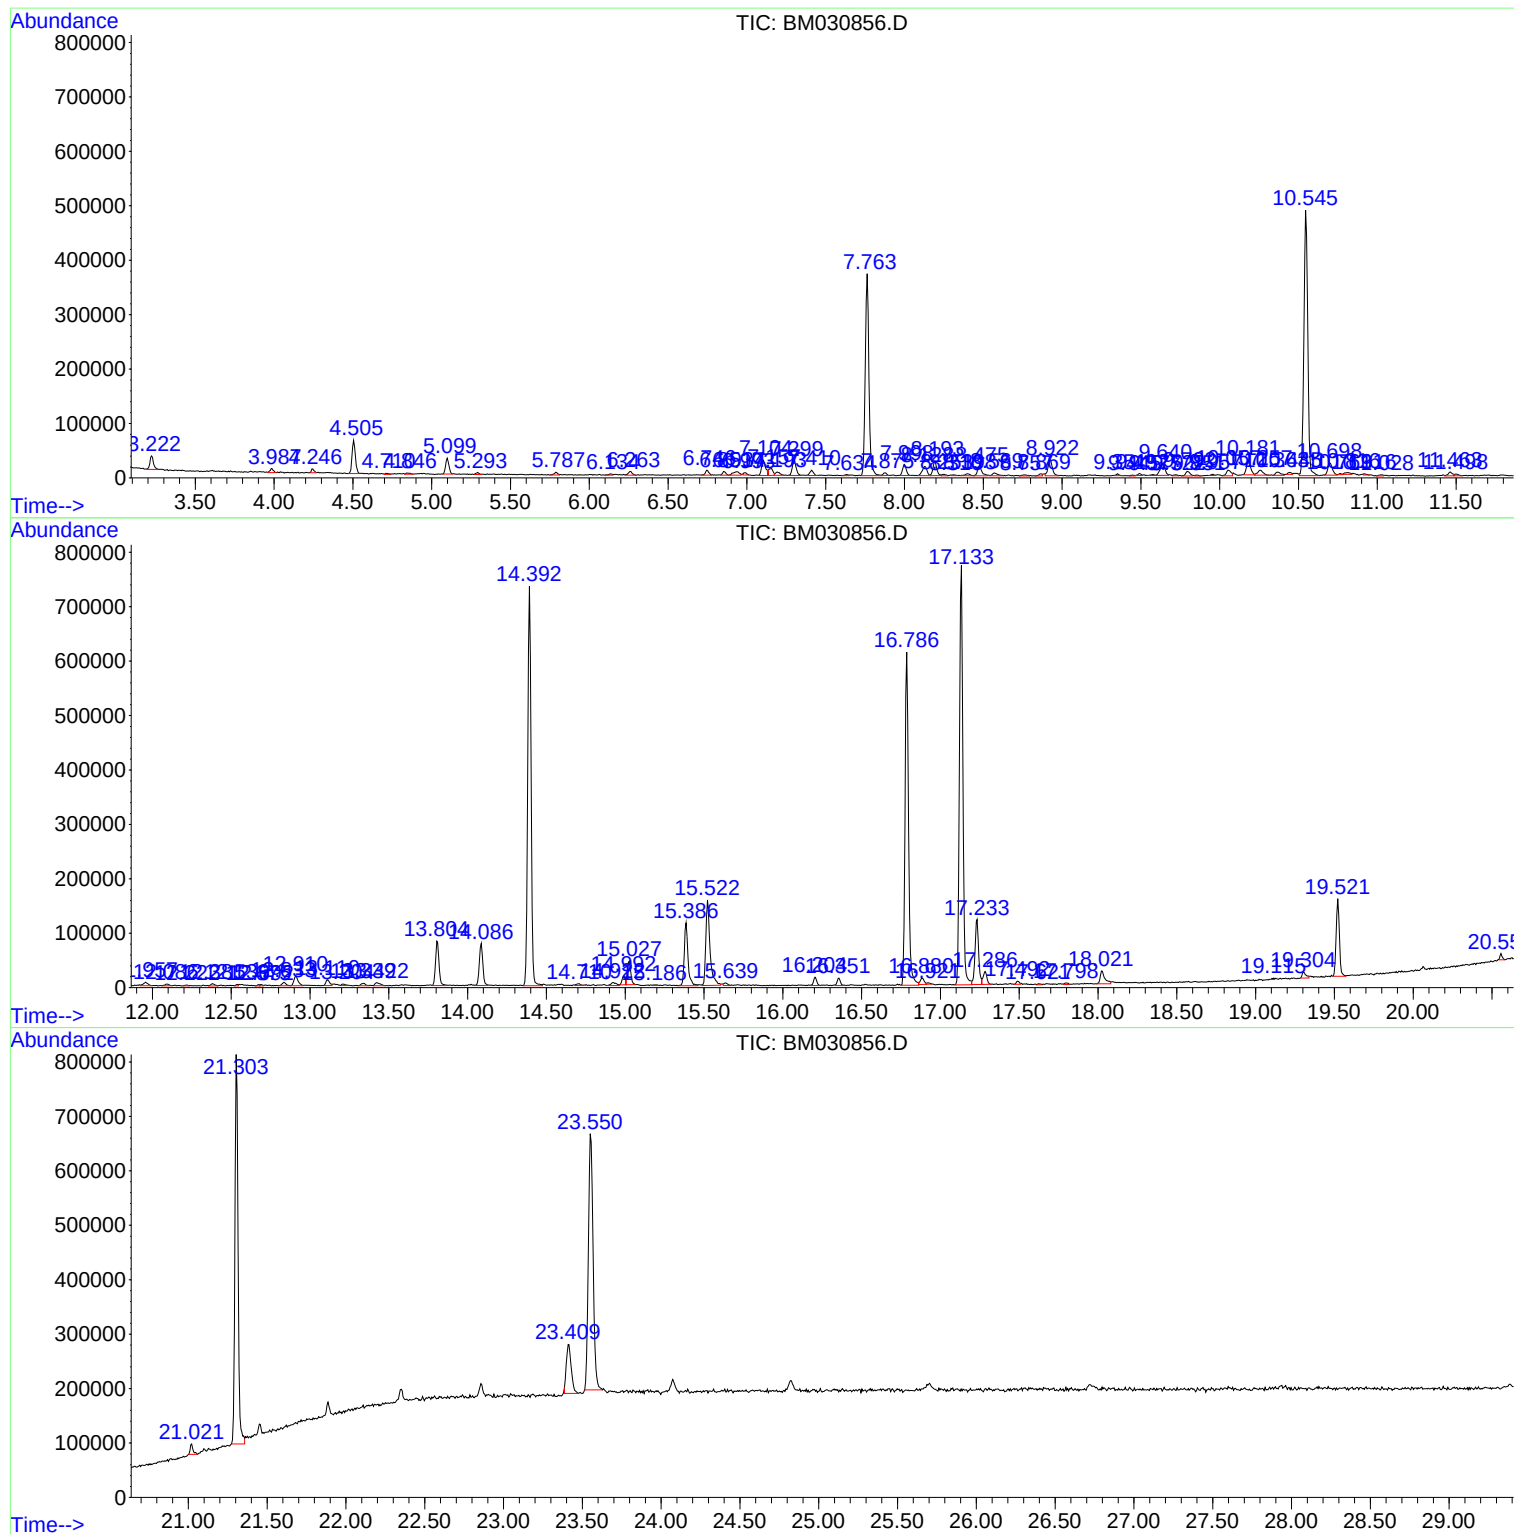

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030856.D
Acq On : 07 Jul 2021 14:38
Operator : CG/JU
Sample : M2905-08DL 5X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK24DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030856.D
Acq On : 07 Jul 2021 14:38
Operator : CG/JU
Sample : M2905-08DL 5X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK24DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
