

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030857.D
 Acq On : 07 Jul 2021 15:15
 Operator : CG/JU
 Sample : M2905-09DL 5X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK25DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030857.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	19	23	30	rVB	21885	31677	2.97%	0.375%
2	3.599	85	87	92	rVB5	1988	2276	0.21%	0.027%
3	3.981	148	152	159	rVB2	6392	10485	0.98%	0.124%
4	4.240	193	196	202	rVB2	5057	8253	0.77%	0.098%
5	4.505	236	241	251	rVB	45681	69822	6.54%	0.827%
6	4.852	295	300	302	rBV2	1686	3262	0.31%	0.039%
7	5.099	336	342	351	rBV	22837	34990	3.28%	0.415%
8	5.287	367	374	382	rVB4	2466	4939	0.46%	0.059%
9	5.787	454	459	464	rVB4	3299	5463	0.51%	0.065%
10	6.263	536	540	543	rBV2	4465	6182	0.58%	0.073%
11	6.746	617	622	628	rVB	6702	10911	1.02%	0.129%
12	6.857	635	641	647	rBV3	4306	7235	0.68%	0.086%
13	6.940	647	655	661	rVV5	6536	16918	1.59%	0.200%
14	6.993	661	664	670	rVB3	3680	5407	0.51%	0.064%
15	7.104	677	683	689	rBV	26412	45702	4.28%	0.542%
16	7.151	689	691	695	rVV2	7666	10295	0.96%	0.122%
17	7.198	695	699	706	rVB3	4114	6867	0.64%	0.081%
18	7.298	711	716	723	rVB2	25425	43073	4.04%	0.510%
19	7.416	730	736	741	rVB	6323	9736	0.91%	0.115%
20	7.763	787	795	805	rBV	356570	580613	54.42%	6.881%
21	7.875	810	814	819	rVB3	4087	6951	0.65%	0.082%
22	7.998	828	835	843	rVB2	13787	23466	2.20%	0.278%
23	8.128	850	857	862	rBV2	13186	25825	2.42%	0.306%
24	8.193	862	868	875	rVV2	16257	28429	2.66%	0.337%
25	8.251	875	878	880	rVB4	1687	2117	0.20%	0.025%
26	8.398	901	903	908	rVB5	2286	3436	0.32%	0.041%
27	8.475	911	916	925	rVV	16213	30870	2.89%	0.366%
28	8.575	928	933	945	rVB8	4231	10701	1.00%	0.127%
29	8.757	960	964	970	rBV7	1746	3681	0.34%	0.044%
30	8.863	977	982	985	rBV4	2410	4206	0.39%	0.050%
31	8.922	987	992	1003	rVB	27372	52125	4.89%	0.618%
32	9.175	1031	1035	1037	rVV3	1694	2501	0.23%	0.030%
33	9.357	1061	1066	1068	rVB4	2257	3083	0.29%	0.037%
34	9.498	1083	1090	1091	rBV4	2686	3868	0.36%	0.046%
35	9.639	1106	1114	1121	rVV2	20849	43309	4.06%	0.513%
36	9.798	1136	1141	1148	rBV6	6472	12363	1.16%	0.147%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030857.D
 Acq On : 07 Jul 2021 15:15
 Operator : CG/JU
 Sample : M2905-09DL 5X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK25DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

37	9.851	1148	1150	1155	rVB4	1478	2029	0.19%	0.024%
38	9.957	1162	1168	1171	rBV7	1628	3373	0.32%	0.040%
39	9.987	1171	1173	1179	rVB5	1521	2392	0.22%	0.028%
40	10.057	1179	1185	1192	rBV	8201	19245	1.80%	0.228%
41	10.181	1197	1206	1214	rVV2	25668	54618	5.12%	0.647%
42	10.263	1214	1220	1226	rVV10	6846	15632	1.47%	0.185%
43	10.357	1229	1236	1247	rBV2	19682	55080	5.16%	0.653%
44	10.445	1249	1251	1257	rVV5	4615	9432	0.88%	0.112%
45	10.486	1257	1258	1261	rVV3	3492	4391	0.41%	0.052%
46	10.545	1261	1268	1281	rVB	472393	808804	75.80%	9.585%
47	10.698	1287	1294	1304	rBV2	21867	49239	4.61%	0.584%
48	10.816	1309	1314	1319	rVV7	3878	9012	0.84%	0.107%
49	10.851	1319	1320	1326	rVV5	2540	3610	0.34%	0.043%
50	10.922	1328	1332	1335	rVB3	2169	2729	0.26%	0.032%
51	11.345	1399	1404	1407	rBV4	1081	1939	0.18%	0.023%
52	11.475	1420	1426	1429	rBV2	2806	5815	0.55%	0.069%
53	11.804	1477	1482	1484	rBV4	1509	2345	0.22%	0.028%
54	11.957	1504	1508	1513	rBV4	3761	6716	0.63%	0.080%
55	12.086	1527	1530	1531	rBV	2064	1905	0.18%	0.023%
56	12.104	1531	1533	1536	rVV4	1965	1851	0.17%	0.022%
57	12.386	1577	1581	1583	rBV3	2527	3004	0.28%	0.036%
58	12.563	1608	1611	1614	rVB4	1636	2148	0.20%	0.025%
59	12.692	1628	1633	1636	rBV3	1621	3246	0.30%	0.038%
60	12.833	1653	1657	1662	rBV5	4153	6853	0.64%	0.081%
61	12.916	1665	1671	1682	rVV3	11181	21965	2.06%	0.260%
62	13.004	1682	1686	1692	rVB3	1147	2295	0.22%	0.027%
63	13.116	1701	1705	1709	rVV4	6259	10816	1.01%	0.128%
64	13.145	1709	1710	1714	rVV3	2022	2579	0.24%	0.031%
65	13.216	1718	1722	1725	rVV4	2952	4060	0.38%	0.048%
66	13.286	1730	1734	1737	rBV3	1327	2155	0.20%	0.026%
67	13.339	1737	1743	1747	rVV5	2939	5421	0.51%	0.064%
68	13.427	1753	1758	1759	rVV4	2670	3211	0.30%	0.038%
69	13.445	1759	1761	1766	rVB4	2457	3009	0.28%	0.036%
70	13.810	1816	1823	1830	rBV	78939	123919	11.61%	1.469%
71	14.033	1855	1861	1864	rBV4	1240	2748	0.26%	0.033%
72	14.086	1864	1870	1875	rBV	78707	113135	10.60%	1.341%
73	14.392	1915	1922	1930	rBV	685199	1019282	95.53%	12.080%
74	14.922	2009	2012	2014	rBV3	2919	3461	0.32%	0.041%
75	14.986	2019	2023	2026	rBV3	10649	15797	1.48%	0.187%
76	15.027	2026	2030	2037	rVB2	28921	44028	4.13%	0.522%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030857.D
 Acq On : 07 Jul 2021 15:15
 Operator : CG/JU
 Sample : M2905-09DL 5X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK25DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

77	15.386	2083	2091	2101	rBV	111676	175586	16.46%	2.081%
78	15.521	2108	2114	2129	rBV	102395	197240	18.49%	2.338%
79	15.633	2132	2133	2137	rVV3	3364	2967	0.28%	0.035%
80	16.204	2227	2230	2237	rVB3	9867	12809	1.20%	0.152%
81	16.357	2252	2256	2261	rVB5	11486	14655	1.37%	0.174%
82	16.515	2279	2283	2288	rBV5	1868	2722	0.26%	0.032%
83	16.786	2323	2329	2343	rVV	413008	617487	57.87%	7.318%
84	16.892	2343	2347	2349	rVV4	8382	13195	1.24%	0.156%
85	16.910	2349	2350	2355	rVV4	3045	5190	0.49%	0.062%
86	17.133	2382	2388	2398	rBV	724960	1066969	100.00%	12.645%
87	17.233	2399	2405	2411	rVV2	111005	184673	17.31%	2.189%
88	17.280	2411	2413	2420	rVB4	16556	25417	2.38%	0.301%
89	17.445	2439	2441	2445	rVB5	2192	2799	0.26%	0.033%
90	17.486	2445	2448	2456	rBV3	4400	10013	0.94%	0.119%
91	17.804	2498	2502	2507	rBV5	5265	6522	0.61%	0.077%
92	18.021	2535	2539	2549	rBV3	21111	43109	4.04%	0.511%
93	18.980	2698	2702	2705	rVB6	6996	9433	0.88%	0.112%
94	19.104	2721	2723	2726	rBV4	2436	3453	0.32%	0.041%
95	19.304	2754	2757	2762	rBV6	10859	16984	1.59%	0.201%
96	19.521	2789	2794	2802	rBV	138256	195861	18.36%	2.321%
97	21.015	3046	3048	3053	rVB4	15978	18606	1.74%	0.221%
98	21.303	3092	3097	3105	rBV	725922	972399	91.14%	11.524%
99	23.409	3452	3455	3467	rVB3	98439	221990	20.81%	2.631%
100	23.550	3473	3479	3492	rVB2	498760	993562	93.12%	11.775%


Sum of corrected areas: 8437967

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030857.D
Acq On : 07 Jul 2021 15:15
Operator : CG/JU
Sample : M2905-09DL 5X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK25DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

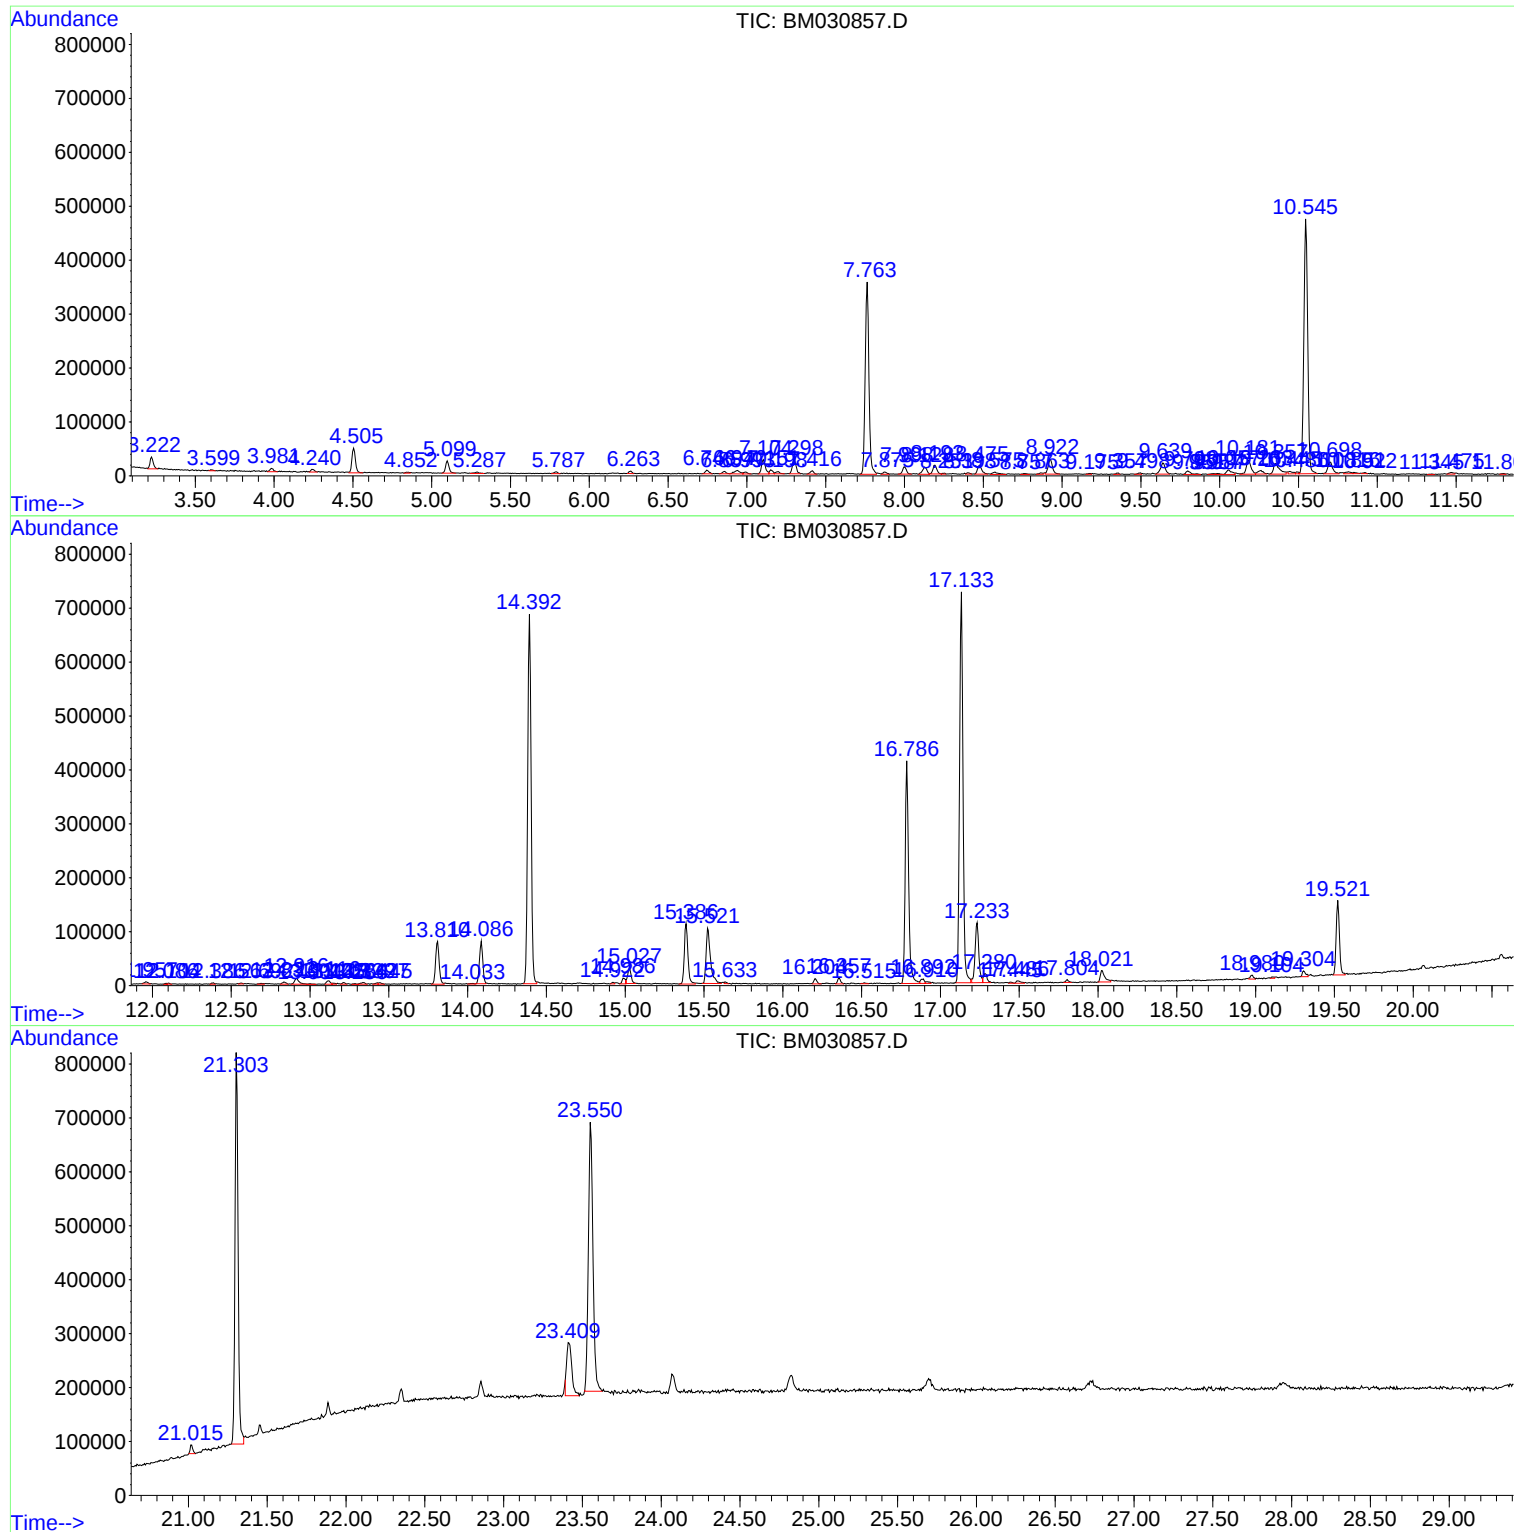

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030857.D
Acq On : 07 Jul 2021 15:15
Operator : CG/JU
Sample : M2905-09DL 5X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK25DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030857.D
Acq On : 07 Jul 2021 15:15
Operator : CG/JU
Sample : M2905-09DL 5X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK25DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
