

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030865.D
 Acq On : 07 Jul 2021 20:14
 Operator : CG/JU
 Sample : M2854-17
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030865.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	10	14	19	rBV3	6517	9797	1.01%	0.093%
2	3.263	27	30	36	rVB2	7243	10217	1.05%	0.097%
3	3.716	104	107	114	rBV2	14685	35348	3.63%	0.334%
4	3.981	149	152	158	rVB2	7001	11567	1.19%	0.109%
5	4.328	207	211	213	rBV4	909	1171	0.12%	0.011%
6	4.534	242	246	248	rBV4	1630	2224	0.23%	0.021%
7	5.422	392	397	403	rBV5	2150	4814	0.49%	0.045%
8	5.781	456	458	461	rBV2	2388	3076	0.32%	0.029%
9	5.869	471	473	475	rBV2	1322	1266	0.13%	0.012%
10	6.198	526	529	531	rVB3	1193	1404	0.14%	0.013%
11	6.475	572	576	579	rVB4	1082	1799	0.18%	0.017%
12	6.757	614	624	630	rBV3	4489	9011	0.92%	0.085%
13	6.875	642	644	648	rVB4	1117	1098	0.11%	0.010%
14	6.934	648	654	663	rBV	123007	214829	22.05%	2.029%
15	7.098	676	682	691	rBV	99439	168107	17.26%	1.588%
16	7.298	709	716	727	rBV	132664	224945	23.09%	2.125%
17	7.381	727	730	739	rVB3	3377	5426	0.56%	0.051%
18	7.604	764	768	773	rBV4	1502	2646	0.27%	0.025%
19	7.763	786	795	803	rBV	313617	520141	53.39%	4.913%
20	7.834	805	807	811	rVV5	2118	2474	0.25%	0.023%
21	7.886	813	816	822	rVB3	3294	5143	0.53%	0.049%
22	7.986	827	833	840	rVB	12118	19170	1.97%	0.181%
23	8.163	861	863	867	rVB5	1546	1644	0.17%	0.016%
24	8.233	870	875	880	rVB5	2833	4713	0.48%	0.045%
25	8.292	880	885	897	rBV	7979	16520	1.70%	0.156%
26	8.428	902	908	909	rBV2	7468	9402	0.97%	0.089%
27	8.469	909	915	930	rVV	136020	242547	24.90%	2.291%
28	8.592	932	936	938	rVV5	1272	1880	0.19%	0.018%
29	8.628	940	942	946	rVV4	3077	4607	0.47%	0.044%
30	8.657	946	947	951	rVB3	1512	1678	0.17%	0.016%
31	8.775	964	967	970	rBV4	1350	1649	0.17%	0.016%
32	8.922	985	992	1003	rBV	111963	202067	20.74%	1.909%
33	9.328	1058	1061	1065	rVB4	876	1225	0.13%	0.012%
34	9.639	1107	1114	1125	rBV	84553	147697	15.16%	1.395%
35	10.175	1198	1205	1217	rBV	111301	229949	23.60%	2.172%
36	10.416	1241	1246	1248	rBV5	1953	3195	0.33%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030865.D
 Acq On : 07 Jul 2021 20:14
 Operator : CG/JU
 Sample : M2854-17
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

37	10.433	1248	1249	1254	rVB4	1105	1121	0.12%	0.011%
38	10.545	1262	1268	1280	rVB	429665	712479	73.14%	6.730%
39	10.692	1287	1293	1315	rBV	105165	238917	24.53%	2.257%
40	11.133	1365	1368	1376	rVB4	684	1178	0.12%	0.011%
41	12.151	1537	1541	1546	rBV2	2175	4070	0.42%	0.038%
42	12.339	1570	1573	1578	rVB4	733	1182	0.12%	0.011%
43	12.751	1641	1643	1646	rVV2	2303	2280	0.23%	0.022%
44	12.774	1646	1647	1652	rVV4	937	1357	0.14%	0.013%
45	12.857	1655	1661	1664	rVB4	928	1421	0.15%	0.013%
46	12.933	1671	1674	1677	rBV4	849	1088	0.11%	0.010%
47	12.998	1682	1685	1690	rVB4	2736	4191	0.43%	0.040%
48	13.221	1719	1723	1727	rBV3	1528	2864	0.29%	0.027%
49	13.804	1815	1822	1838	rBV	249586	382043	39.22%	3.609%
50	14.086	1861	1870	1880	rBV	286642	427041	43.84%	4.034%
51	14.292	1898	1905	1908	rBV6	1944	2367	0.24%	0.022%
52	14.392	1915	1922	1936	rBV	633409	935179	96.00%	8.834%
53	14.621	1956	1961	1977	rBV5	17262	61992	6.36%	0.586%
54	14.721	1977	1978	1985	rVB6	2974	4025	0.41%	0.038%
55	14.986	2018	2023	2028	rVB6	2972	5254	0.54%	0.050%
56	15.198	2053	2059	2061	rBV4	1423	2524	0.26%	0.024%
57	15.215	2061	2062	2065	rVV	1426	1569	0.16%	0.015%
58	15.239	2065	2066	2072	rVB3	2083	2347	0.24%	0.022%
59	15.386	2084	2091	2104	rBV	369689	565772	58.08%	5.344%
60	15.521	2109	2114	2126	rVV	31178	62579	6.42%	0.591%
61	15.627	2130	2132	2137	rVB2	4348	4659	0.48%	0.044%
62	15.804	2158	2162	2168	rVV2	3535	5453	0.56%	0.052%
63	15.857	2168	2171	2174	rVB3	995	1091	0.11%	0.010%
64	15.998	2190	2195	2196	rBV4	837	1159	0.12%	0.011%
65	16.045	2200	2203	2205	rBV4	1053	1039	0.11%	0.010%
66	16.168	2220	2224	2230	rVB7	3441	4492	0.46%	0.042%
67	16.274	2238	2242	2246	rBV5	2189	3557	0.37%	0.034%
68	16.368	2250	2258	2262	rBV6	3532	6054	0.62%	0.057%
69	16.521	2278	2284	2288	rBV6	5180	9206	0.95%	0.087%
70	16.592	2292	2296	2300	rVB5	1672	2475	0.25%	0.023%
71	16.686	2307	2312	2314	rBV4	1111	1563	0.16%	0.015%
72	16.798	2329	2331	2334	rVB3	1813	1570	0.16%	0.015%
73	16.868	2340	2343	2346	rBV4	1977	3188	0.33%	0.030%
74	16.892	2346	2347	2350	rVV3	2730	3096	0.32%	0.029%
75	16.921	2350	2352	2354	rVV2	3019	2969	0.30%	0.028%
76	16.939	2354	2355	2360	rVV5	1545	2253	0.23%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030865.D
 Acq On : 07 Jul 2021 20:14
 Operator : CG/JU
 Sample : M2854-17
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDW1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

77	17.062	2374	2376	2378	rVB3	1248	1251	0.13%	0.012%
78	17.133	2381	2388	2395	rBV	650736	974165	100.00%	9.202%
79	17.227	2397	2404	2418	rVB	329926	556978	57.17%	5.261%
80	17.415	2433	2436	2437	rVV3	1425	1510	0.16%	0.014%
81	17.427	2437	2438	2441	rVB2	1587	1529	0.16%	0.014%
82	17.662	2476	2478	2481	rBV3	1355	1516	0.16%	0.014%
83	17.733	2487	2490	2491	rBV3	1408	1295	0.13%	0.012%
84	17.780	2494	2498	2500	rBV4	1565	2619	0.27%	0.025%
85	17.803	2500	2502	2506	rVB4	3048	3224	0.33%	0.030%
86	17.898	2515	2518	2523	rBV5	6829	10302	1.06%	0.097%
87	17.974	2528	2531	2533	rBV3	1750	2478	0.25%	0.023%
88	18.021	2535	2539	2546	rBV2	38718	59631	6.12%	0.563%
89	18.403	2600	2604	2606	rBV5	1676	1991	0.20%	0.019%
90	18.474	2610	2616	2624	rVV	13032	28371	2.91%	0.268%
91	18.568	2628	2632	2635	rVV5	1644	3016	0.31%	0.028%
92	18.698	2652	2654	2656	rBV2	1849	2169	0.22%	0.020%
93	19.156	2730	2732	2733	rBV2	3740	3828	0.39%	0.036%
94	19.303	2754	2757	2763	rBV6	16100	25561	2.62%	0.241%
95	19.521	2788	2794	2800	rBV	351526	502769	51.61%	4.749%
96	20.515	2958	2963	2968	rBV	563994	646646	66.38%	6.108%
97	21.303	3092	3097	3110	rBV	630207	859648	88.24%	8.120%
98	22.474	3293	3296	3301	rVB	60984	75119	7.71%	0.710%
99	23.403	3449	3454	3467	rVB	164993	364573	37.42%	3.444%
100	23.550	3473	3479	3493	rVB2	418736	853024	87.56%	8.058%


Sum of corrected areas: 10586323

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030865.D
Acq On : 07 Jul 2021 20:14
Operator : CG/JU
Sample : M2854-17
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDW1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

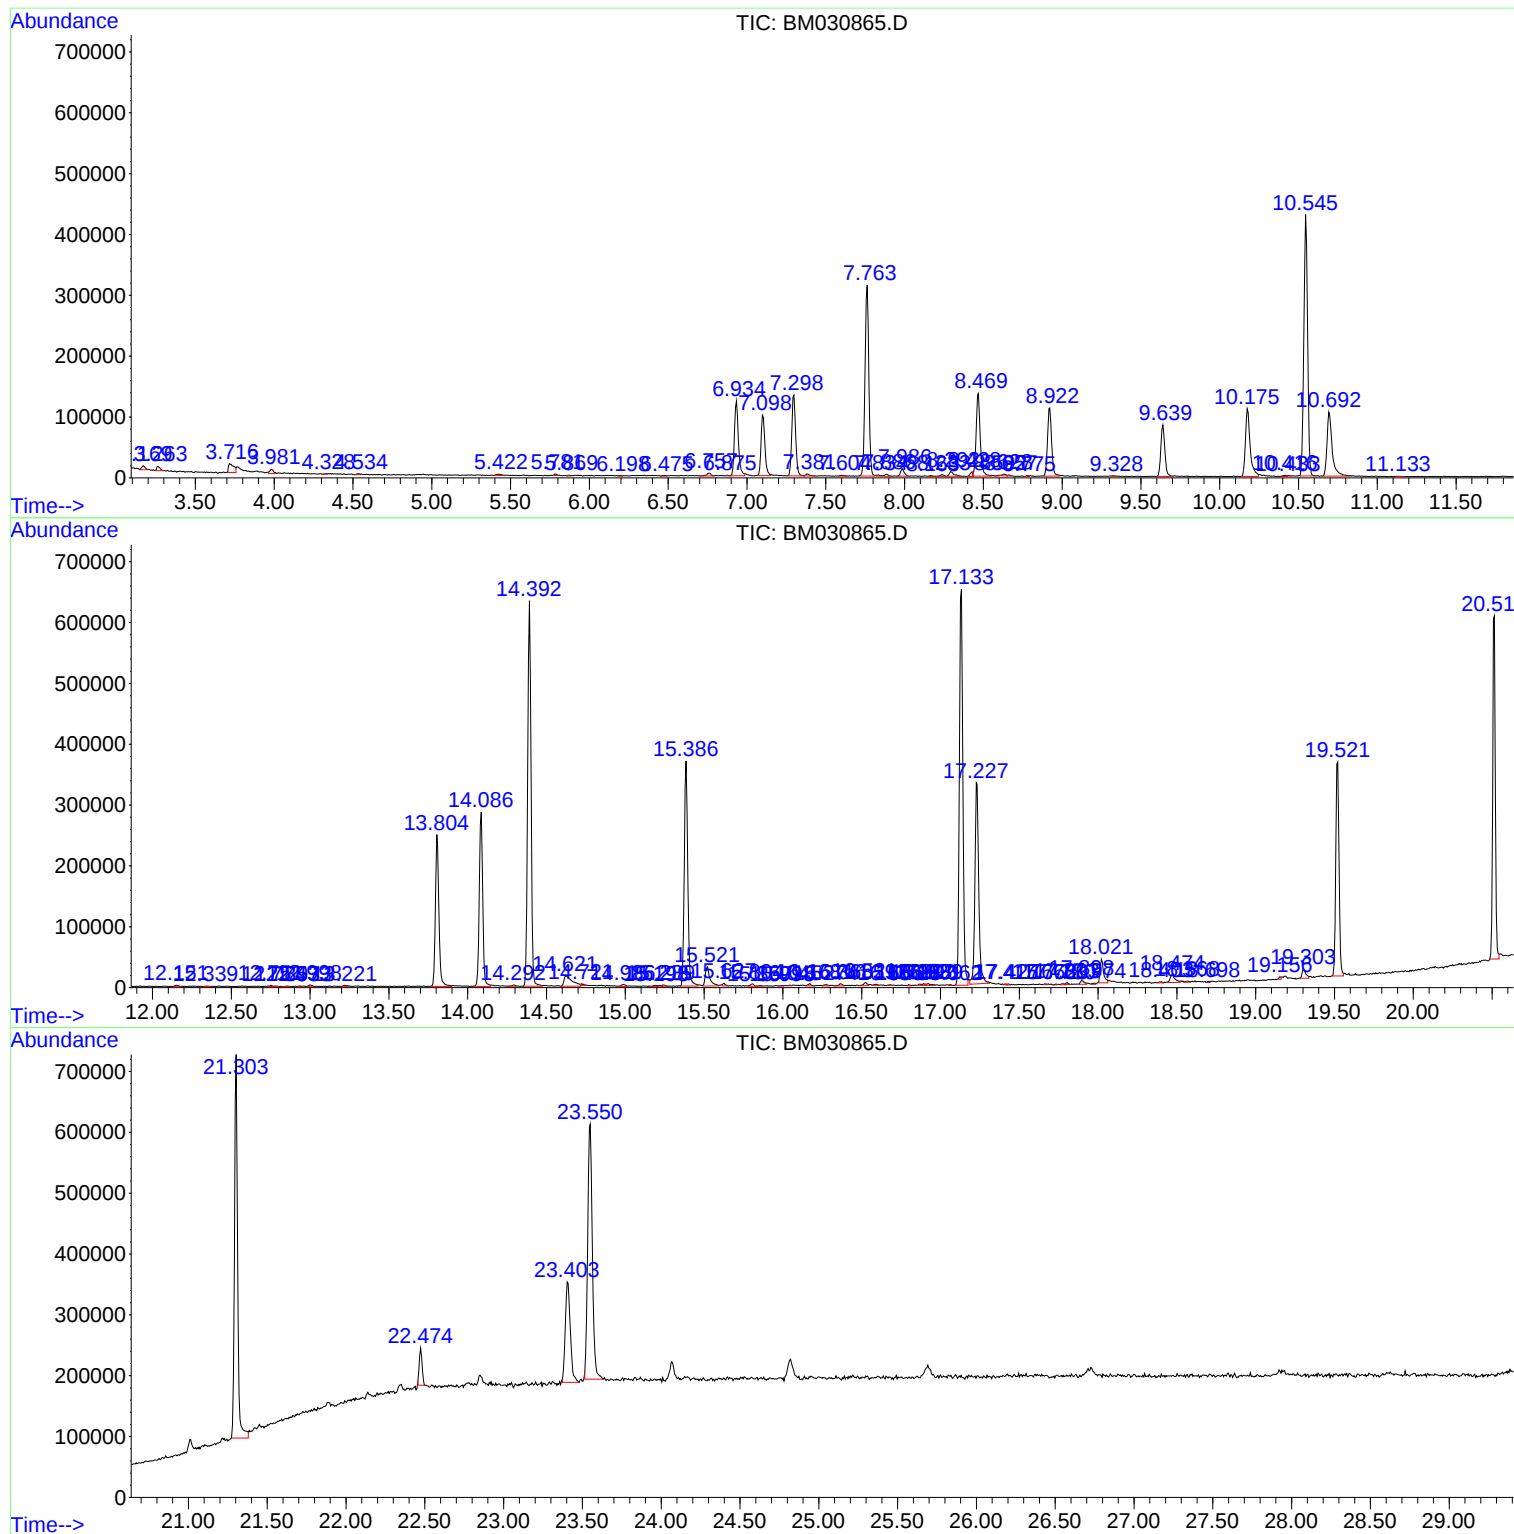

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030865.D
Acq On : 07 Jul 2021 20:14
Operator : CG/JU
Sample : M2854-17
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDW1










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Diisooctyl adipate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.520	15.04 ng/ul	646646	Chrysene-d12	21.303

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diisooctyl adipate	370	C22H42O4	001330-86-5	87
2			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	87
3			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	78
4			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	76
5			Hexanedioic acid, mono(2-ethylhe...	258	C14H26O4	004337-65-9	64

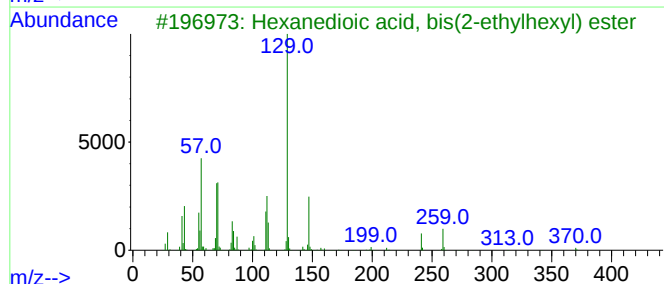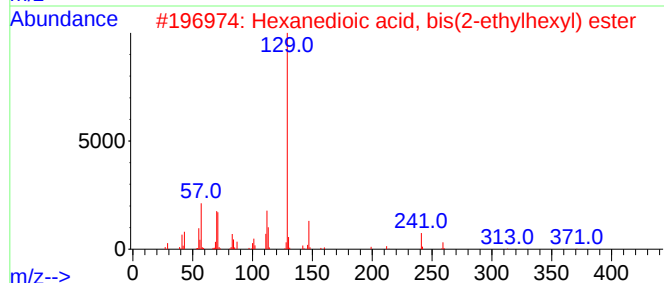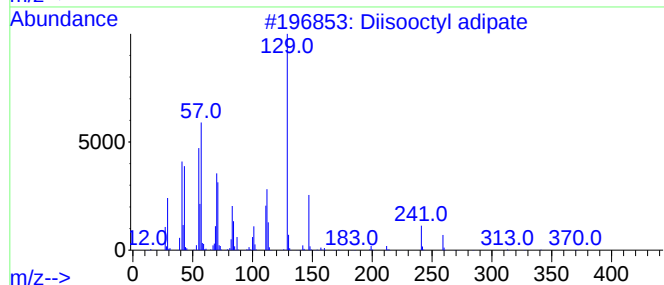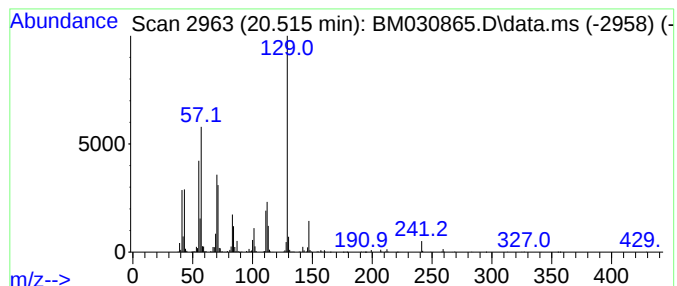

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030865.D
Acq On : 07 Jul 2021 20:14
Operator : CG/JU
Sample : M2854-17
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDW1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diisooctyl adipate	20.520	15.0	ng/ul	646646	5	21.303	859648	20.0