

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030866.D
 Acq On : 07 Jul 2021 20:52
 Operator : CG/JU
 Sample : M2877-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030866.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	38	rVB2	7552	13416	1.43%	0.132%
2	3.710	103	106	115	rBV	22700	61417	6.55%	0.605%
3	3.887	135	136	141	rVB5	3339	3384	0.36%	0.033%
4	3.987	149	153	157	rVB2	6004	8102	0.86%	0.080%
5	4.410	223	225	226	rVB2	1895	1199	0.13%	0.012%
6	5.422	394	397	399	rBV4	1084	1223	0.13%	0.012%
7	5.469	402	405	409	rVB5	1055	1521	0.16%	0.015%
8	5.593	424	426	428	rVB2	1465	1054	0.11%	0.010%
9	5.781	456	458	464	rVB5	1380	1586	0.17%	0.016%
10	5.904	476	479	482	rBV3	1125	1166	0.12%	0.011%
11	6.757	620	624	627	rBV5	1703	2677	0.29%	0.026%
12	6.934	645	654	666	rBV	113758	201242	21.47%	1.983%
13	7.098	676	682	694	rBV	96674	161522	17.23%	1.591%
14	7.298	710	716	726	rBV	127549	214074	22.84%	2.109%
15	7.387	726	731	736	rVB5	2662	4131	0.44%	0.041%
16	7.651	772	776	777	rBV2	1030	1119	0.12%	0.011%
17	7.763	788	795	806	rBV	322522	522440	55.74%	5.147%
18	7.840	806	808	813	rVB6	1372	1839	0.20%	0.018%
19	7.887	813	816	818	rBV3	1596	1200	0.13%	0.012%
20	7.993	827	834	837	rBV4	2749	4906	0.52%	0.048%
21	8.298	880	886	889	rBV3	2349	3678	0.39%	0.036%
22	8.328	889	891	894	rVB3	825	993	0.11%	0.010%
23	8.428	902	908	909	rBV6	2075	2855	0.30%	0.028%
24	8.463	909	914	925	rVB	131696	229454	24.48%	2.261%
25	8.593	932	936	941	rBV2	2684	3992	0.43%	0.039%
26	8.628	941	942	945	rVV3	1306	1306	0.14%	0.013%
27	8.916	985	991	1001	rBV	109695	195175	20.82%	1.923%
28	9.087	1017	1020	1026	rVB5	1679	2657	0.28%	0.026%
29	9.157	1029	1032	1033	rBV	1169	1029	0.11%	0.010%
30	9.328	1059	1061	1063	rVB2	1324	1055	0.11%	0.010%
31	9.639	1108	1114	1126	rVB	82637	142236	15.17%	1.401%
32	10.104	1191	1193	1198	rVB3	749	1004	0.11%	0.010%
33	10.175	1198	1205	1221	rBV	104974	216819	23.13%	2.136%
34	10.339	1232	1233	1240	rBV3	874	1031	0.11%	0.010%
35	10.416	1241	1246	1247	rBV4	1444	1870	0.20%	0.018%
36	10.545	1261	1268	1275	rBV	437279	724210	77.26%	7.135%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030866.D
 Acq On : 07 Jul 2021 20:52
 Operator : CG/JU
 Sample : M2877-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

37	10.692	1286	1293	1308	rBV	102269	222020	23.69%	2.187%
38	10.786	1308	1309	1312	rVB2	2246	1223	0.13%	0.012%
39	12.145	1537	1540	1545	rBV3	1898	3234	0.35%	0.032%
40	12.751	1636	1643	1646	rBV5	2445	3820	0.41%	0.038%
41	13.004	1680	1686	1689	rVB4	3001	4266	0.46%	0.042%
42	13.292	1728	1735	1741	rBV	24096	40049	4.27%	0.395%
43	13.575	1779	1783	1785	rBV3	680	995	0.11%	0.010%
44	13.633	1790	1793	1797	rVB2	850	1112	0.12%	0.011%
45	13.804	1816	1822	1827	rBV	223105	328857	35.08%	3.240%
46	13.851	1827	1830	1841	rVB	54760	84430	9.01%	0.832%
47	14.086	1860	1870	1880	rBV	243495	383595	40.92%	3.779%
48	14.298	1901	1906	1907	rBV3	908	1087	0.12%	0.011%
49	14.392	1915	1922	1932	rBV	614981	904903	96.54%	8.915%
50	14.627	1955	1962	1974	rBV3	16548	54977	5.87%	0.542%
51	14.745	1980	1982	1987	rVB3	1490	1748	0.19%	0.017%
52	14.792	1987	1990	1992	rVV3	989	993	0.11%	0.010%
53	14.951	2012	2017	2023	rBV2	4110	7204	0.77%	0.071%
54	15.192	2053	2058	2063	rBV3	1805	3935	0.42%	0.039%
55	15.386	2084	2091	2105	rVV	324250	492142	52.50%	4.849%
56	15.516	2108	2113	2127	rVB	33330	63167	6.74%	0.622%
57	15.621	2127	2131	2133	rBV3	2609	2572	0.27%	0.025%
58	15.739	2147	2151	2153	rBV2	1177	1479	0.16%	0.015%
59	15.892	2175	2177	2181	rBV2	809	1080	0.12%	0.011%
60	15.939	2184	2185	2190	rVB4	1045	1022	0.11%	0.010%
61	16.016	2195	2198	2200	rVB4	1492	1531	0.16%	0.015%
62	16.057	2200	2205	2206	rBV4	1449	1972	0.21%	0.019%
63	16.110	2211	2214	2216	rVV3	1275	1163	0.12%	0.011%
64	16.168	2220	2224	2226	rBV3	1971	2318	0.25%	0.023%
65	16.274	2235	2242	2245	rBV7	1215	2185	0.23%	0.022%
66	16.357	2253	2256	2257	rBV	1078	1005	0.11%	0.010%
67	16.480	2275	2277	2280	rVB4	1100	1007	0.11%	0.010%
68	16.516	2280	2283	2286	rBV3	1013	1429	0.15%	0.014%
69	16.557	2288	2290	2293	rVB4	1248	1524	0.16%	0.015%
70	16.586	2293	2295	2298	rBV4	1308	1455	0.16%	0.014%
71	16.763	2322	2325	2326	rBV2	1096	987	0.11%	0.010%
72	16.880	2340	2345	2348	rBV5	1867	4643	0.50%	0.046%
73	16.921	2350	2352	2356	rBV2	2447	3000	0.32%	0.030%
74	16.963	2356	2359	2360	rBV3	1105	1060	0.11%	0.010%
75	17.133	2381	2388	2399	rBV	607519	935039	99.76%	9.212%
76	17.233	2399	2405	2419	rVB	299348	481523	51.37%	4.744%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
 Data File : BM030866.D
 Acq On : 07 Jul 2021 20:52
 Operator : CG/JU
 Sample : M2877-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
 Title : SVOA CALIBRATION

77	17.427	2434	2438	2441	rBV5	1346	2046	0.22%	0.020%
78	17.515	2448	2453	2455	rBV6	2416	3488	0.37%	0.034%
79	17.627	2469	2472	2475	rBV4	2007	2830	0.30%	0.028%
80	17.804	2500	2502	2505	rVB4	1666	1252	0.13%	0.012%
81	17.915	2520	2521	2524	rBV3	1484	1391	0.15%	0.014%
82	17.980	2529	2532	2534	rBV3	1404	1720	0.18%	0.017%
83	18.021	2534	2539	2549	rBV3	39842	76270	8.14%	0.751%
84	18.204	2566	2570	2574	rBV7	4585	7467	0.80%	0.074%
85	18.268	2580	2581	2583	rBV2	1458	1404	0.15%	0.014%
86	18.410	2603	2605	2608	rBV4	2249	2421	0.26%	0.024%
87	18.486	2614	2618	2620	rVV5	1636	2521	0.27%	0.025%
88	18.621	2637	2641	2644	rVB4	3476	4441	0.47%	0.044%
89	18.698	2652	2654	2655	rBV2	1638	1370	0.15%	0.013%
90	18.786	2666	2669	2671	rBV3	2811	3397	0.36%	0.033%
91	18.827	2674	2676	2678	rBV3	1625	1342	0.14%	0.013%
92	19.109	2722	2724	2726	rBV3	2147	1487	0.16%	0.015%
93	19.186	2733	2737	2742	rVB2	31028	43739	4.67%	0.431%
94	19.304	2753	2757	2761	rBV4	15059	26522	2.83%	0.261%
95	19.515	2788	2793	2809	rBV	340020	545703	58.22%	5.376%
96	20.509	2958	2962	2967	rBV	208154	238126	25.40%	2.346%
97	21.009	3044	3047	3053	rBV5	32009	38843	4.14%	0.383%
98	21.298	3091	3096	3109	rBV	661749	937333	100.00%	9.235%
99	23.403	3449	3454	3468	rVB	225560	485043	51.75%	4.779%
100	23.544	3472	3478	3490	rVB	483114	929520	99.17%	9.158%


Sum of corrected areas: 10150009

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030866.D
Acq On : 07 Jul 2021 20:52
Operator : CG/JU
Sample : M2877-01
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDY9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

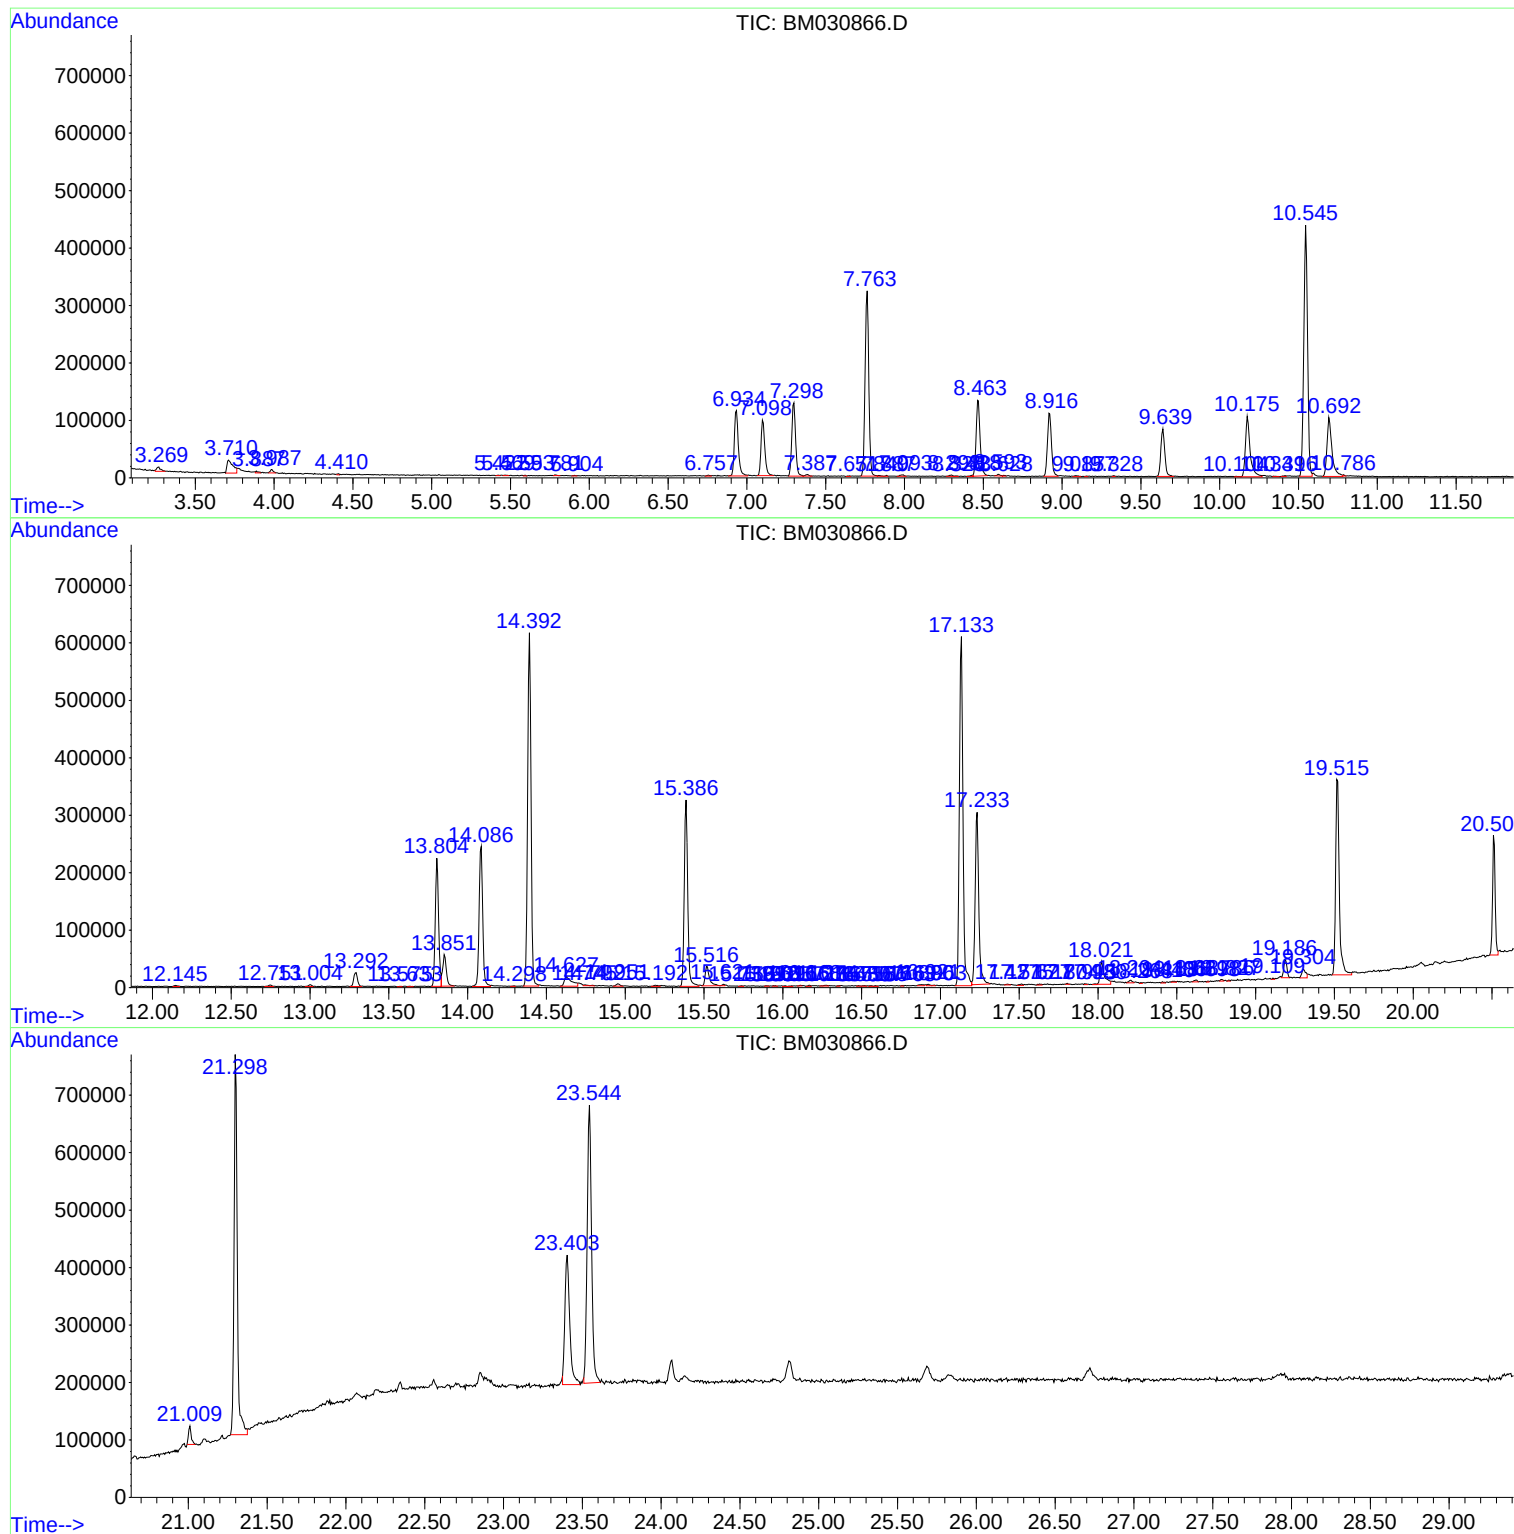

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030866.D
Acq On : 07 Jul 2021 20:52
Operator : CG/JU
Sample : M2877-01
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDY9










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Diisooctyl adipate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.510	5.08 ng/ul	238126	Chrysene-d12	21.298

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diisooctyl adipate	370	C22H42O4	001330-86-5	91
2			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	91
3			Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	90
4			Adipic acid, 2-ethylhexyl octyl ...	370	C22H42O4	1000324-48-6	87
5			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	86

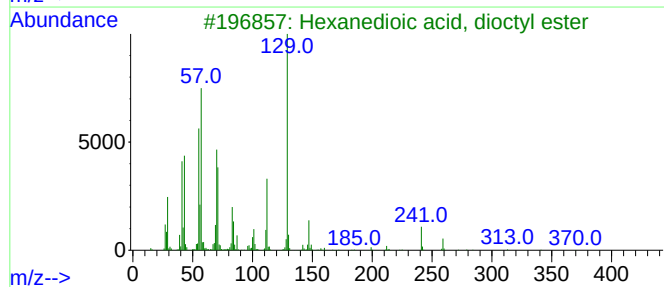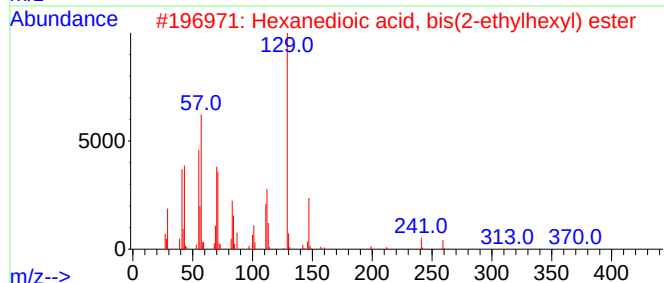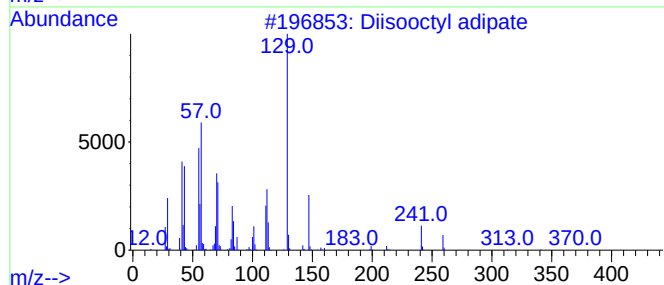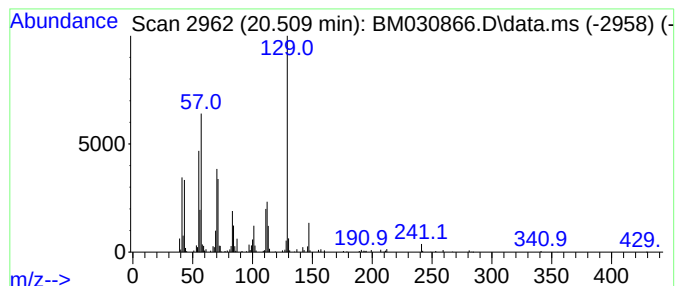

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070621\
Data File : BM030866.D
Acq On : 07 Jul 2021 20:52
Operator : CG/JU
Sample : M2877-01
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDY9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM070621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diisooctyl adipate	20.510	5.1	ng/ul	238126	5	21.298	937333	20.0