
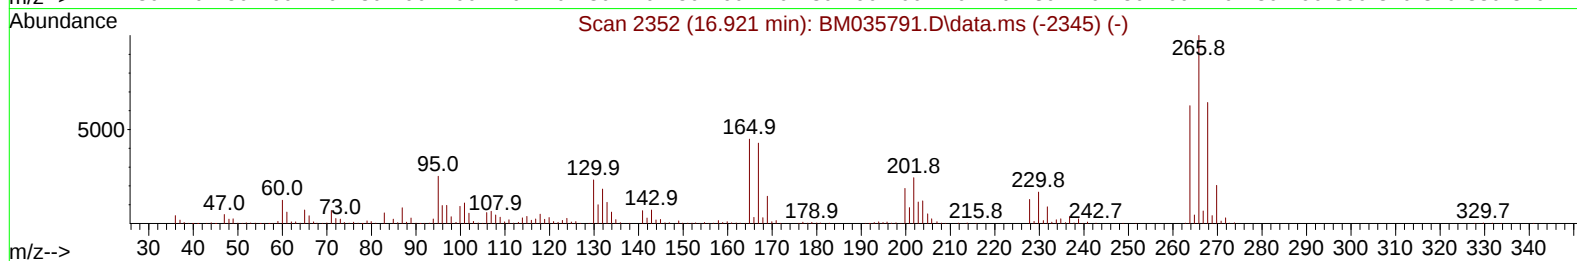
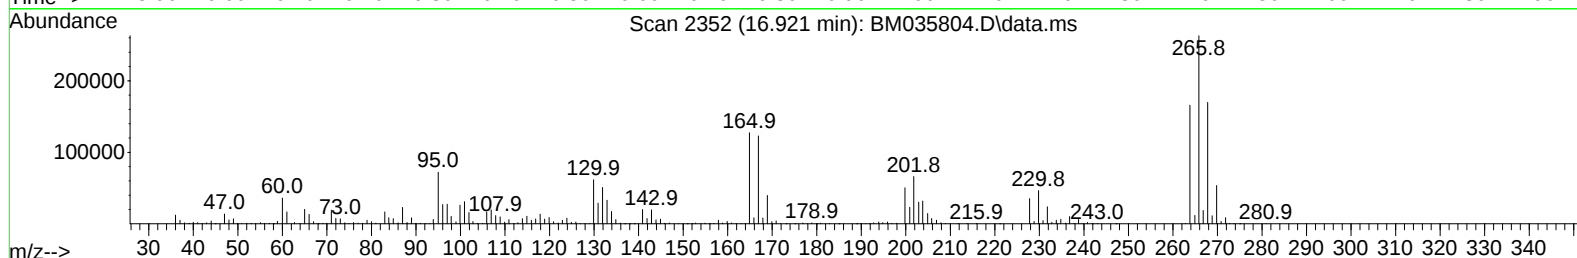


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071422\
 Data File : BM035804.D
 Acq On : 14 Jul 2022 09:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 05:38:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 14 01:21:21 2022
 Response via : Initial Calibration

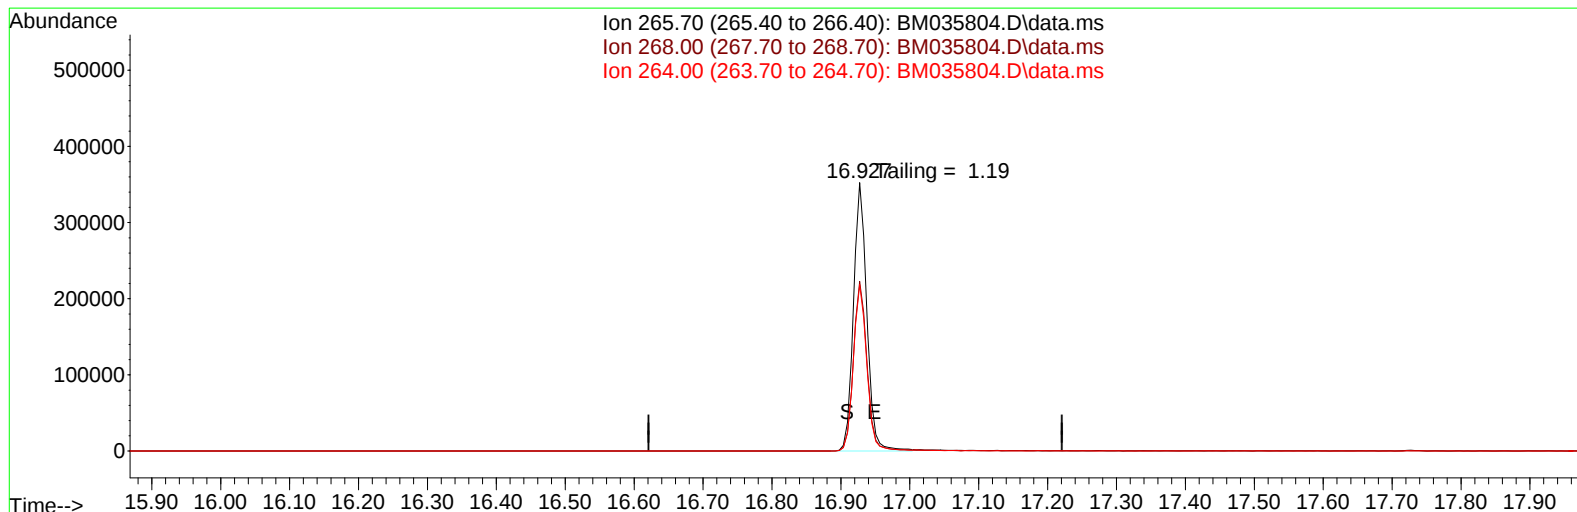

TIC: BM035804.D\data.ms

(70) Pentachlorophenol (C)




16.921min (-16.921) 0.00 ng

response 0

Ion	Exp%	Act%
265.70	100.00	0.00
268.00	64.90	0.00#
264.00	63.30	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071422\
 Data File : BM035804.D
 Acq On : 14 Jul 2022 09:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 05:38:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 14 01:21:21 2022
 Response via : Initial Calibration

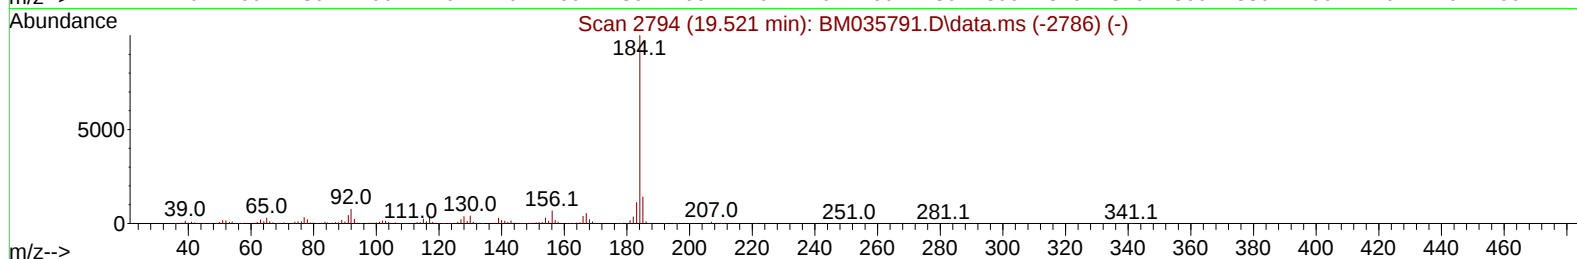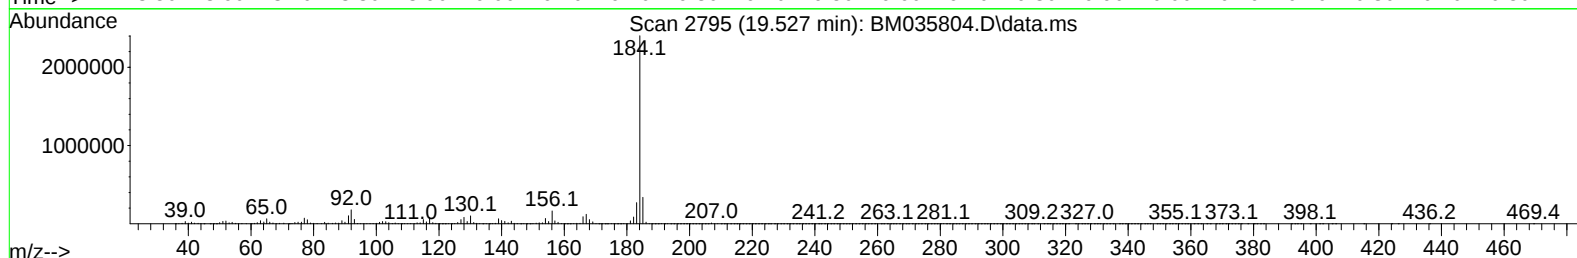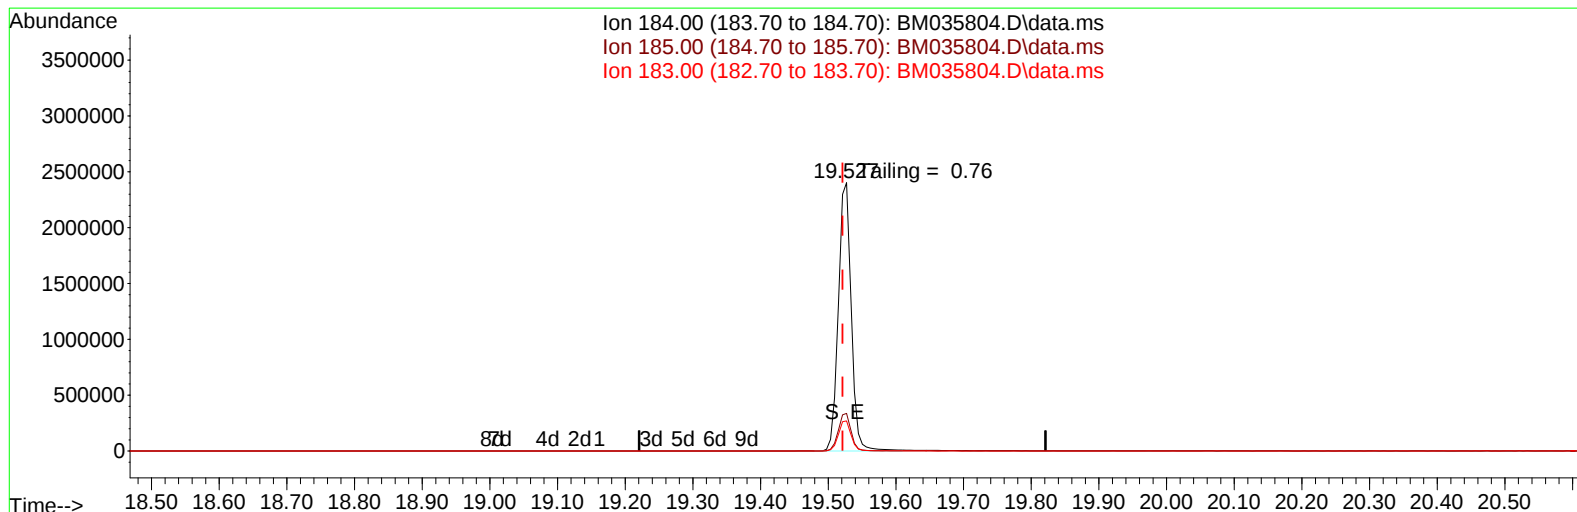

TIC: BM035804.D\data.ms

(77) Benzidine

19.527min (+ 0.006) 1102360.52 ng m

response 3179181

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.02
183.00	11.90	11.22
0.00	0.00	0.00