

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM071422\  
 Data File : BM035806.D  
 Acq On : 14 Jul 2022 11:07  
 Operator : CG/JU  
 Sample : PB146188BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 PB146188BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM071322.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035806.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.469       | 398           | 405         | 414          | rBV      | 5347959        | 7626453       | 30.92%          | 7.900%        |
| 2         | 7.075       | 670           | 678         | 694          | rBV      | 5464324        | 8416334       | 34.12%          | 8.718%        |
| 3         | 7.910       | 812           | 820         | 831          | rBV      | 1227651        | 1881695       | 7.63%           | 1.949%        |
| 4         | 9.075       | 1009          | 1018        | 1027         | rBV      | 3366376        | 5376363       | 21.80%          | 5.569%        |
| 5         | 10.716      | 1289          | 1297        | 1305         | rBV      | 1772050        | 2899553       | 11.76%          | 3.004%        |
| 6         | 13.175      | 1708          | 1715        | 1725         | rBV      | 9478306        | 13910430      | 56.40%          | 14.410%       |
| 7         | 14.545      | 1941          | 1948        | 1957         | rBV      | 2837362        | 4046368       | 16.40%          | 4.192%        |
| 8         | 16.027      | 2193          | 2200        | 2217         | rBV      | 8132517        | 11262166      | 45.66%          | 11.666%       |
| 9         | 17.280      | 2407          | 2413        | 2422         | rBV      | 3628679        | 5076037       | 20.58%          | 5.258%        |
| 10        | 19.909      | 2854          | 2860        | 2872         | rBV      | 19691829       | 24665731      | 100.00%         | 25.551%       |
| 11        | 21.456      | 3118          | 3123        | 3133         | rBV      | 4519850        | 5510171       | 22.34%          | 5.708%        |
| 12        | 23.845      | 3522          | 3529        | 3539         | rVB2     | 2928518        | 5863181       | 23.77%          | 6.074%        |




Sum of corrected areas: 96534482

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM071422\  
Data File : BM035806.D  
Acq On : 14 Jul 2022 11:07  
Operator : CG/JU  
Sample : PB146188BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB146188BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM071322.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

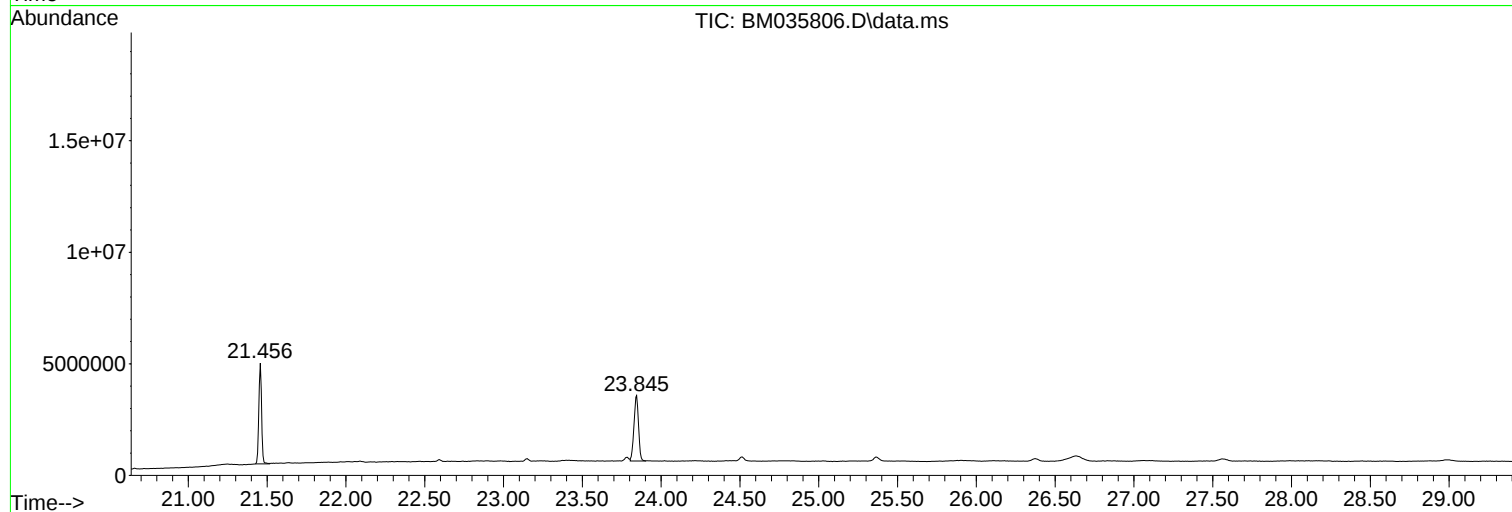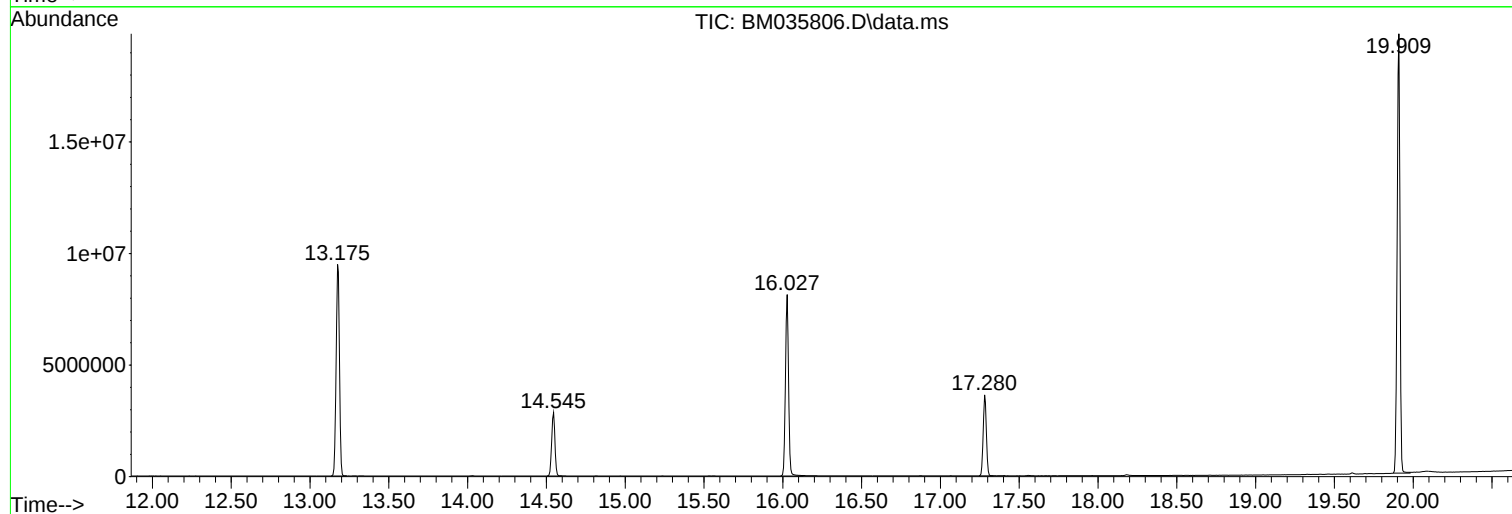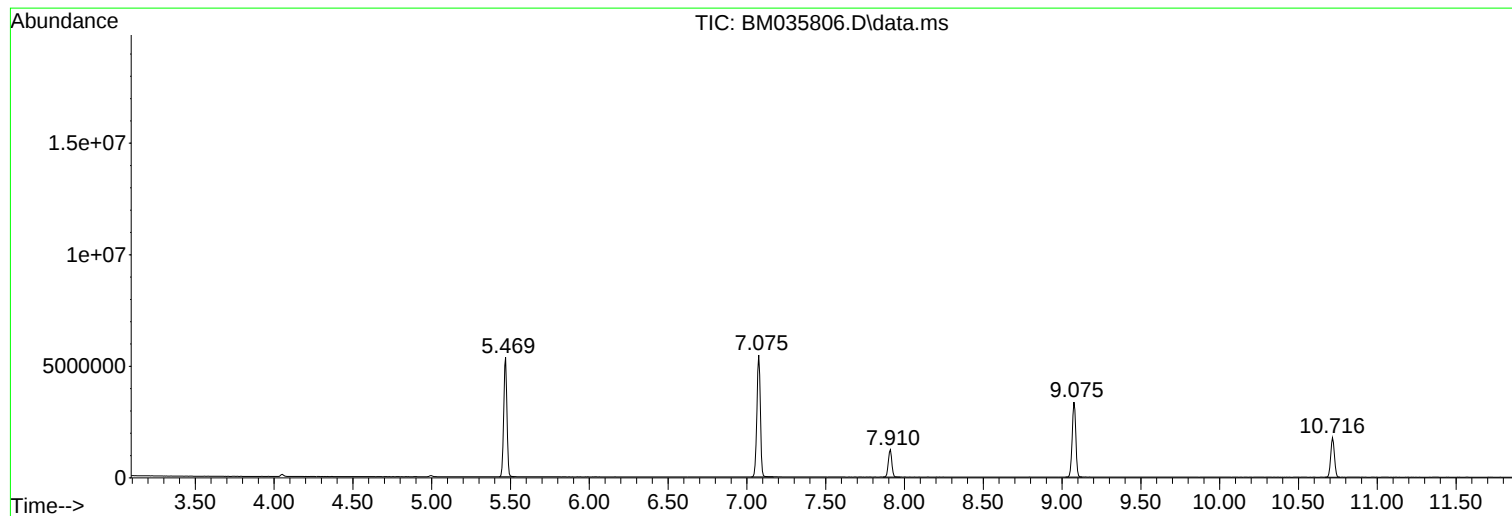

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM071422\  
Data File : BM035806.D  
Acq On : 14 Jul 2022 11:07  
Operator : CG/JU  
Sample : PB146188BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB146188BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM071322.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM071422\  
Data File : BM035806.D  
Acq On : 14 Jul 2022 11:07  
Operator : CG/JU  
Sample : PB146188BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB146188BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM071322.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|