
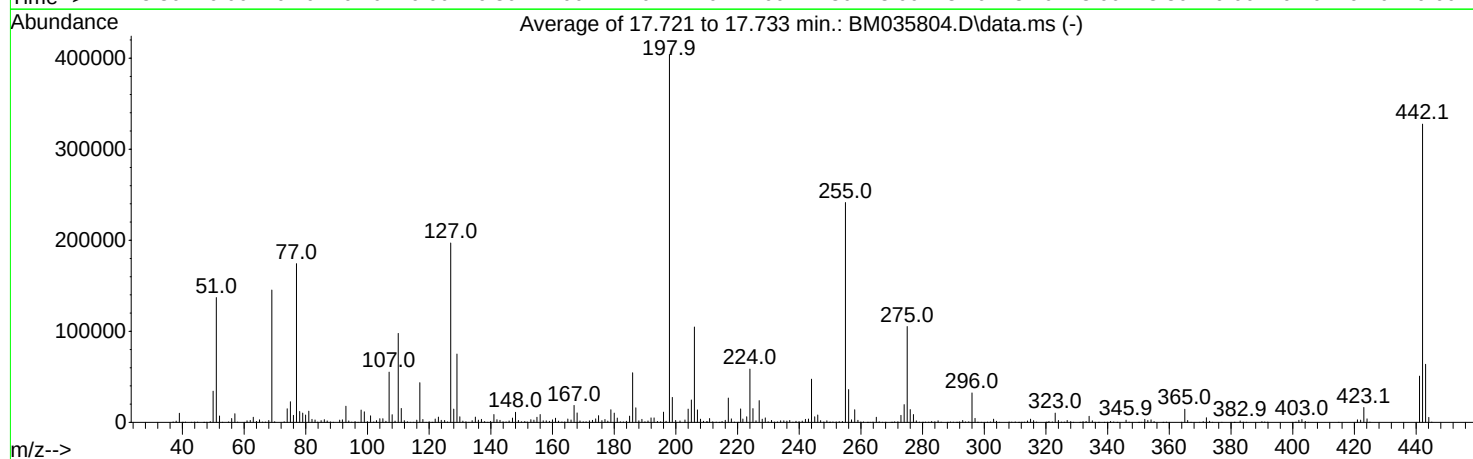


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071422\
 Data File : BM035804.D
 Acq On : 14 Jul 2022 09:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 14 01:21:21 2022

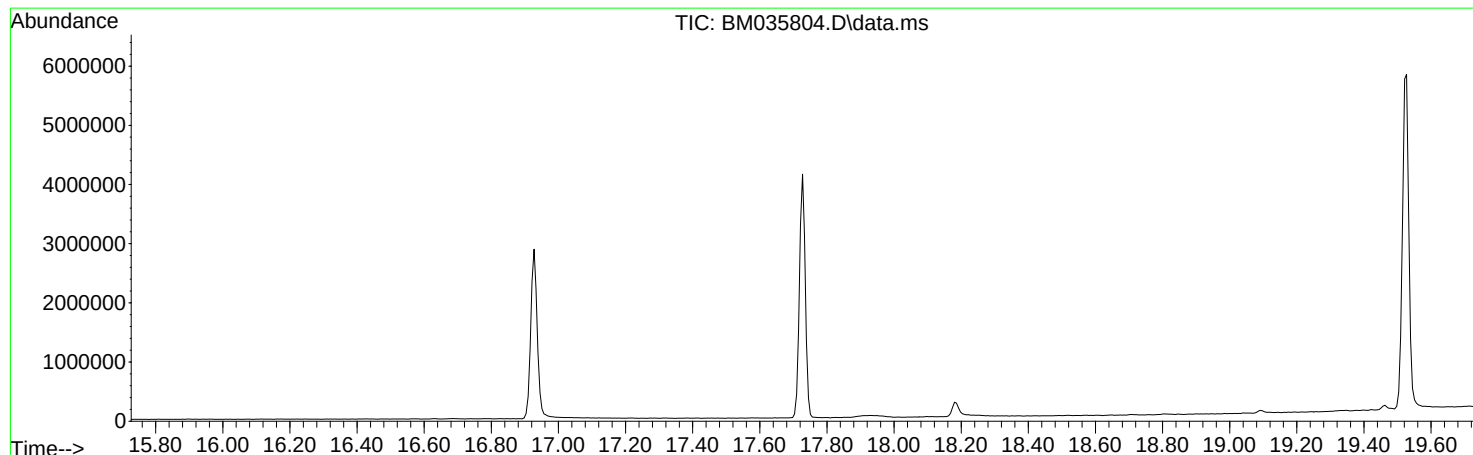




AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	137108	PASS
68	69	0.00	2	1.5	2180	PASS
69	198	0.00	100	36.0	145421	PASS
70	69	0.00	2	0.5	668	PASS
127	198	10	80	48.8	197056	PASS
197	198	0.00	2	0.3	1154	PASS
198	198	100	100	100.0	404032	PASS
199	198	5	9	6.8	27458	PASS
275	198	10	60	26.0	105237	PASS
365	198	1	100	3.6	14437	PASS
441	198	0.01	100	12.6	50789	PASS
442	442	50	100	100.0	327509	PASS
443	442	15	24	19.5	63776	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071422\
 Data File : BM035804.D
 Acq On : 14 Jul 2022 09:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jul 15 05:38:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 14 01:21:21 2022
 Response via : Initial Calibration

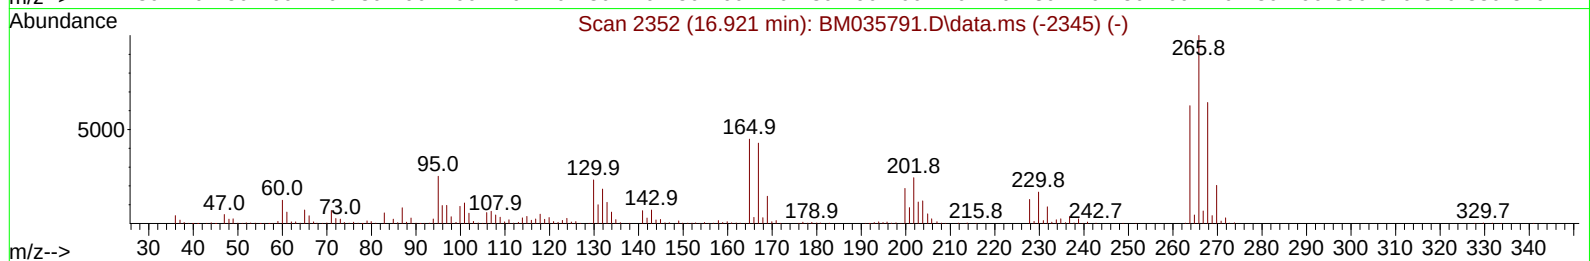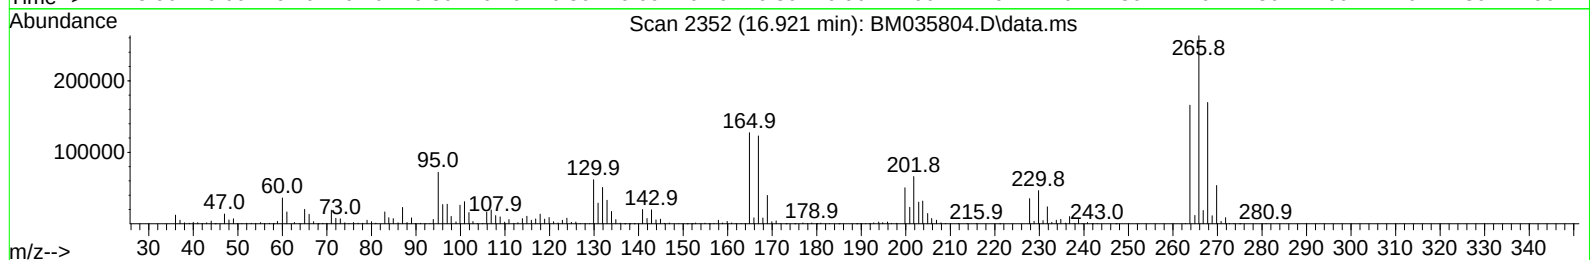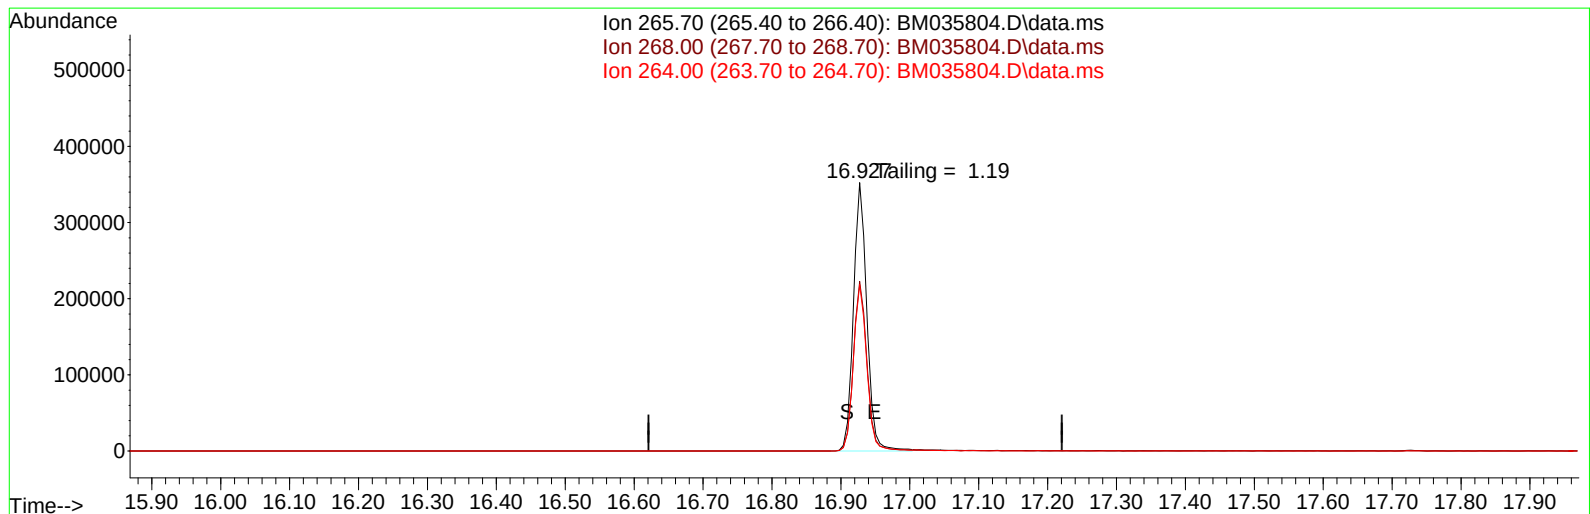

TIC: BM035804.D\data.ms

(70) Pentachlorophenol (C)

16.921min (-16.921) 0.00 ng




response 0

Ion	Exp%	Act%
265.70	100.00	0.00
268.00	64.90	0.00#
264.00	63.30	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071422\
 Data File : BM035804.D
 Acq On : 14 Jul 2022 09:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jul 15 05:38:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 14 01:21:21 2022
 Response via : Initial Calibration

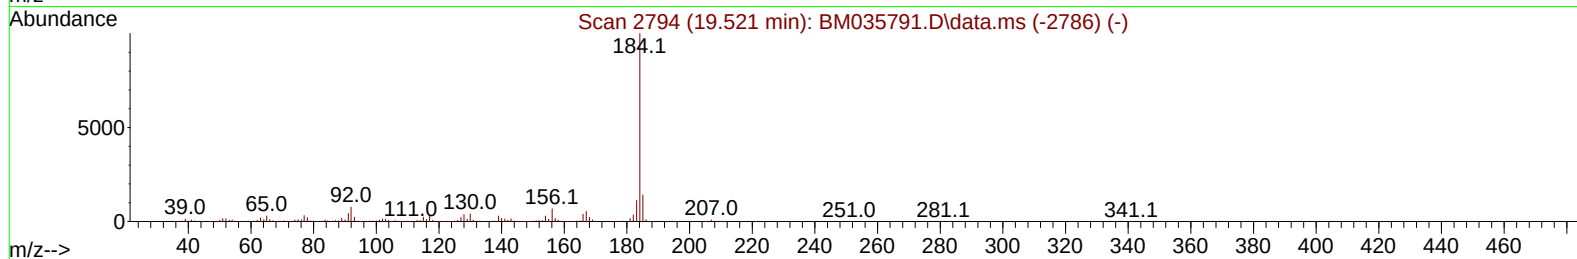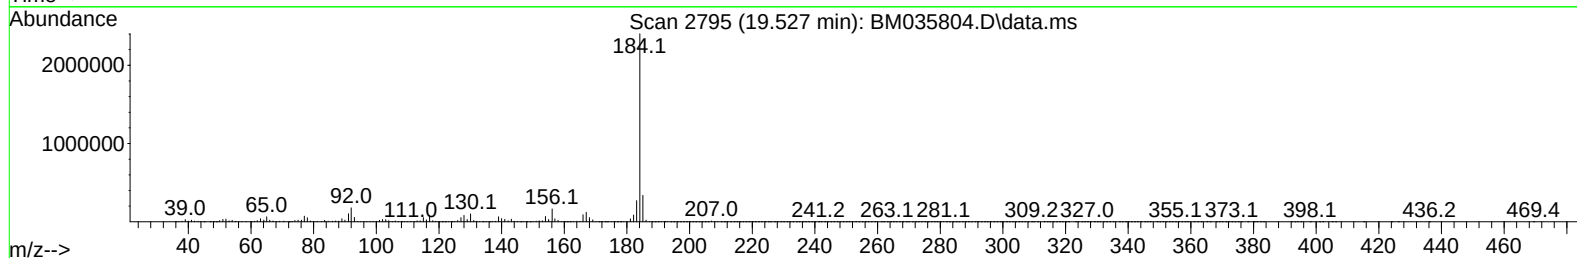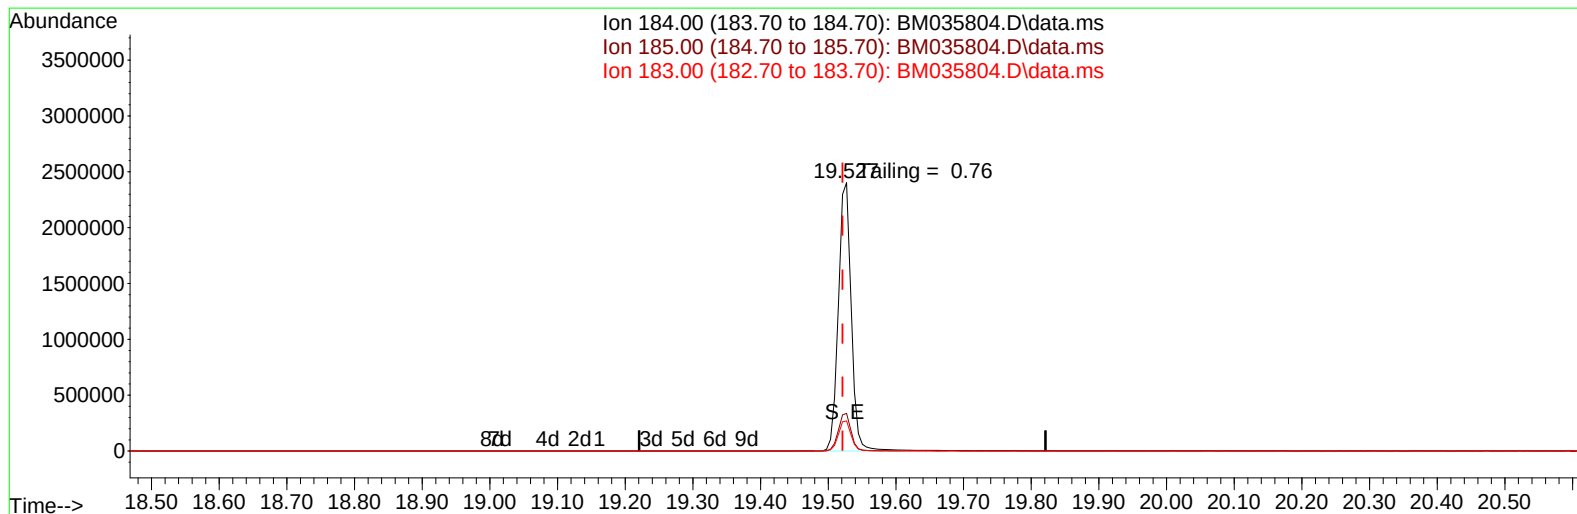

TIC: BM035804.D\data.ms

(77) Benzidine

19.527min (+ 0.006) 1102360.52 ng m

response 3179181

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.02
183.00	11.90	11.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/14/2022	BNA_M	<u>BM035804.D</u>
Compound Name	Response	Retention Time
DDT	1338941	20.756
DDD	19959	20.315
DDE	1235	19.809
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21194	1360135	1.56

Instrument :
BNA_M
ClientSampleId :
DFTPP