

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071525\
 Data File : BM050452.D
 Acq On : 15 Jul 2025 12:50
 Operator : RC/JU
 Sample : Q2489-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G2(0-6)

Quant Time: Jul 15 13:38:52 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 08 18:32:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	498520	20.000	ng	0.00
21) Naphthalene-d8	10.651	136	1816983	20.000	ng	-0.01
39) Acenaphthene-d10	14.481	164	1165990	20.000	ng	-0.01
64) Phenanthrene-d10	17.216	188	2348719	20.000	ng	-0.01
76) Chrysene-d12	21.433	240	2483396	20.000	ng	-0.02
86) Perylene-d12	24.462	264	2659318	20.000	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.434	112	1811175	62.537	ng	0.00
7) Phenol-d6	7.016	99	1378028	37.745	ng	0.00
23) Nitrobenzene-d5	9.010	82	2952957	82.914	ng	-0.01
42) 2,4,6-Tribromophenol	15.963	330	2240807	158.172	ng	-0.01
45) 2-Fluorobiphenyl	13.110	172	7694729	81.497	ng	-0.01
79) Terphenyl-d14	19.827	244	11820635	83.748	ng	-0.02
Target Compounds						
50) Dimethylphthalate	13.934	163	797621	9.936	ng	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071525\
Data File : BM050452.D
Acq On : 15 Jul 2025 12:50
Operator : RC/JU
Sample : Q2489-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G2(0-6)

Quant Time: Jul 15 13:38:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

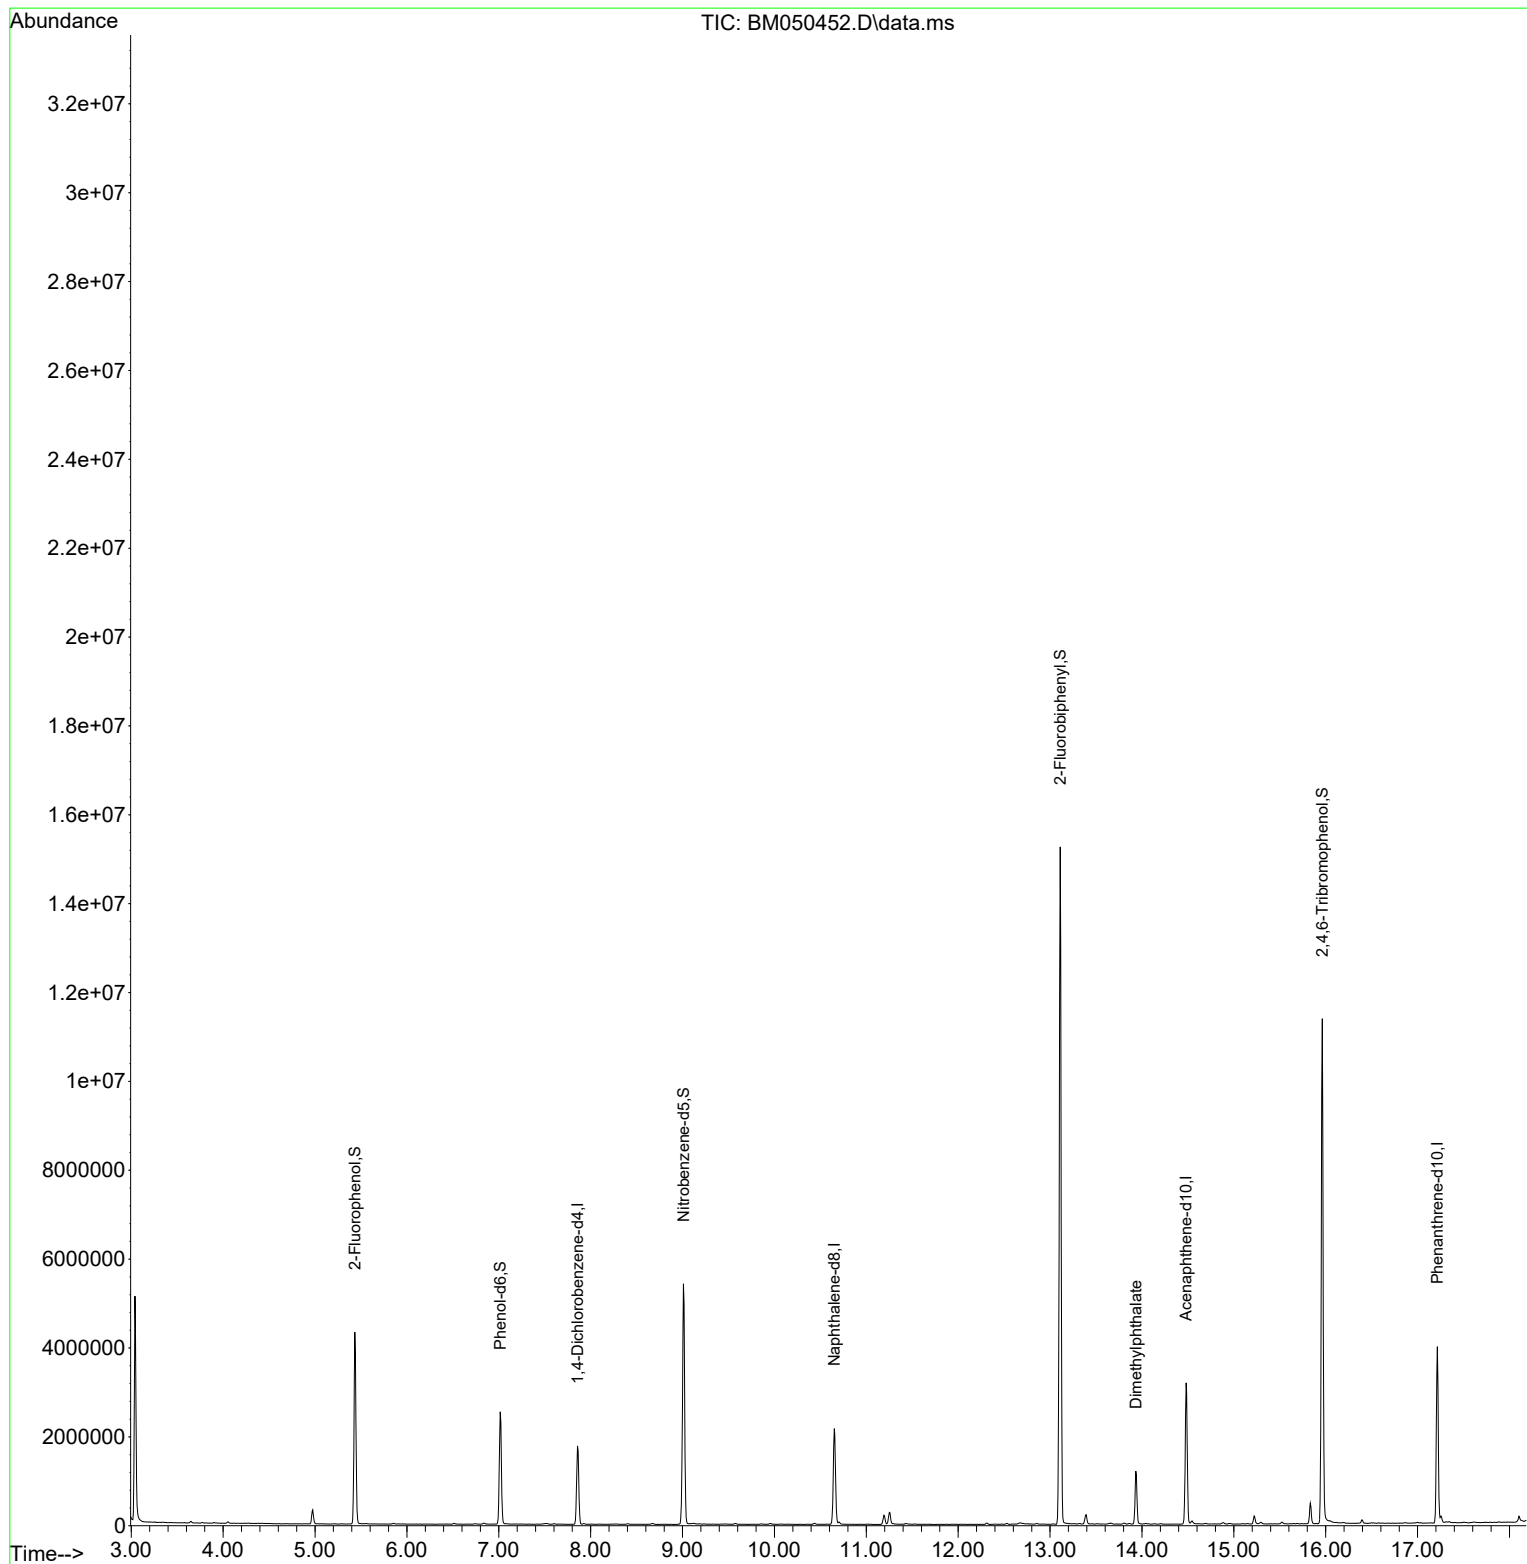

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071525\
Data File : BM050452.D
Acq On : 15 Jul 2025 12:50
Operator : RC/JU
Sample : Q2489-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G2(0-6)

Quant Time: Jul 15 13:38:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

