

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071525\
 Data File : BM050457.D
 Acq On : 15 Jul 2025 16:11
 Operator : RC/JU
 Sample : Q2489-04DL 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G3(6-12)DL

Quant Time: Jul 15 16:49:34 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 08 18:32:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	513226	20.000	ng	0.00
21) Naphthalene-d8	10.651	136	1868972	20.000	ng	-0.01
39) Acenaphthene-d10	14.480	164	1192981	20.000	ng	-0.01
64) Phenanthrene-d10	17.215	188	2410807	20.000	ng	-0.01
76) Chrysene-d12	21.433	240	2705442	20.000	ng	-0.02
86) Perylene-d12	24.462	264	3056124	20.000	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.434	112	167518	5.618	ng	0.00
7) Phenol-d6	7.016	99	121079	3.221	ng	0.00
23) Nitrobenzene-d5	9.010	82	267976	7.315	ng	-0.01
42) 2,4,6-Tribromophenol	15.963	330	184931	12.758	ng	-0.01
45) 2-Fluorobiphenyl	13.110	172	787192	8.149	ng	-0.01
79) Terphenyl-d14	19.827	244	1281629	8.335	ng	-0.02
Target Compounds						
84) Bis(2-ethylhexyl)phtha...	21.350	149	2675275	29.497	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071525\
Data File : BM050457.D
Acq On : 15 Jul 2025 16:11
Operator : RC/JU
Sample : Q2489-04DL 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G3(6-12)DL

Quant Time: Jul 15 16:49:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

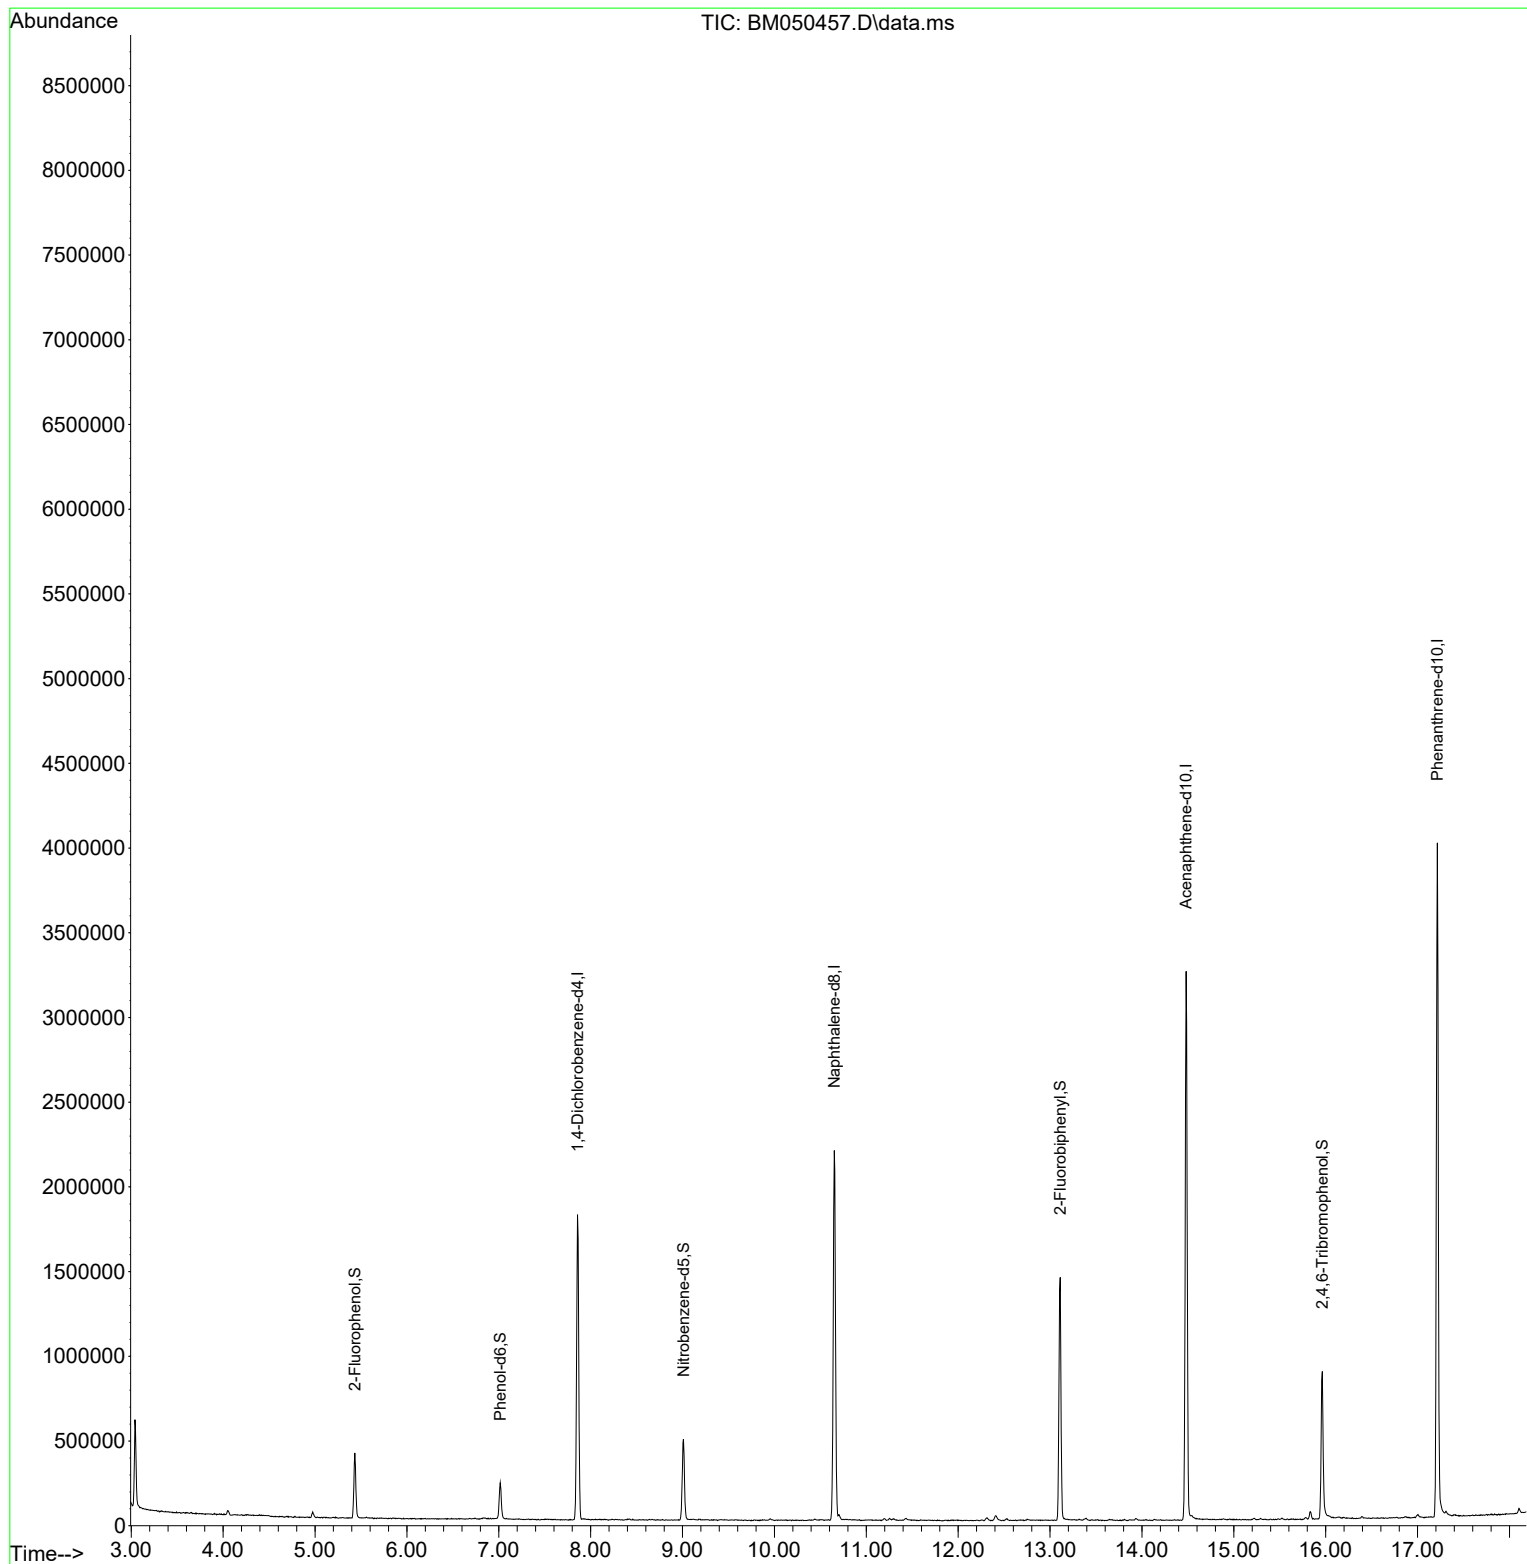

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071525\
Data File : BM050457.D
Acq On : 15 Jul 2025 16:11
Operator : RC/JU
Sample : Q2489-04DL 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G3(6-12)DL

Quant Time: Jul 15 16:49:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

