
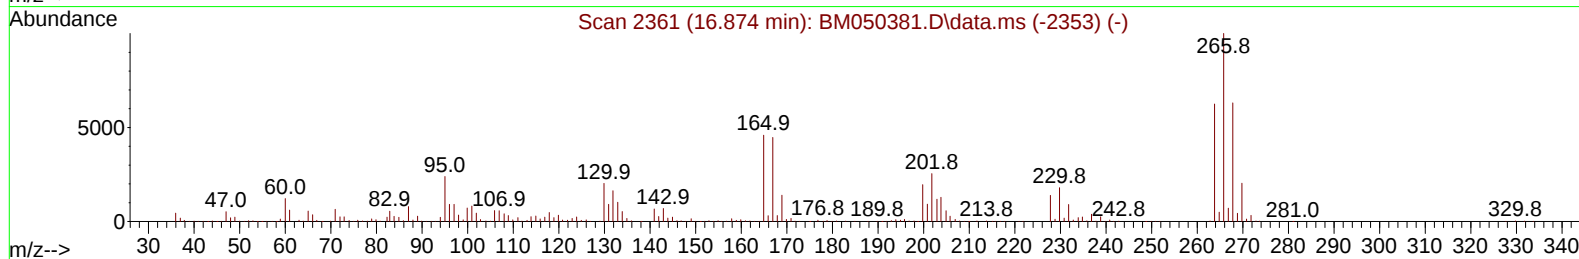
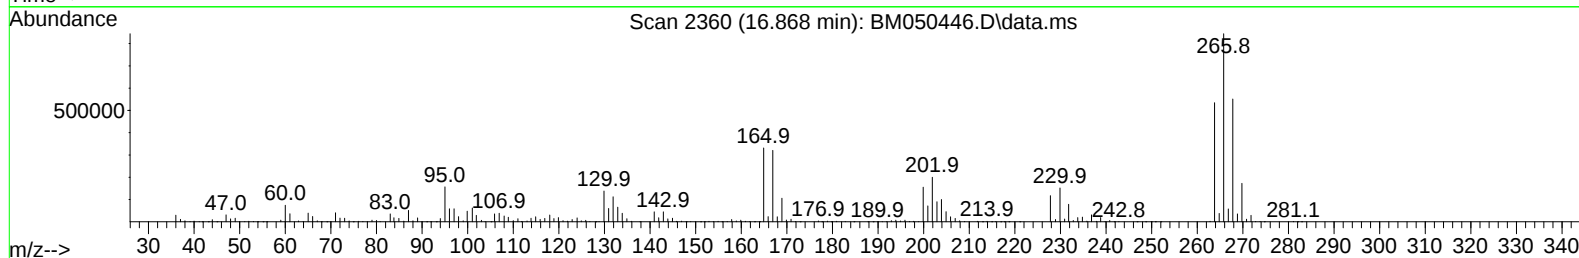


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071525\
Data File : BM050446.D
Acq On : 15 Jul 2025 08:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 10:52:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

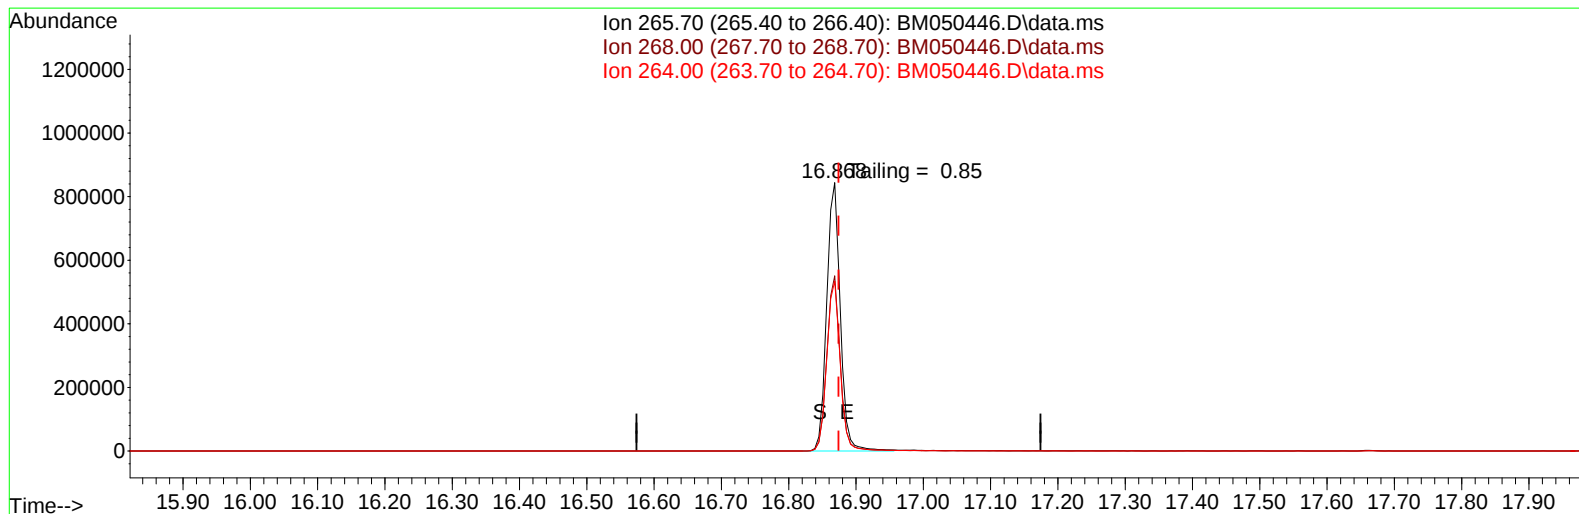

TIC: BM050446.D\data.ms

(70) Pentachlorophenol (C)




16.868min (-0.006) 502476.02 ng

response 1184472

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.29
264.00	62.40	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071525\
Data File : BM050446.D
Acq On : 15 Jul 2025 08:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 10:52:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

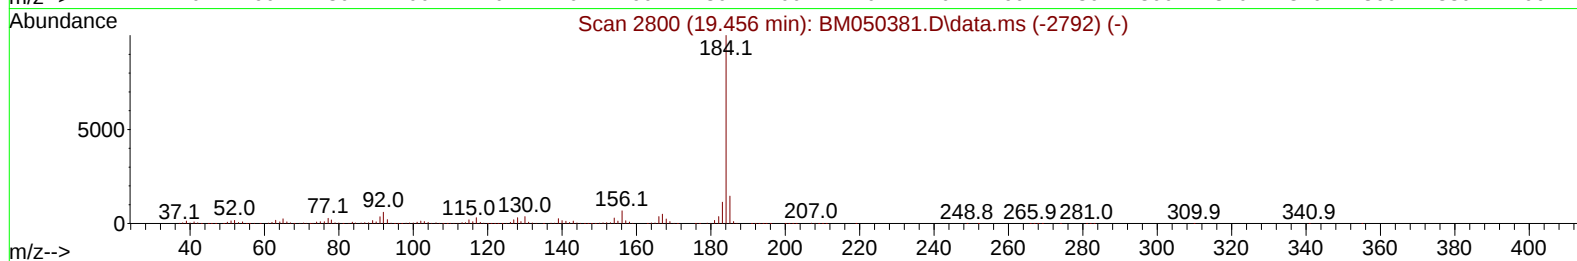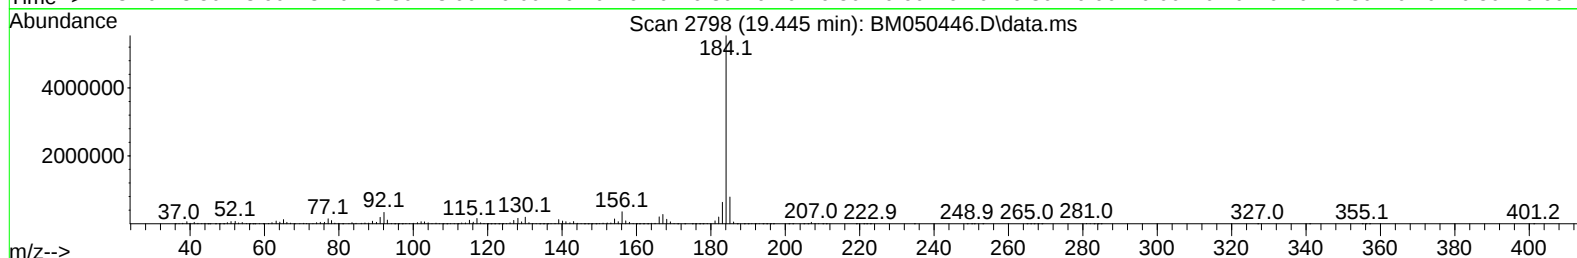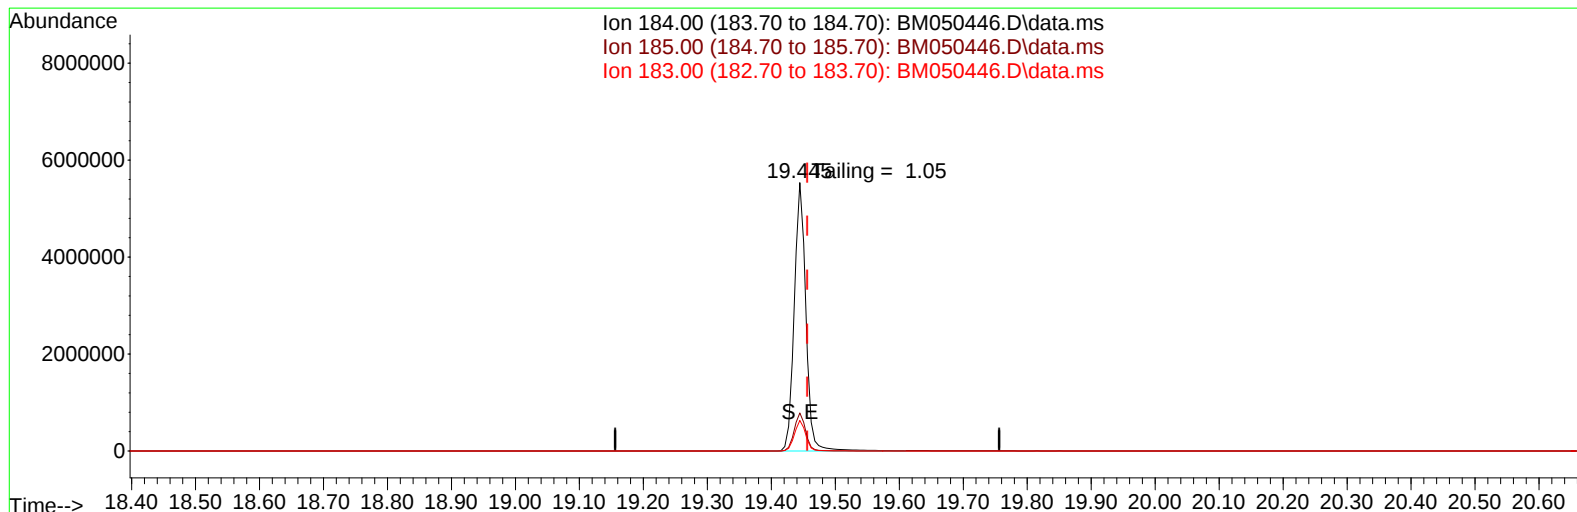

TIC: BM050446.D\data.ms

(77) Benzidine**19.445min (-0.012) 90011.87 ng****response 7016203**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.20
183.00	11.30	11.39
0.00	0.00	0.00