

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071525\
 Data File : BM050463.D
 Acq On : 15 Jul 2025 20:11
 Operator : RC/JU
 Sample : Q2586-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP-16

Quant Time: Jul 16 02:01:55 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 08 18:32:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	484044	20.000	ng	0.00
21) Naphthalene-d8	10.651	136	1711215	20.000	ng	-0.01
39) Acenaphthene-d10	14.480	164	1090948	20.000	ng	-0.01
64) Phenanthrene-d10	17.215	188	2280100	20.000	ng	-0.01
76) Chrysene-d12	21.433	240	2350387	20.000	ng	-0.02
86) Perylene-d12	24.462	264	2428164	20.000	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.434	112	3775223	134.252	ng	0.00
7) Phenol-d6	7.022	99	4458064	125.760	ng	0.00
23) Nitrobenzene-d5	9.010	82	2949809	87.945	ng	-0.01
42) 2,4,6-Tribromophenol	15.963	330	2215797	167.165	ng	-0.01
45) 2-Fluorobiphenyl	13.110	172	7528291	85.219	ng	-0.01
79) Terphenyl-d14	19.821	244	12229962	91.551	ng	-0.02


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071525\
Data File : BM050463.D
Acq On : 15 Jul 2025 20:11
Operator : RC/JU
Sample : Q2586-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-16


Quant Time: Jul 16 02:01:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

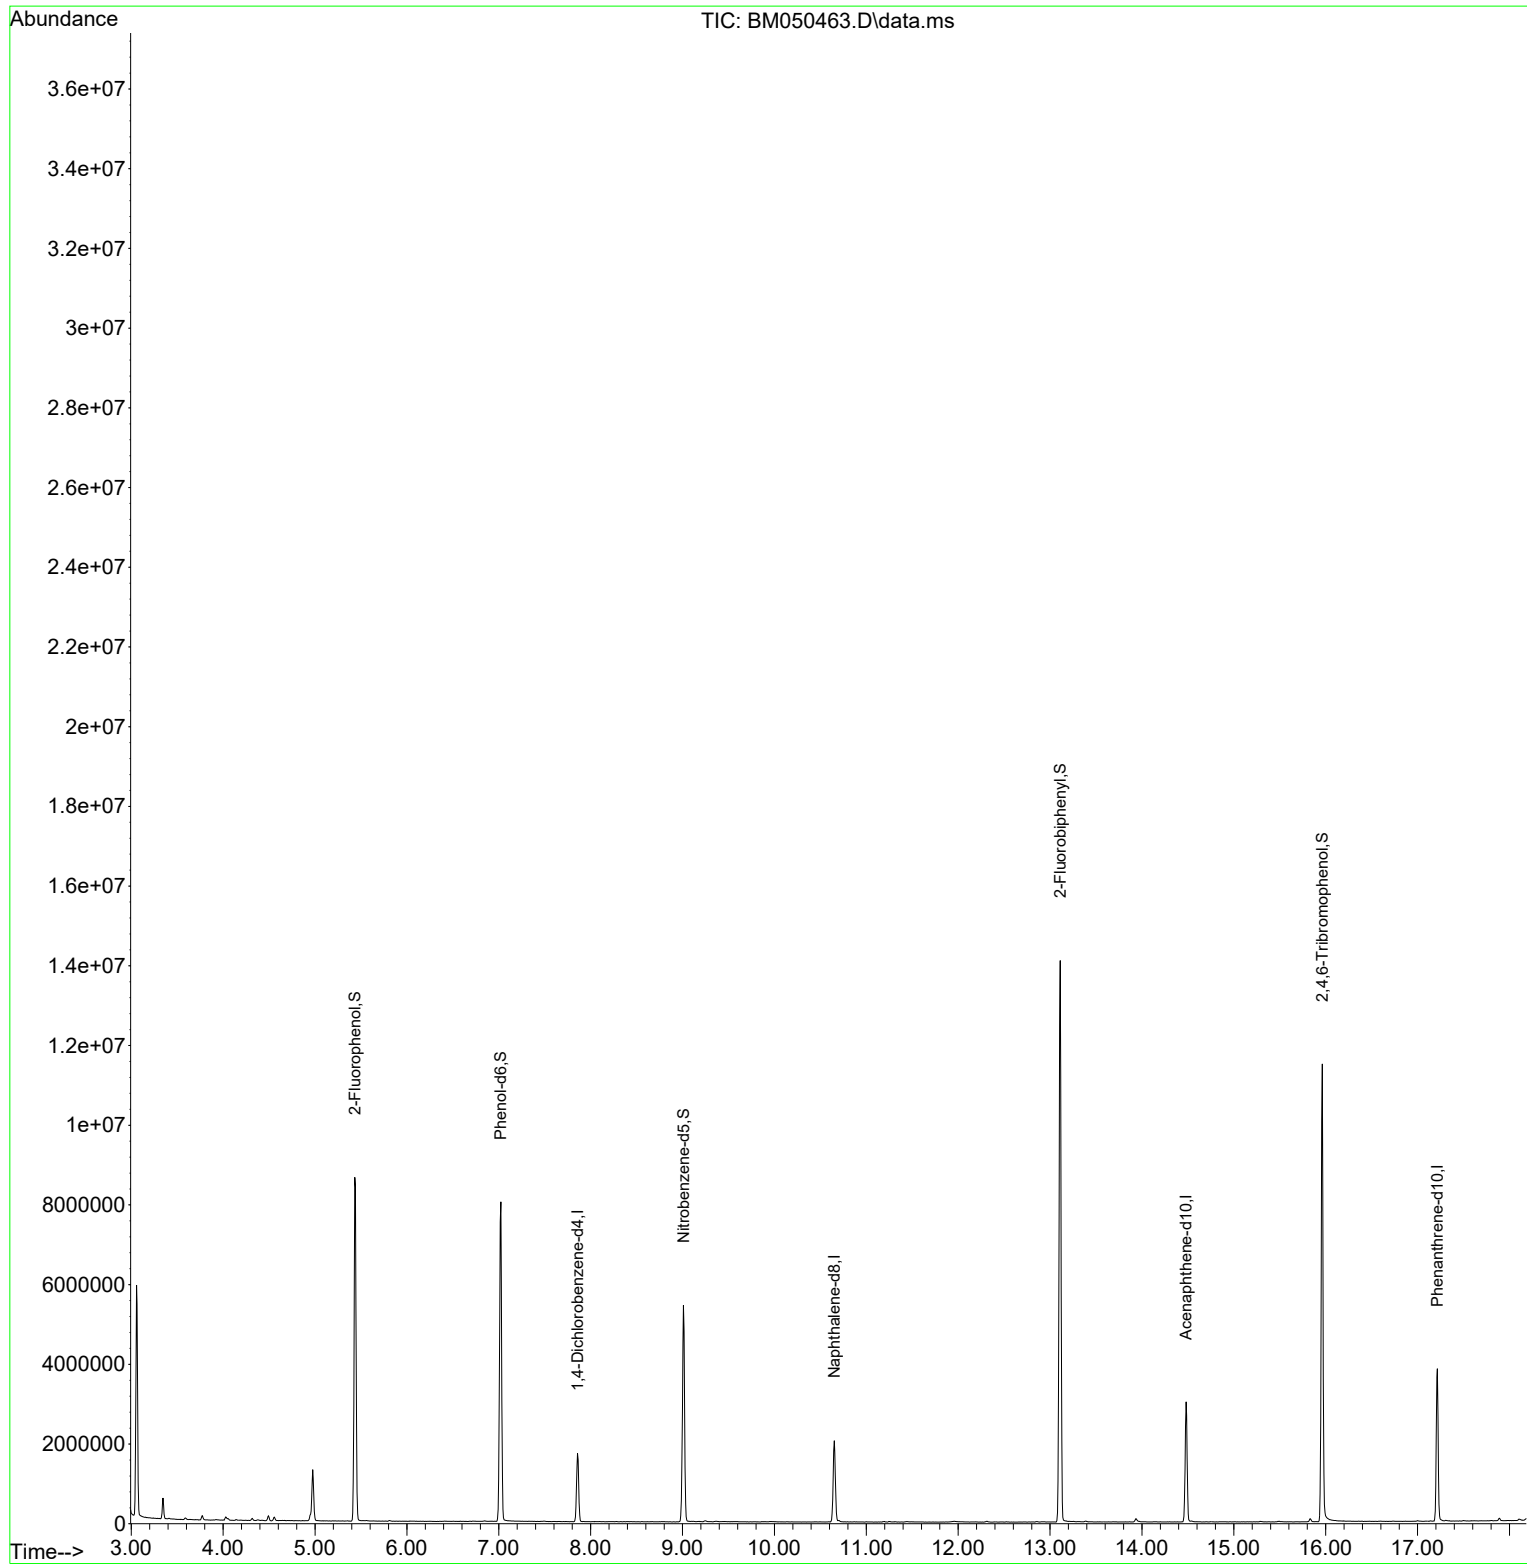


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071525\
Data File : BM050463.D
Acq On : 15 Jul 2025 20:11
Operator : RC/JU
Sample : Q2586-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-16

Quant Time: Jul 16 02:01:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration




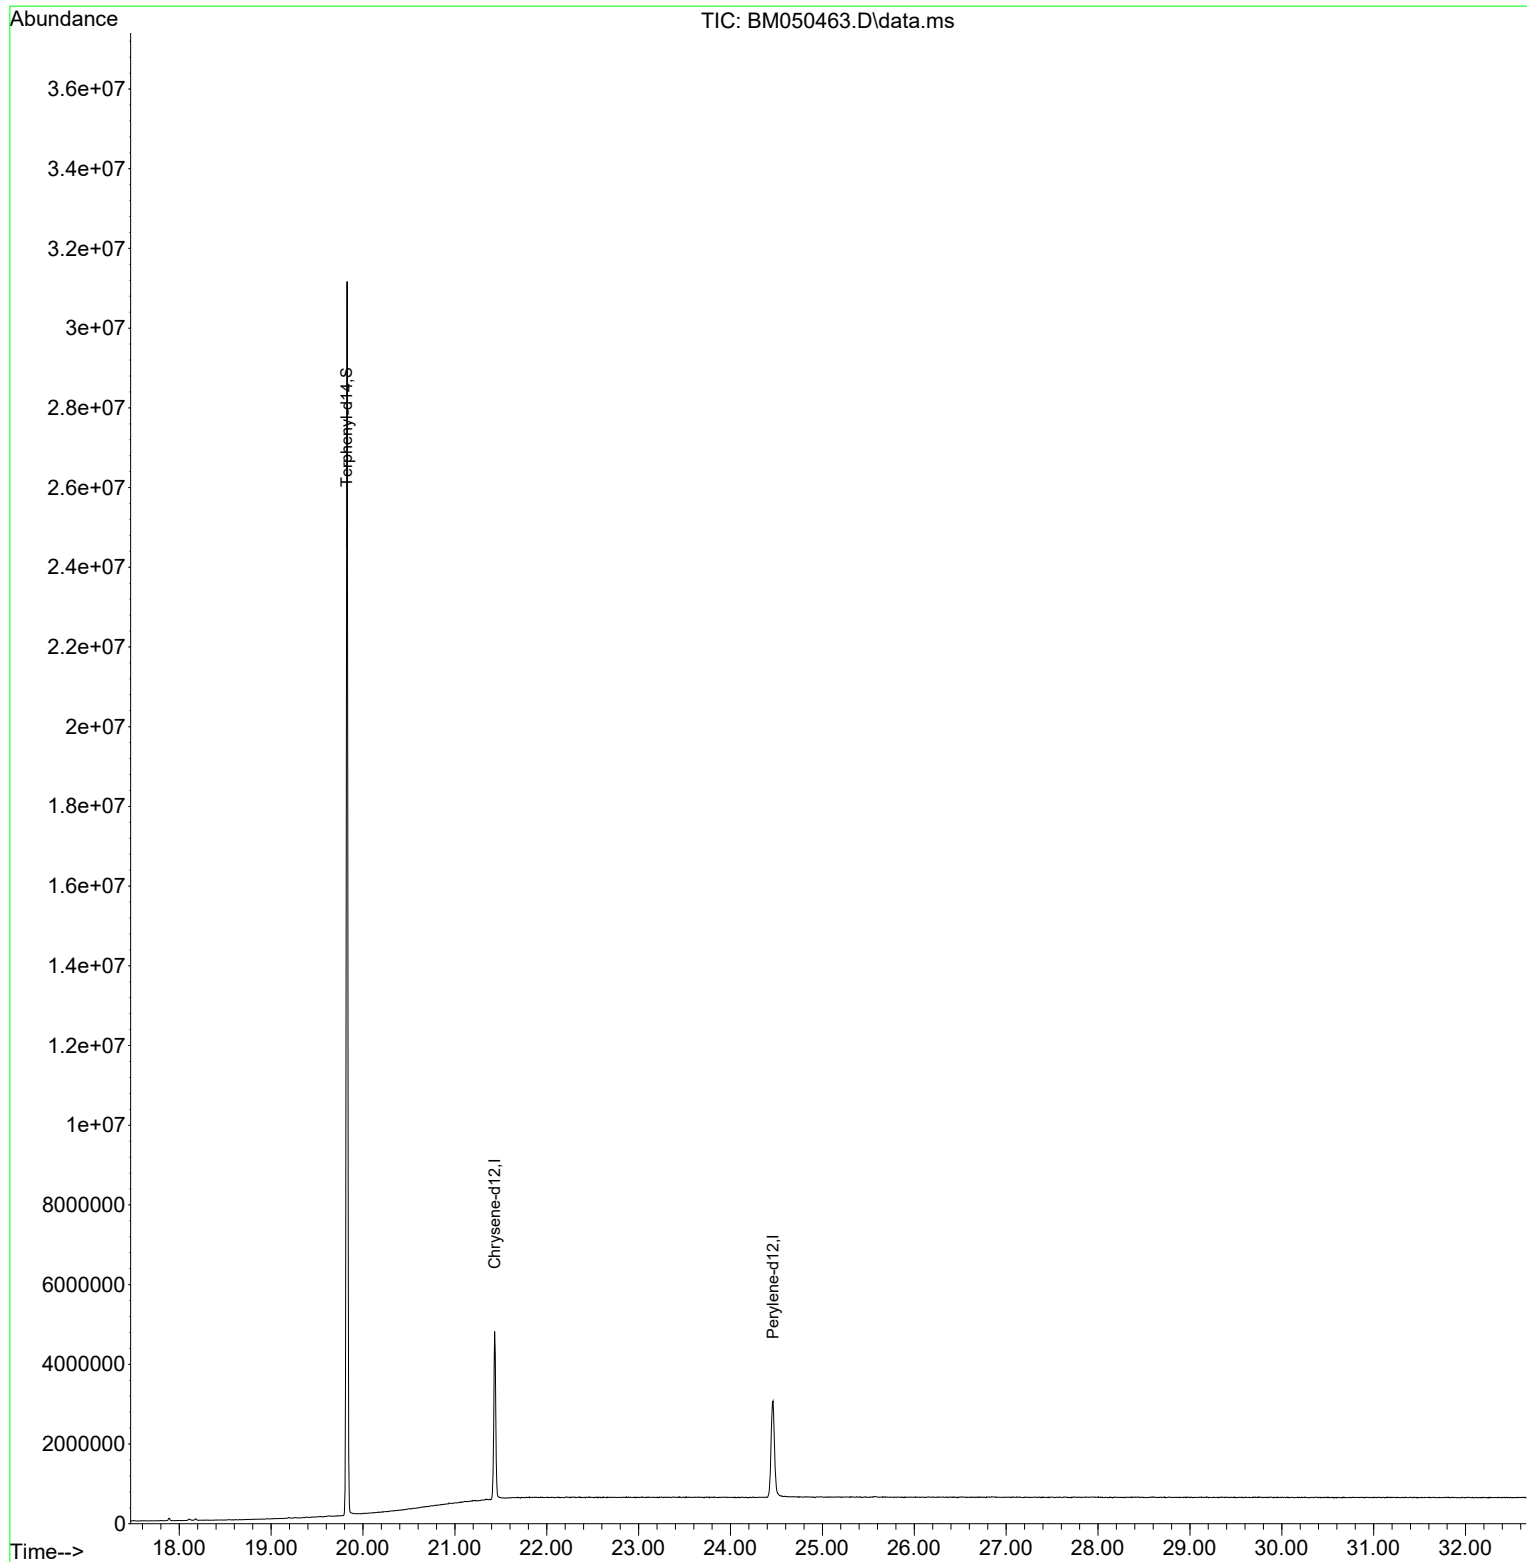


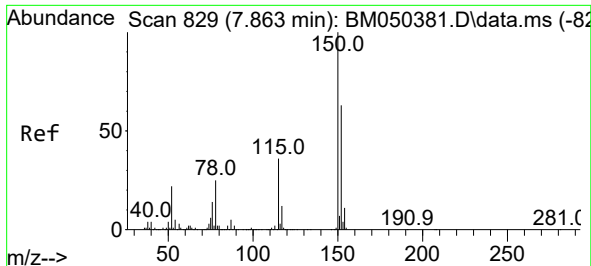

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.857 min Scan# 81
Delta R.T. -0.006 min
Lab File: BM050463.D
Acq: 15 Jul 2025 20:11




Instrument :
BNA_M
ClientSampleId :
TP-16


Tgt Ion:152 Resp: 484044
Ion Ratio Lower Upper
152 100
150 154.0 126.2 189.4
115 53.2 45.8 68.8

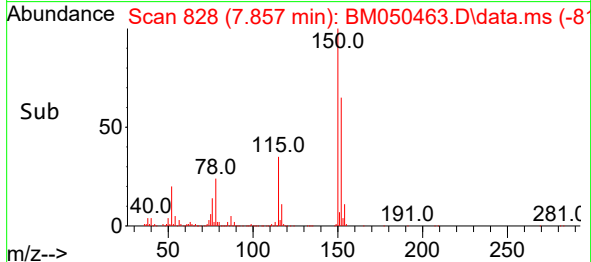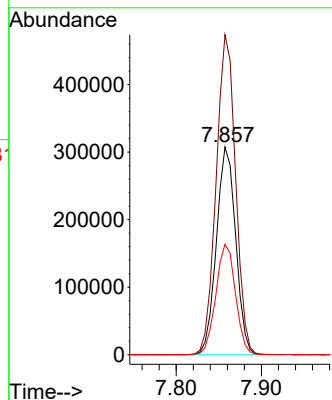

#5
2-Fluorophenol
Concen: 134.252 ng
RT: 5.434 min Scan# 416
Delta R.T. 0.000 min
Lab File: BM050463.D
Acq: 15 Jul 2025 20:11

Tgt Ion:112 Resp: 3775223
Ion Ratio Lower Upper
112 100
64 56.8 45.5 68.3
63 29.4 24.2 36.4


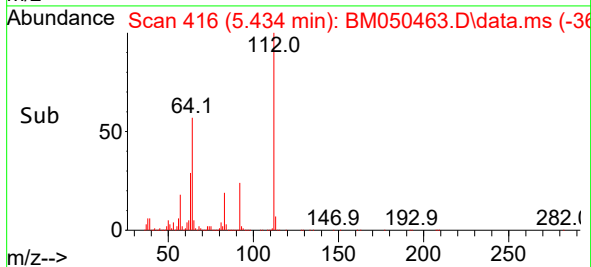
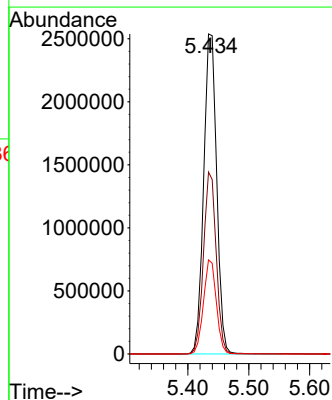
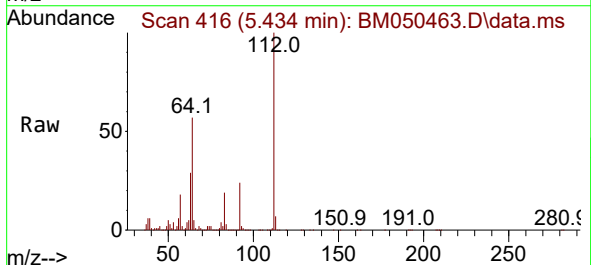


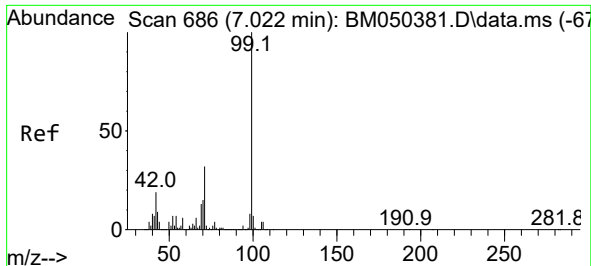

#7
Phenol-d6
Concen: 125.760 ng
RT: 7.022 min Scan# 686
Delta R.T. 0.000 min
Lab File: BM050463.D
Acq: 15 Jul 2025 20:11




Instrument :
BNA_M
ClientSampleId :
TP-16


Tgt Ion: 99 Resp: 4458064
Ion Ratio Lower Upper
99 100
42 17.7 15.0 22.6
71 31.4 25.9 38.9

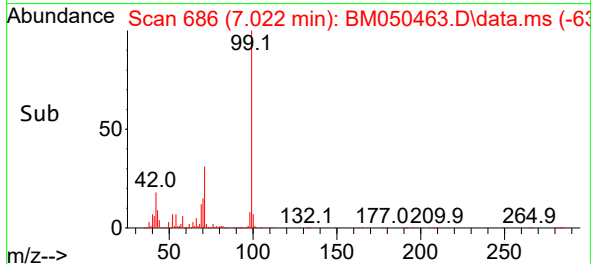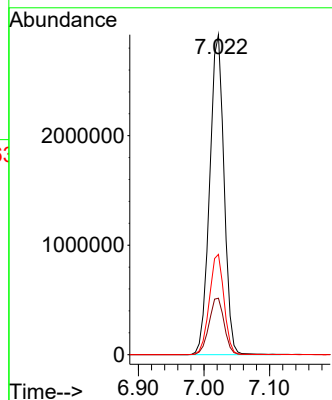

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.651 min Scan# 1303
Delta R.T. -0.012 min
Lab File: BM050463.D
Acq: 15 Jul 2025 20:11


Tgt Ion: 136 Resp: 1711215
Ion Ratio Lower Upper
136 100
137 11.1 8.8 13.2
54 7.8 6.3 9.5
68 5.1 4.2 6.2

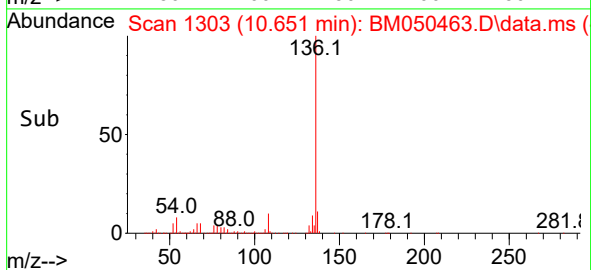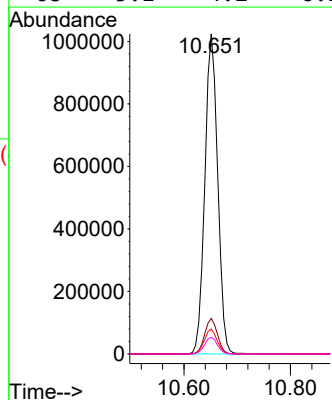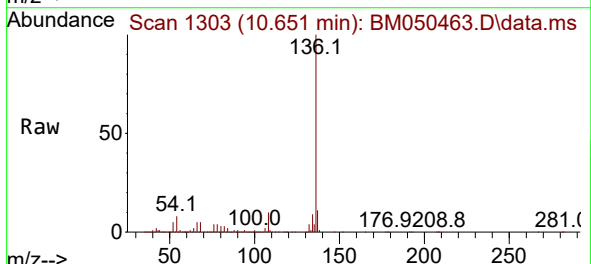

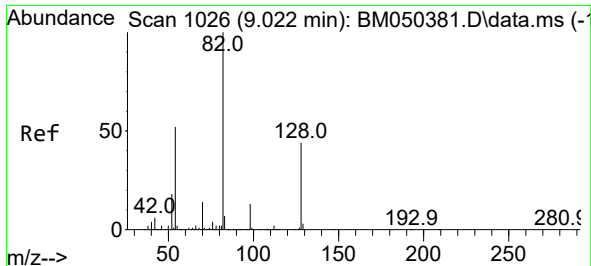




#23
Nitrobenzene-d5
Concen: 87.945 ng
RT: 9.010 min Scan# 1024
Delta R.T. -0.012 min
Lab File: BM050463.D
Acq: 15 Jul 2025 20:11

Instrument :
BNA_M
ClientSampleId :
TP-16



Tgt Ion: 82 Resp: 2949809




Ion	Ratio	Lower	Upper
82	100		
128	43.9	35.2	52.8
54	50.9	41.5	62.3

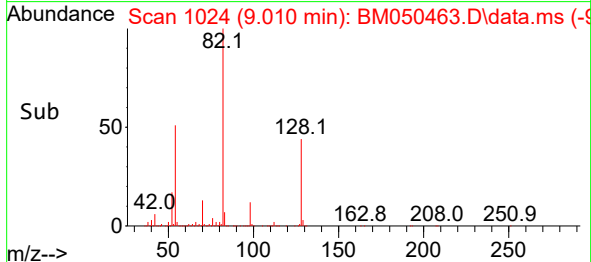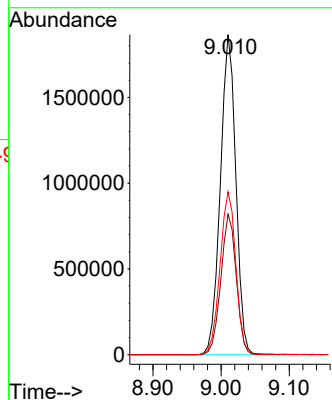


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.480 min Scan# 1954
Delta R.T. -0.012 min
Lab File: BM050463.D
Acq: 15 Jul 2025 20:11

Tgt Ion: 164 Resp: 1090948

Ion	Ratio	Lower	Upper
164	100		
162	99.3	79.9	119.9
160	44.7	36.2	54.4


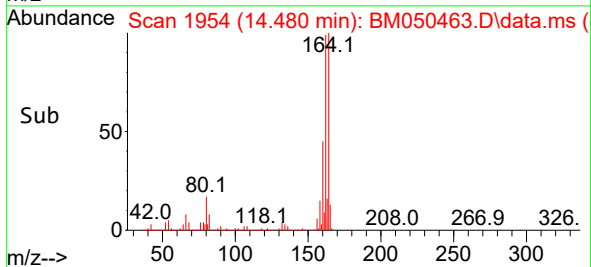
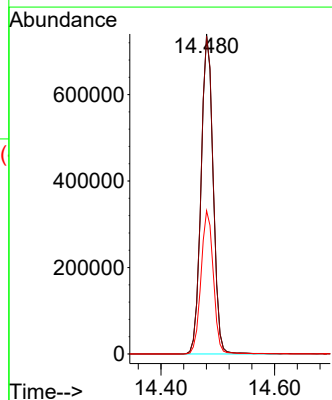
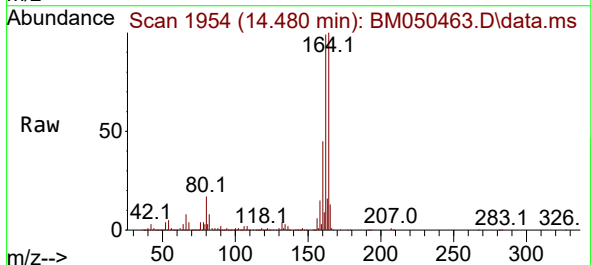


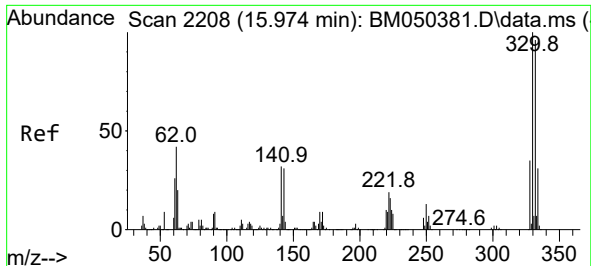

#42
2,4,6-Tribromophenol
Concen: 167.165 ng
RT: 15.963 min Scan# 21
Delta R.T. -0.012 min
Lab File: BM050463.D
Acq: 15 Jul 2025 20:11




Instrument :
BNA_M
ClientSampleId :
TP-16


Tgt Ion:330 Resp: 2215797
Ion Ratio Lower Upper
330 100
332 96.0 76.9 115.3
141 30.5 27.4 41.0

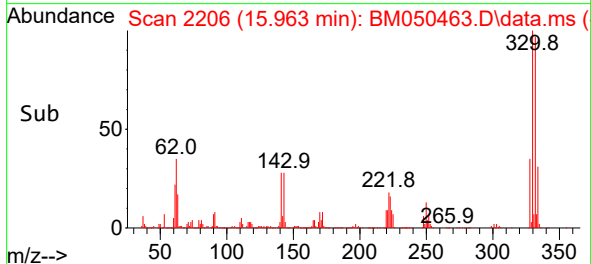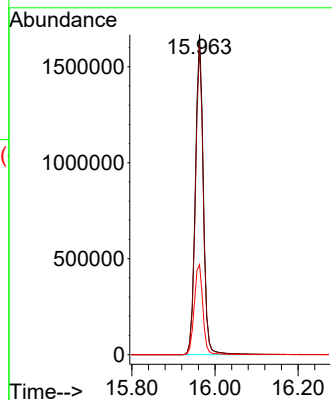

#45
2-Fluorobiphenyl
Concen: 85.219 ng
RT: 13.110 min Scan# 1721
Delta R.T. -0.012 min
Lab File: BM050463.D
Acq: 15 Jul 2025 20:11

Tgt Ion:172 Resp: 7528291
Ion Ratio Lower Upper
172 100
171 34.8 27.7 41.5
170 23.2 18.8 28.2

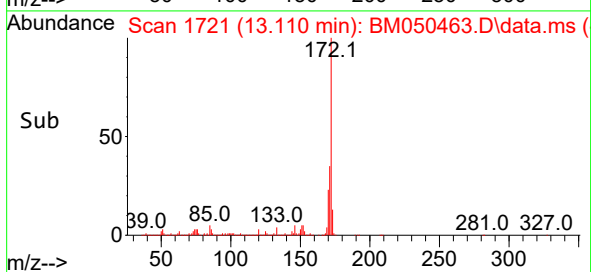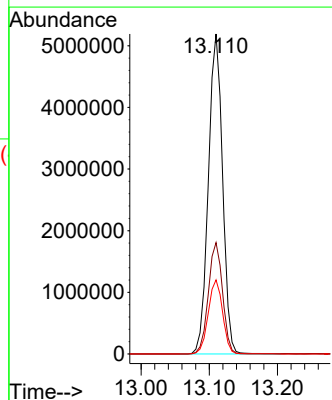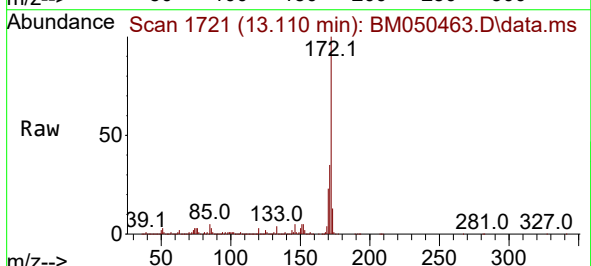



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.215 min Scan# 24

Delta R.T. -0.012 min

Lab File: BM050463.D

Acq: 15 Jul 2025 20:11

Instrument :

BNA_M

ClientSampleId :

TP-16





Tgt Ion:188 Resp: 2280100

Ion Ratio Lower Upper

188 100

94 7.5 6.0 9.0

80 7.8 6.5 9.7

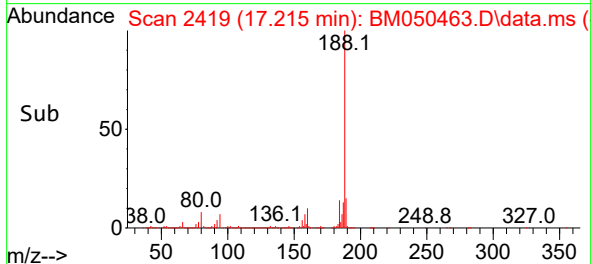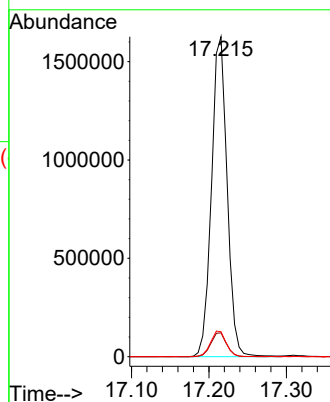

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.433 min Scan# 3136

Delta R.T. -0.023 min

Lab File: BM050463.D

Acq: 15 Jul 2025 20:11




Tgt Ion:240 Resp: 2350387


Ion Ratio Lower Upper

240 100

120 9.0 6.7 10.1

236 26.5 20.7 31.1

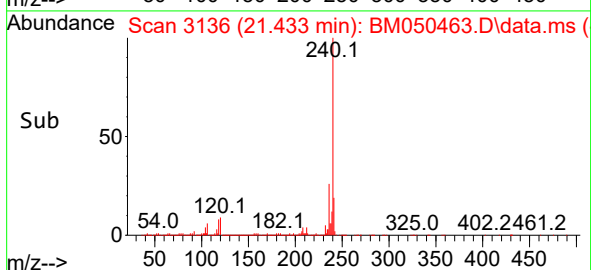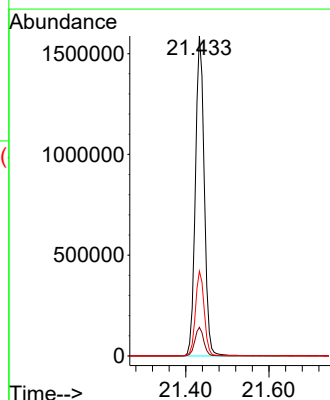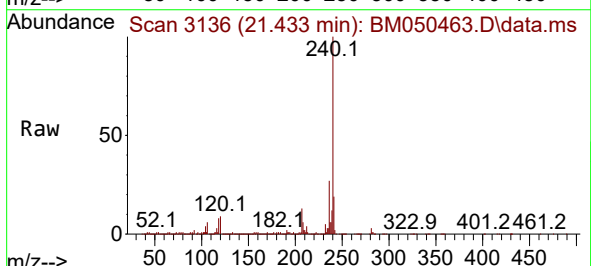



#79

Terphenyl-d14

Concen: 91.551 ng

RT: 19.821 min Scan# 21

Delta R.T. -0.023 min

Lab File: BM050463.D

Acq: 15 Jul 2025 20:11

Instrument :

BNA_M

ClientSampleId :

TP-16





Tgt Ion:244 Resp:12229962

Ion Ratio Lower Upper

244 100

212 8.0 5.7 8.5

122 10.2 6.2 9.2#

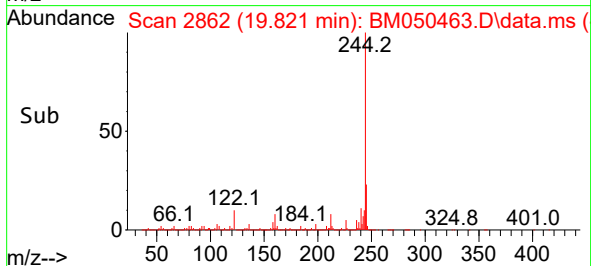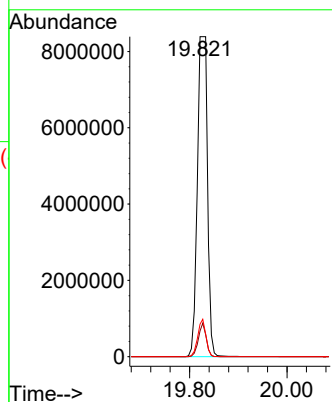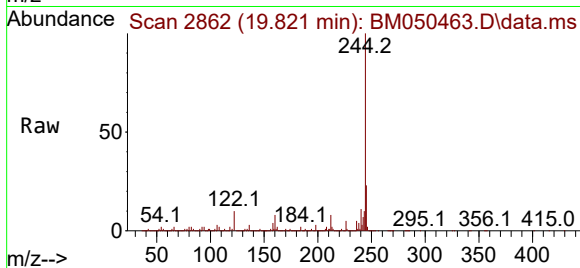

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.462 min Scan# 3651

Delta R.T. -0.035 min

Lab File: BM050463.D

Acq: 15 Jul 2025 20:11

Tgt Ion:264 Resp: 2428164

Ion Ratio Lower Upper

264 100

260 23.9 19.2 28.8

265 22.1 17.8 26.6

