
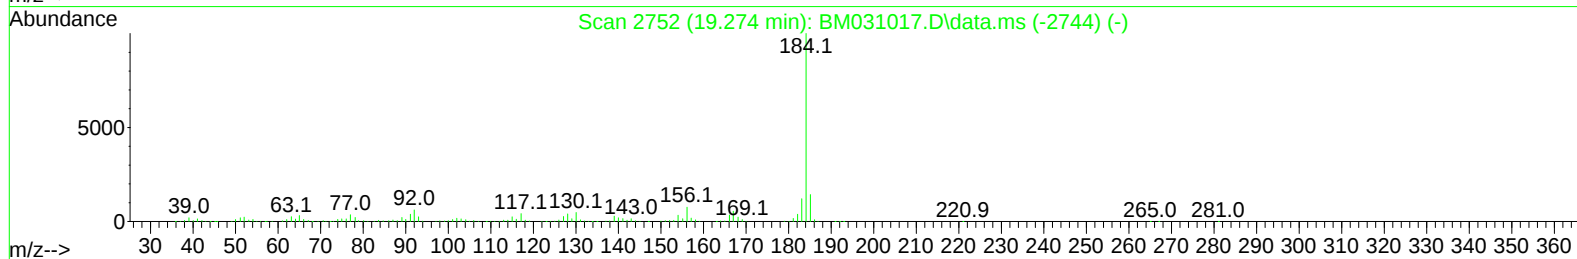
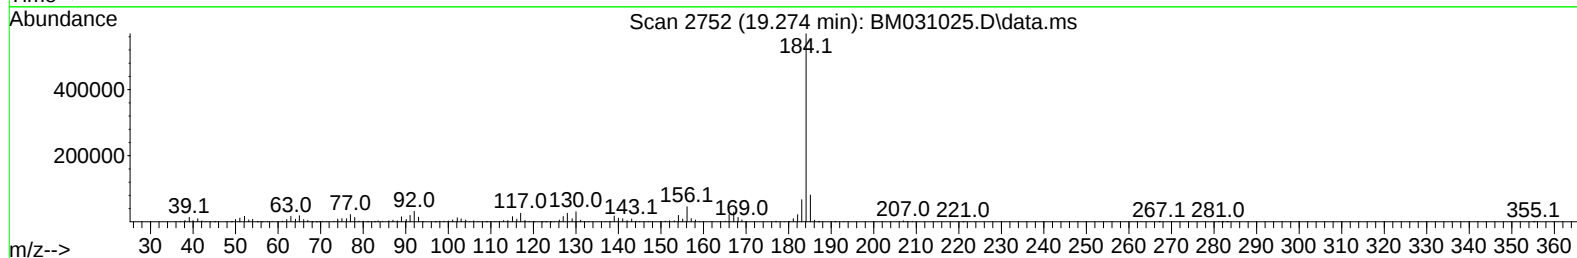


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072021\
Data File : BM031025.D
Acq On : 20 Jul 2021 16:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 17:15:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 20 13:21:40 2021
Response via : Initial Calibration

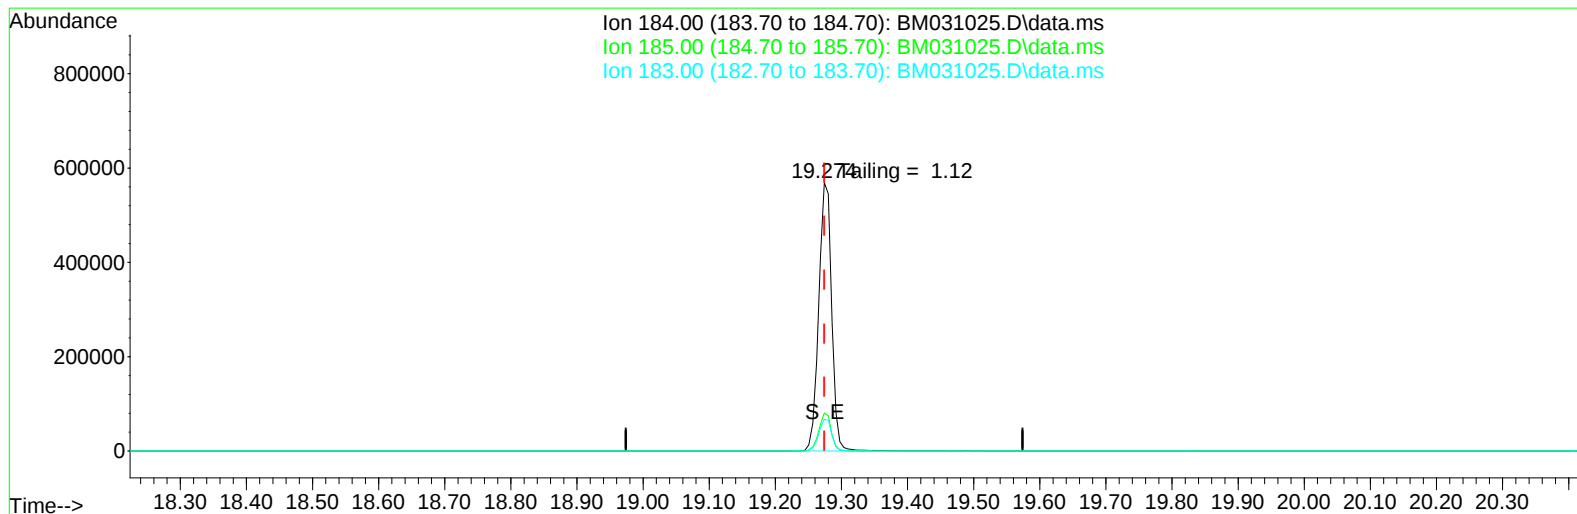

TIC: BM031025.D\data.ms

(77) Benzidine




19.274min (+ 0.000) 0.00 ng

response 773611

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.22
183.00	12.30	11.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072021\
 Data File : BM031025.D
 Acq On : 20 Jul 2021 16:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 17:15:44 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 20 13:21:40 2021
 Response via : Initial Calibration

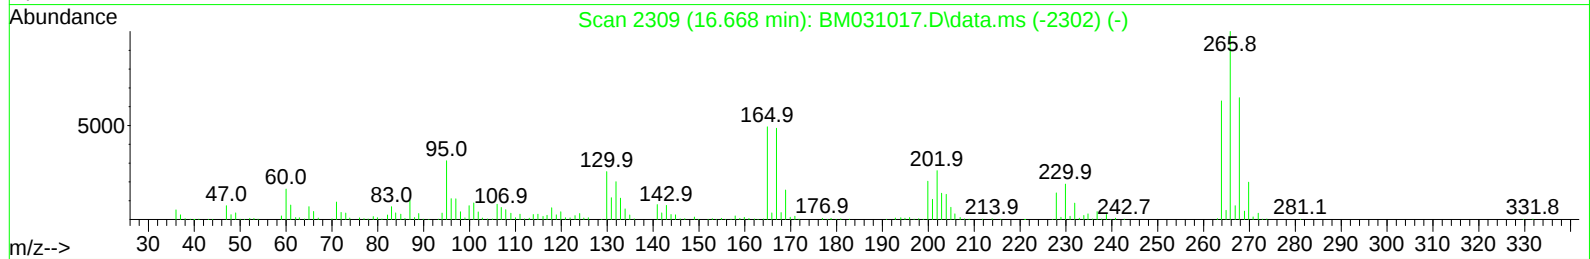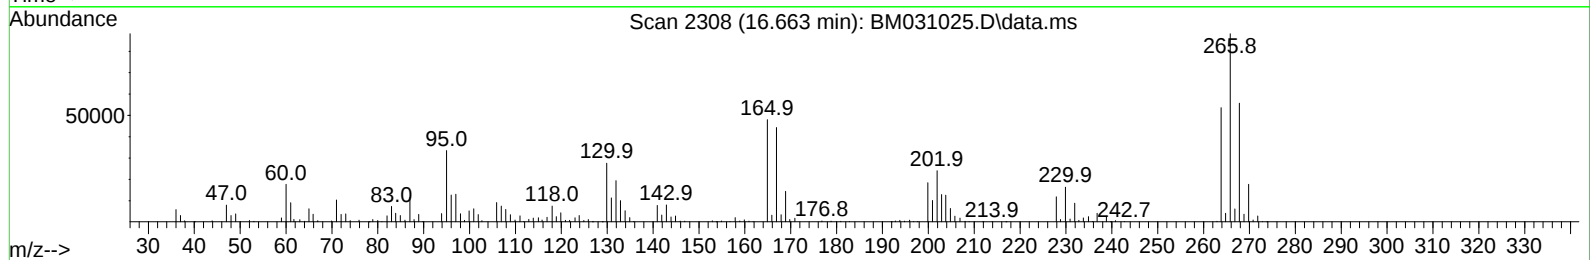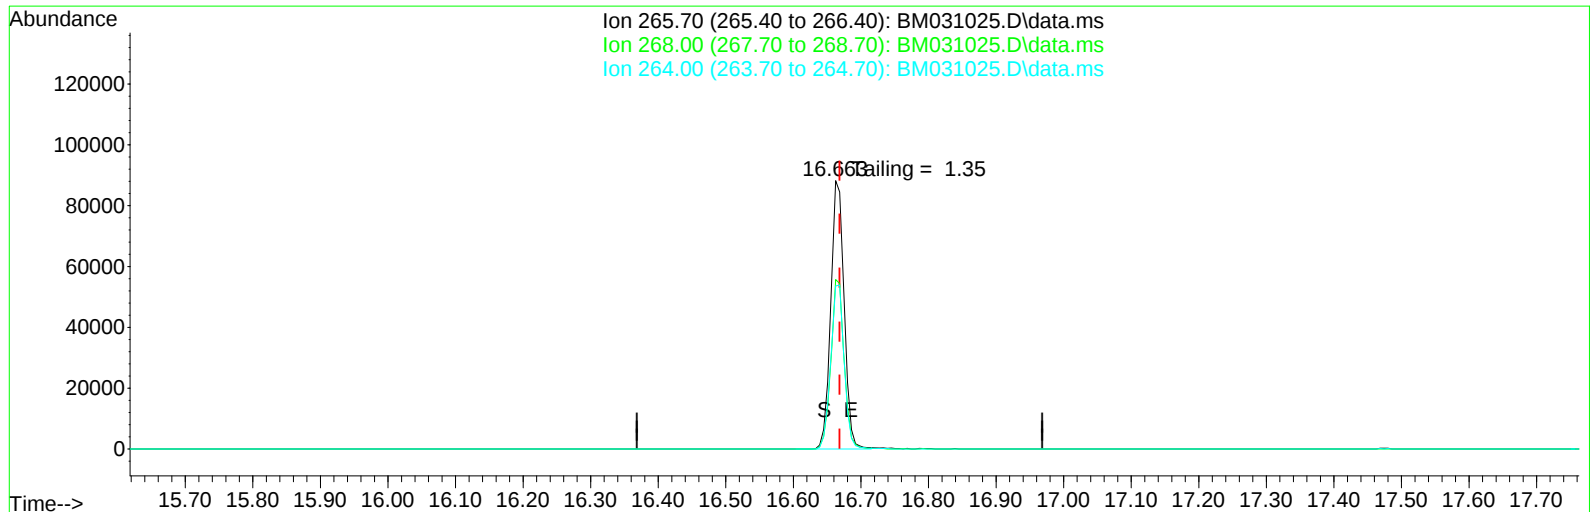

TIC: BM031025.D\data.ms

(70) Pentachlorophenol (C)

16.663min (-0.006) 0.00 ng

response 122320

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	63.13
264.00	64.90	60.74
0.00	0.00	0.00