

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072021\
 Data File : BM031027.D
 Acq On : 20 Jul 2021 17:46
 Operator : CG/JU
 Sample : PB137646BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB137646BL

Quant Time: Jul 20 18:21:46 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 20 13:21:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	71281	20.000	ng	0.00
21) Naphthalene-d8	10.404	136	306229	20.000	ng	# 0.00
39) Acenaphthene-d10	14.268	164	214802	20.000	ng	0.00
64) Phenanthrene-d10	17.015	188	484293	20.000	ng	0.00
76) Chrysene-d12	21.203	240	526169	20.000	ng	0.00
86) Perylene-d12	23.380	264	550907	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.263	112	647650	163.155	ng	0.00
7) Phenol-d6	6.822	99	840963	146.143	ng	0.00
23) Nitrobenzene-d5	8.786	82	541287	88.750	ng	0.00
42) 2,4,6-Tribromophenol	15.762	330	362656	129.292	ng	0.00
45) 2-Fluorobiphenyl	12.886	172	1275484	88.598	ng	0.00
79) Terphenyl-d14	19.656	244	2567015	96.527	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072021\
Data File : BM031027.D
Acq On : 20 Jul 2021 17:46
Operator : CG/JU
Sample : PB137646BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB137646BL

Quant Time: Jul 20 18:21:46 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 20 13:21:40 2021
Response via : Initial Calibration




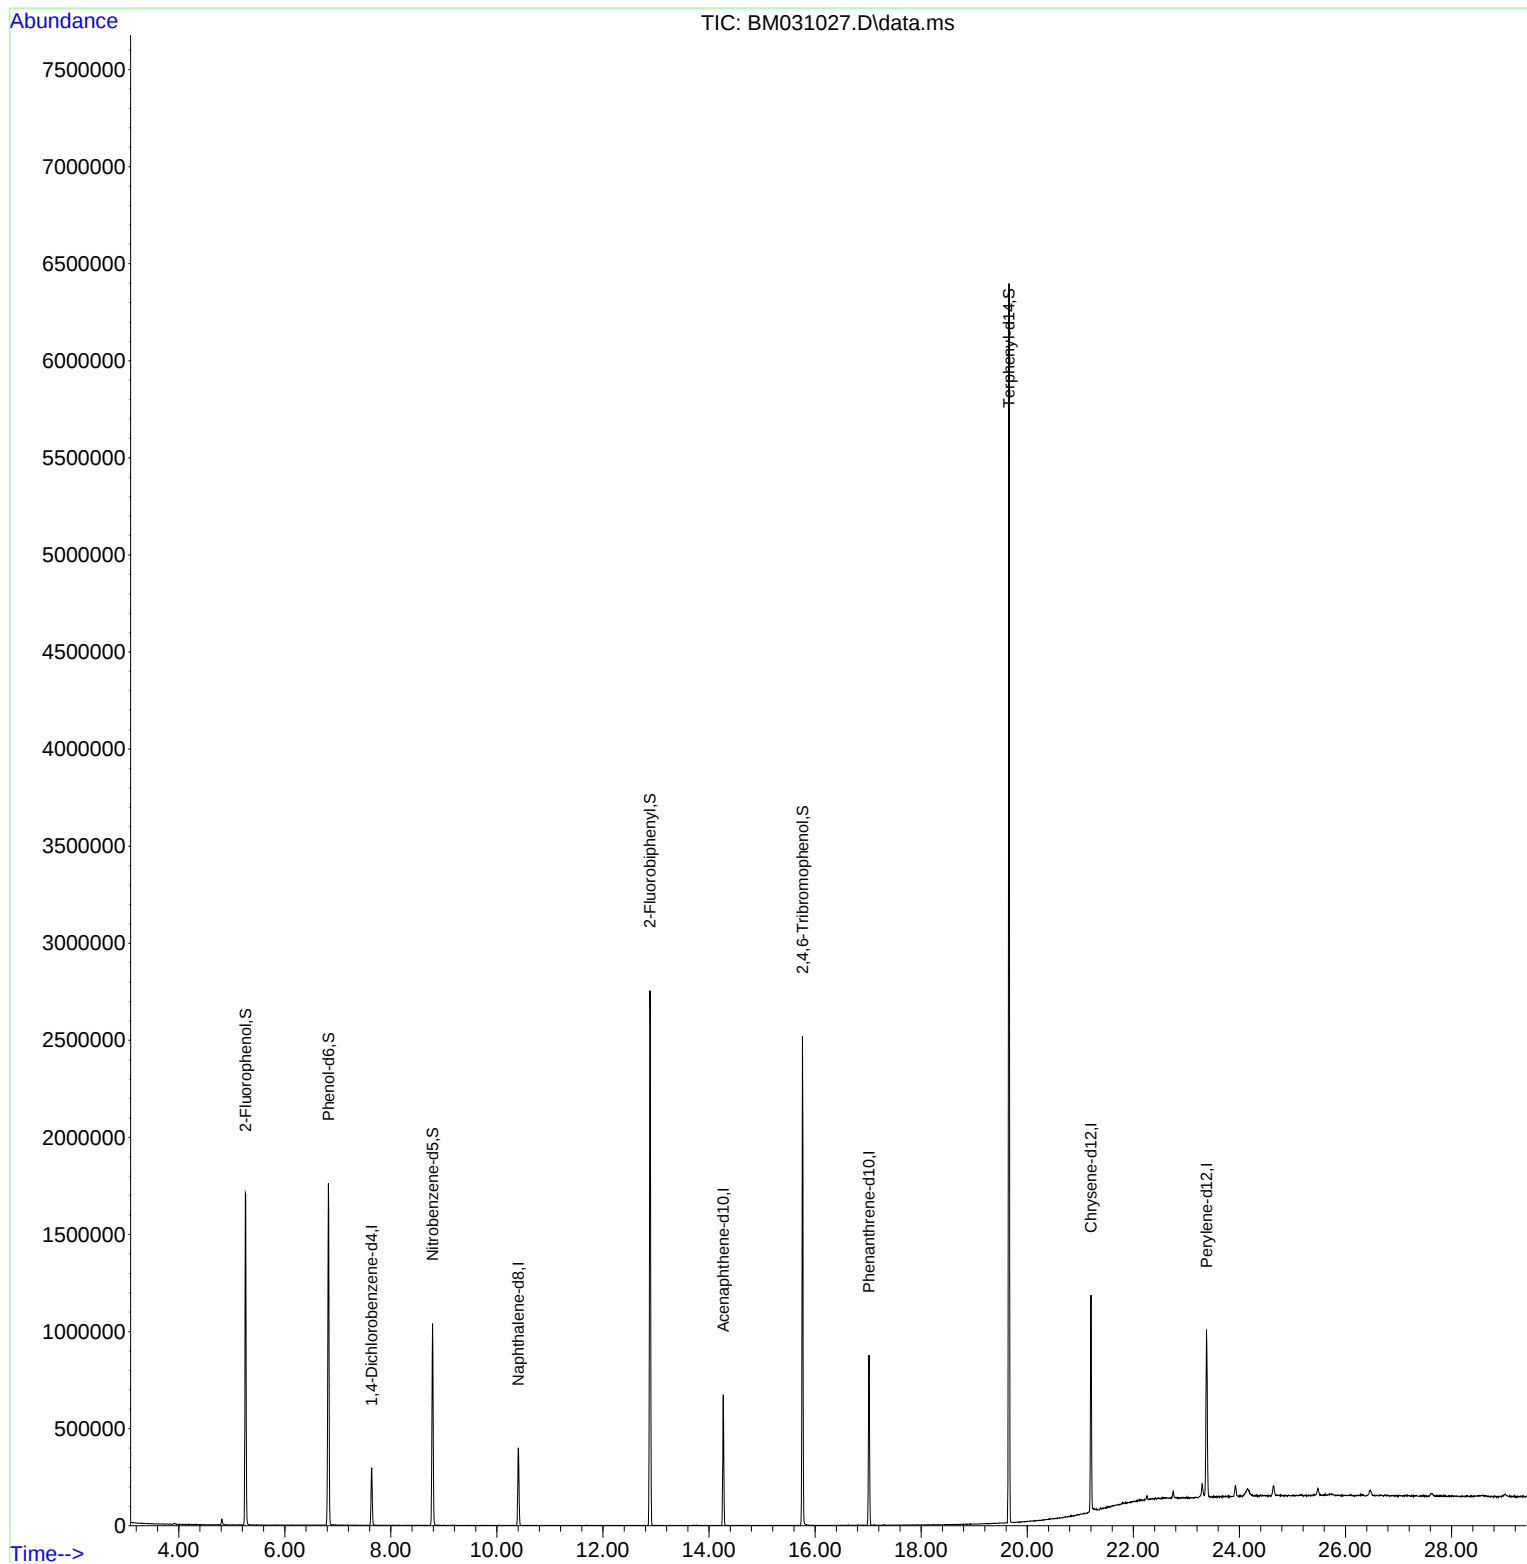




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.640 min Scan# 774
Delta R.T. 0.000 min
Lab File: BM031027.D
Acq: 20 Jul 2021 17:46




Instrument :
BNA_M
ClientSampleId :
PB137646BL


Tgt Ion:152 Resp: 71281
Ion Ratio Lower Upper
152 100
150 149.1 125.9 188.9
115 59.5 44.6 67.0

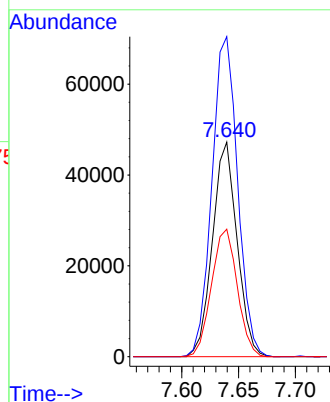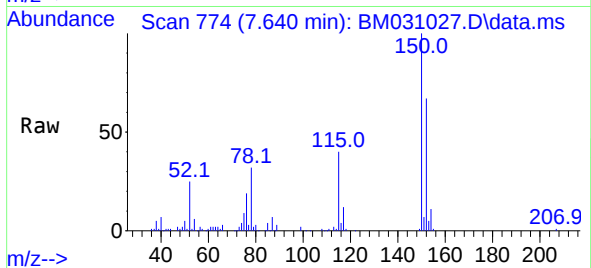

#5
2-Fluorophenol
Concen: 163.155 ng
RT: 5.263 min Scan# 370
Delta R.T. 0.006 min
Lab File: BM031027.D
Acq: 20 Jul 2021 17:46

Tgt Ion:112 Resp: 647650
Ion Ratio Lower Upper
112 100
64 56.8 47.1 70.7
63 34.8 27.3 40.9

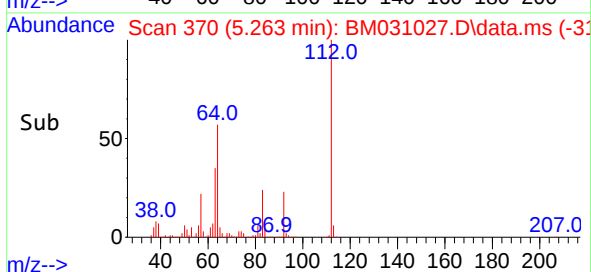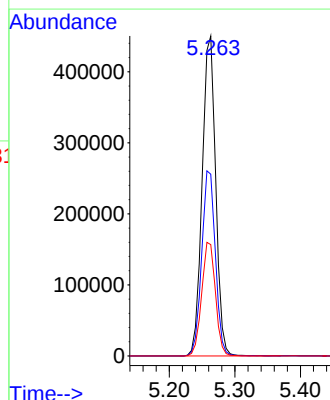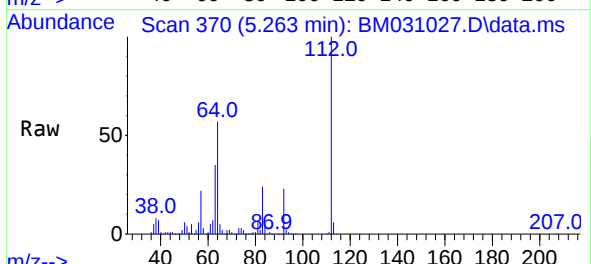







#7
Phenol-d6
Concen: 146.143 ng
RT: 6.822 min Scan# 635
Delta R.T. 0.000 min
Lab File: BM031027.D
Acq: 20 Jul 2021 17:46

Instrument :
BNA_M
ClientSampleId :
PB137646BL

Tgt Ion: 99 Resp: 840963




Ion	Ratio	Lower	Upper
99	100		
42	23.9	18.0	27.0
71	43.7	30.9	46.3

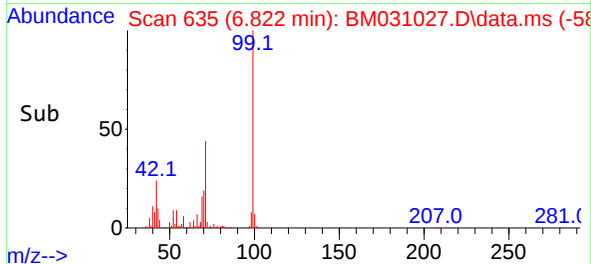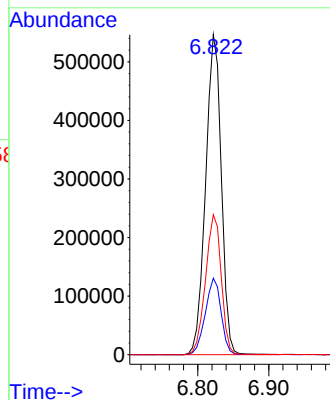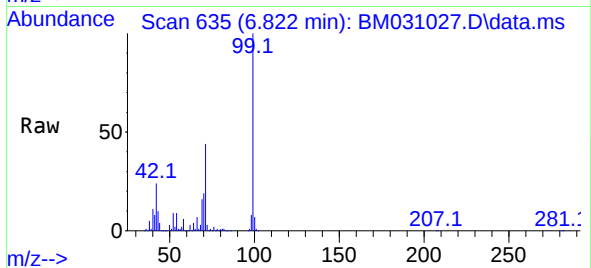


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.404 min Scan# 1244
Delta R.T. -0.006 min
Lab File: BM031027.D
Acq: 20 Jul 2021 17:46

Tgt Ion: 136 Resp: 306229

Ion	Ratio	Lower	Upper
136	100		
137	10.2	8.4	12.6
54	7.7	5.5	8.3
68	4.1	4.2	6.2

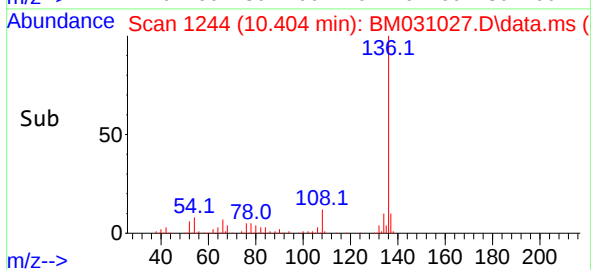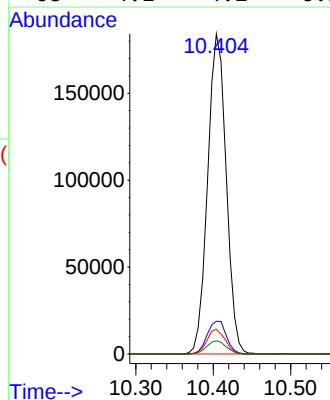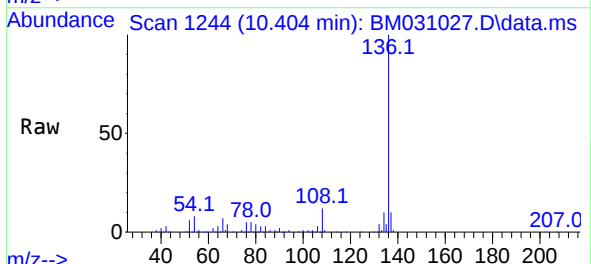







#23
Nitrobenzene-d5
Concen: 88.750 ng
RT: 8.786 min Scan# 969
Delta R.T. -0.006 min
Lab File: BM031027.D
Acq: 20 Jul 2021 17:46

Instrument :
BNA_M
ClientSampleId :
PB137646BL

Tgt Ion: 82 Resp: 541287




Ion	Ratio	Lower	Upper
82	100		
128	38.3	31.1	46.7
54	53.3	37.3	55.9

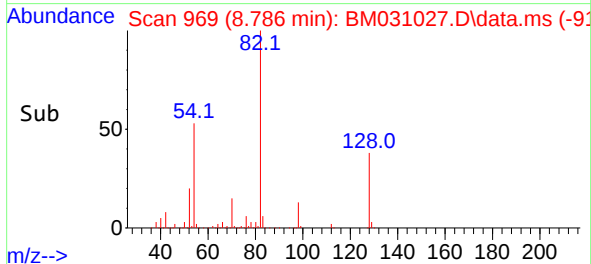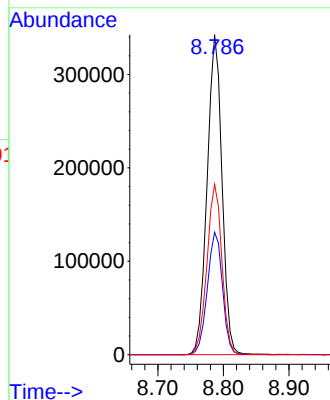


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.268 min Scan# 1901
Delta R.T. -0.006 min
Lab File: BM031027.D
Acq: 20 Jul 2021 17:46

Tgt Ion: 164 Resp: 214802

Ion	Ratio	Lower	Upper
164	100		
162	103.1	83.4	125.0
160	45.1	37.2	55.8


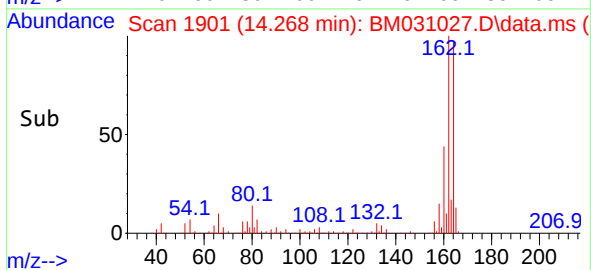
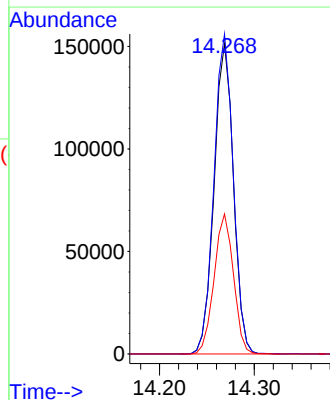
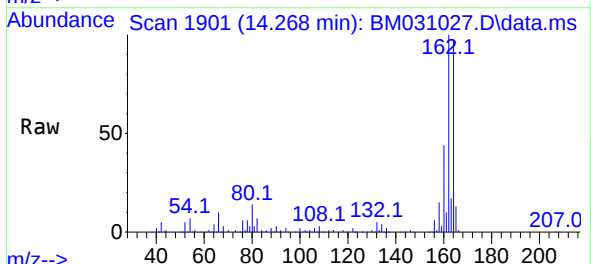




#42
2,4,6-Tribromophenol
Concen: 129.292 ng
RT: 15.762 min Scan# 2155
Delta R.T. -0.006 min
Lab File: BM031027.D
Acq: 20 Jul 2021 17:46




Instrument :
BNA_M
ClientSampleId :
PB137646BL


Tgt Ion:330 Resp: 362656
Ion Ratio Lower Upper
330 100
332 96.5 77.0 115.4
141 47.7 30.2 45.2#

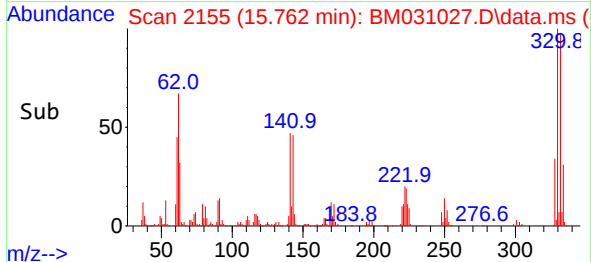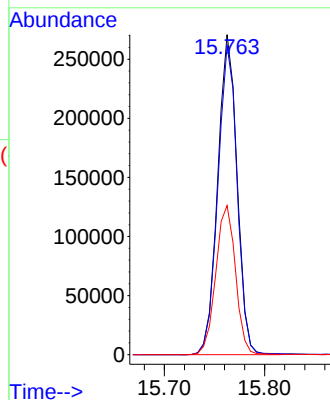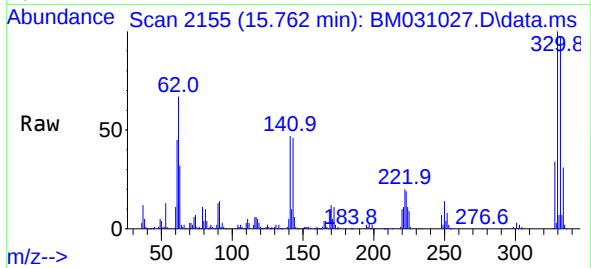

#45
2-Fluorobiphenyl
Concen: 88.598 ng
RT: 12.886 min Scan# 1666
Delta R.T. -0.006 min
Lab File: BM031027.D
Acq: 20 Jul 2021 17:46

Tgt Ion:172 Resp: 1275484
Ion Ratio Lower Upper
172 100
171 35.7 28.6 43.0
170 23.4 18.4 27.6


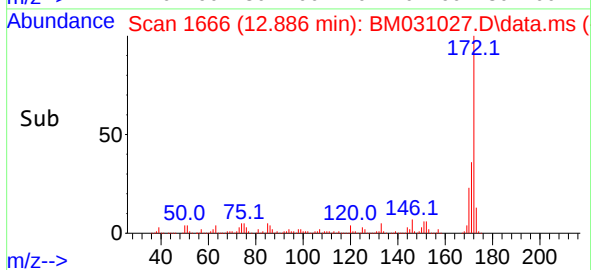
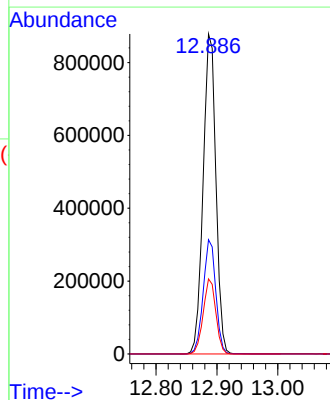
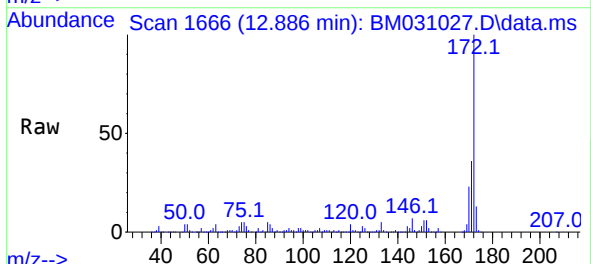




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.015 min Scan# 2368
Delta R.T. -0.006 min
Lab File: BM031027.D
Acq: 20 Jul 2021 17:46




Instrument :
BNA_M
ClientSampleId :
PB137646BL


Tgt Ion:188 Resp: 484293
Ion Ratio Lower Upper
188 100
94 6.3 6.0 9.0
80 7.8 6.6 9.8

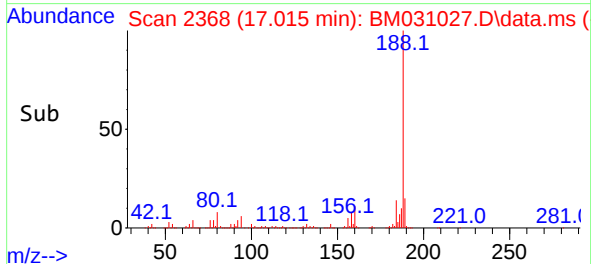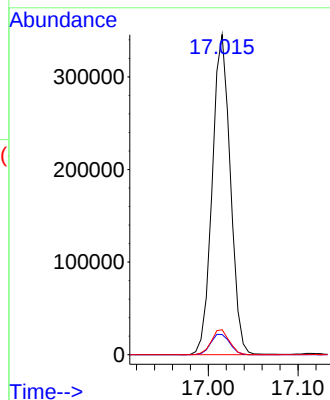

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.203 min Scan# 3080
Delta R.T. -0.006 min
Lab File: BM031027.D
Acq: 20 Jul 2021 17:46

Tgt Ion:240 Resp: 526169
Ion Ratio Lower Upper
240 100
120 8.1 7.0 10.6
236 24.5 21.0 31.4

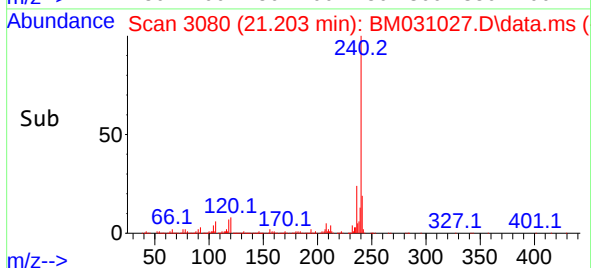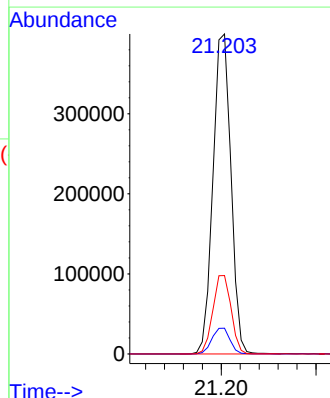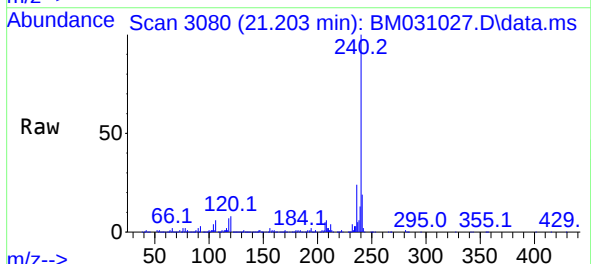







#79
 Terphenyl-d14
 Concen: 96.527 ng
 RT: 19.656 min Scan# 2817
 Delta R.T. 0.000 min
 Lab File: BM031027.D
 Acq: 20 Jul 2021 17:46

Instrument :
 BNA_M
 ClientSampleId :
 PB137646BL

Tgt Ion:244 Resp: 2567015

Ion	Ratio	Lower	Upper
244	100		
212	7.8	6.3	9.5
122	9.5	6.9	10.3

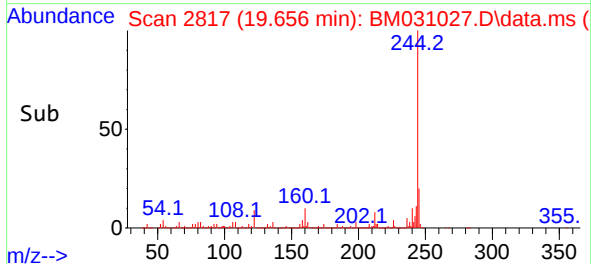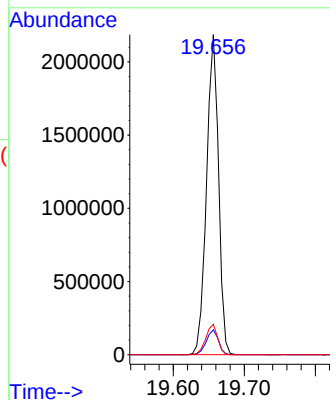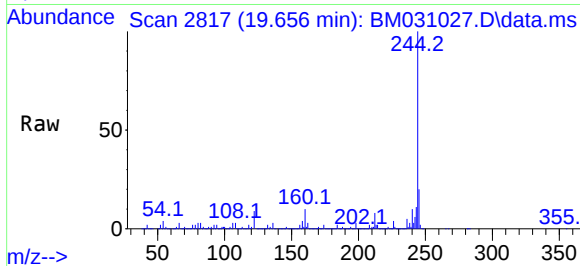

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.380 min Scan# 3450
 Delta R.T. -0.012 min
 Lab File: BM031027.D
 Acq: 20 Jul 2021 17:46

Tgt Ion:264 Resp: 550907

Ion	Ratio	Lower	Upper
264	100		
260	22.7	19.8	29.8
265	21.8	17.7	26.5

