

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072021\
 Data File : BM031027.D
 Acq On : 20 Jul 2021 17:46
 Operator : CG/JU
 Sample : PB137646BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB137646BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031027.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.257	363	369	385	rBV	1708972	2514056	33.32%	8.912%
2	6.822	627	635	651	rBV	1759705	2753280	36.49%	9.760%
3	7.640	766	774	781	rVB	296218	462737	6.13%	1.640%
4	8.786	961	969	981	rBV	1039546	1663350	22.04%	5.896%
5	10.404	1237	1244	1255	rVB	400189	665378	8.82%	2.359%
6	12.886	1659	1666	1675	rBV	2754481	3968475	52.59%	14.067%
7	14.268	1894	1901	1908	rBV	673734	964889	12.79%	3.420%
8	15.763	2148	2155	2171	rBV	2517787	3424185	45.38%	12.138%
9	17.015	2362	2368	2376	rBV	876832	1228675	16.28%	4.355%
10	19.656	2811	2817	2822	rBV	6383006	7545747	100.00%	26.748%
11	21.203	3074	3080	3085	rBV	1115885	1497611	19.85%	5.309%
12	23.380	3444	3450	3458	rVB2	860815	1522489	20.18%	5.397%




Sum of corrected areas: 28210872

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072021\
Data File : BM031027.D
Acq On : 20 Jul 2021 17:46
Operator : CG/JU
Sample : PB137646BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB137646BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

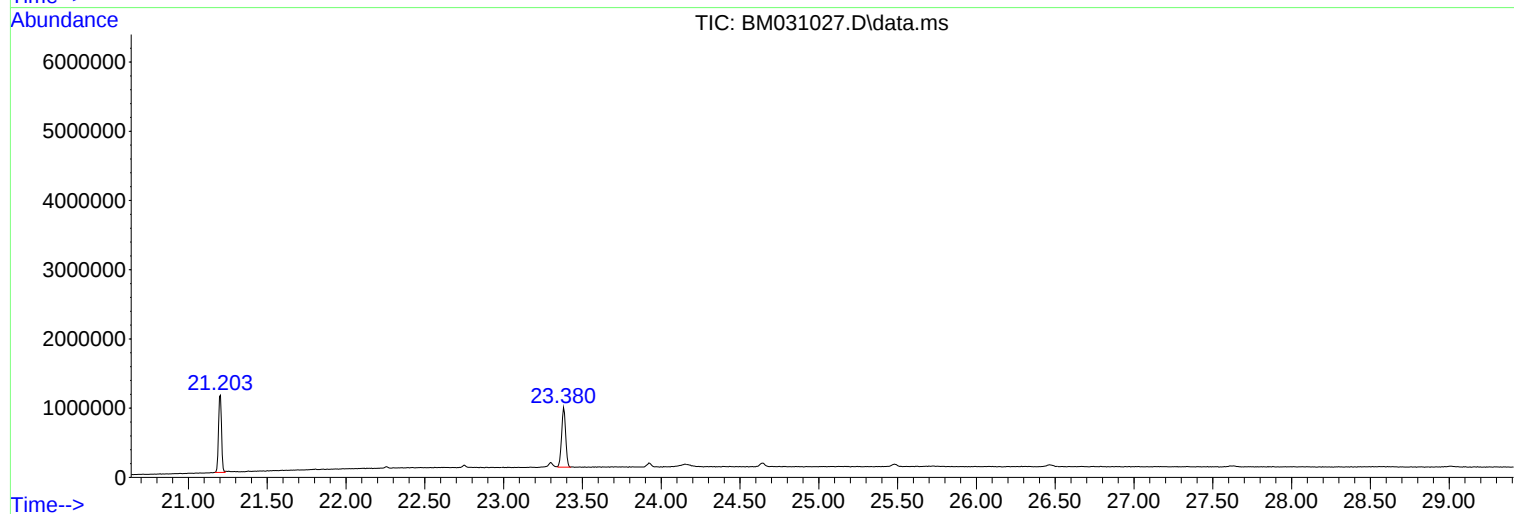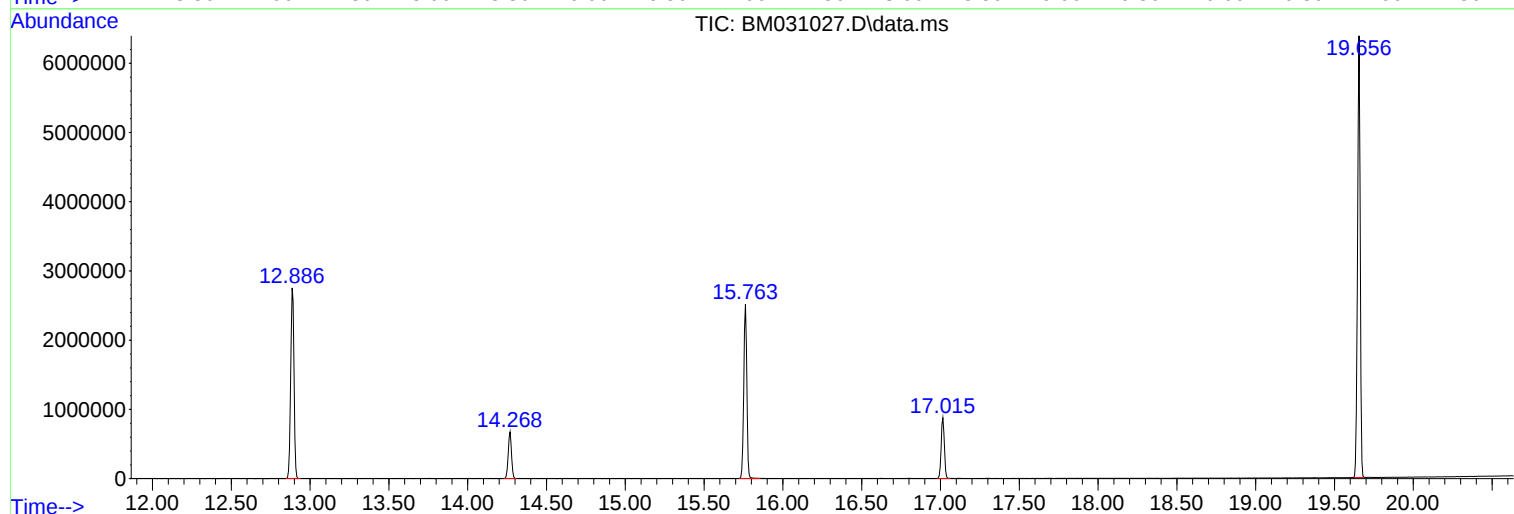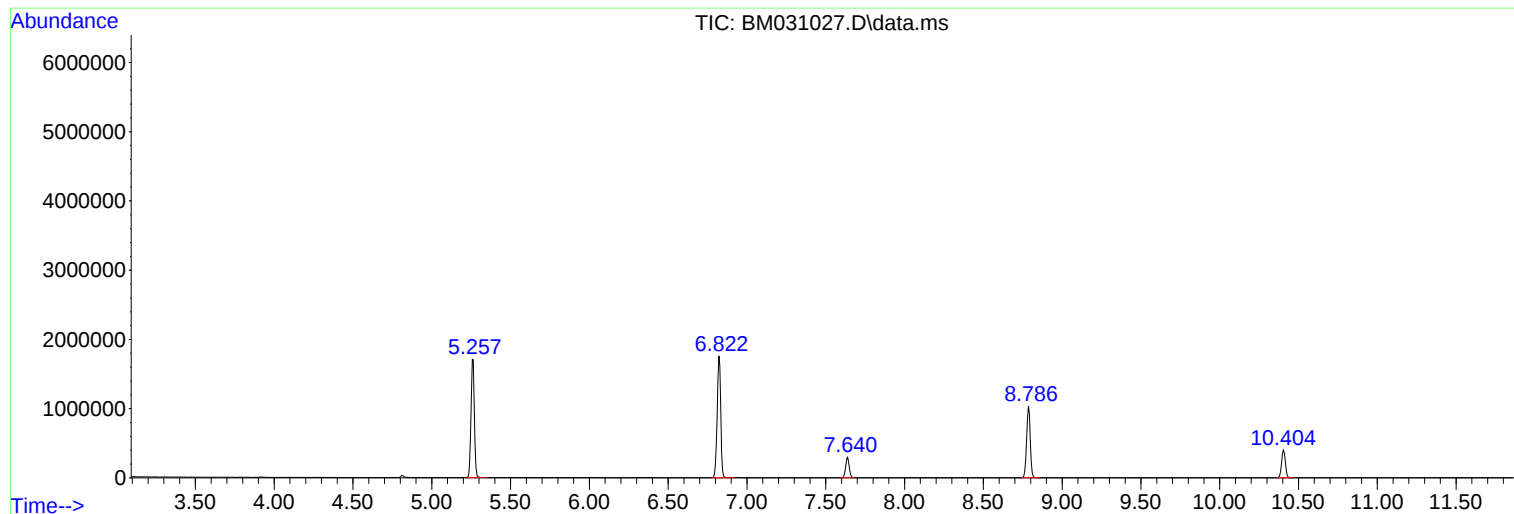

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072021\
Data File : BM031027.D
Acq On : 20 Jul 2021 17:46
Operator : CG/JU
Sample : PB137646BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB137646BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072021\
Data File : BM031027.D
Acq On : 20 Jul 2021 17:46
Operator : CG/JU
Sample : PB137646BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB137646BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------