
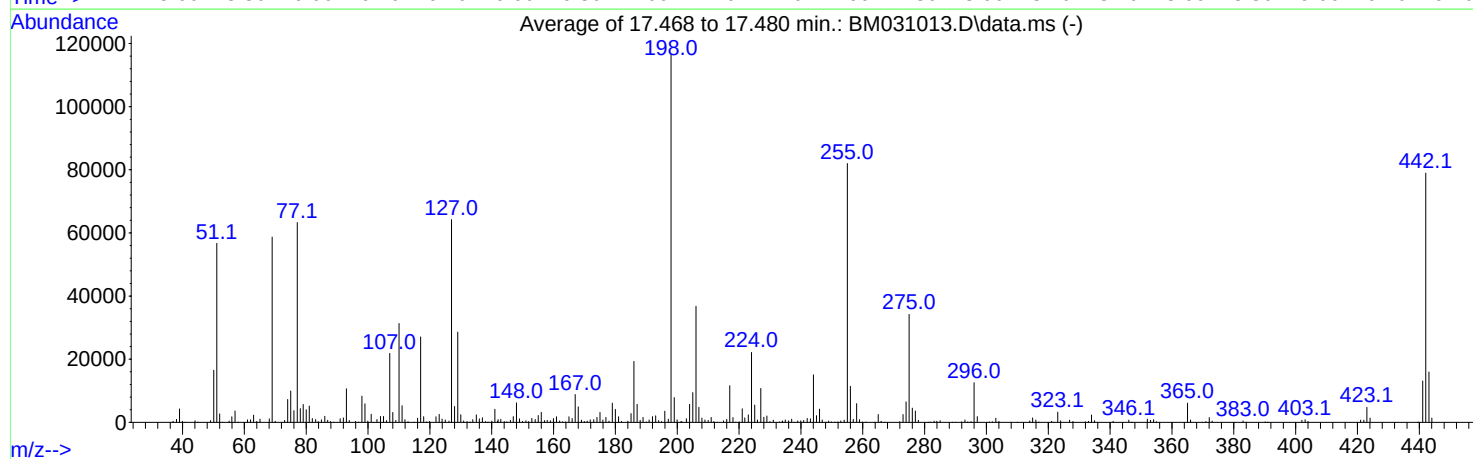


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072021\
 Data File : BM031013.D
 Acq On : 20 Jul 2021 08:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 20 13:21:40 2021

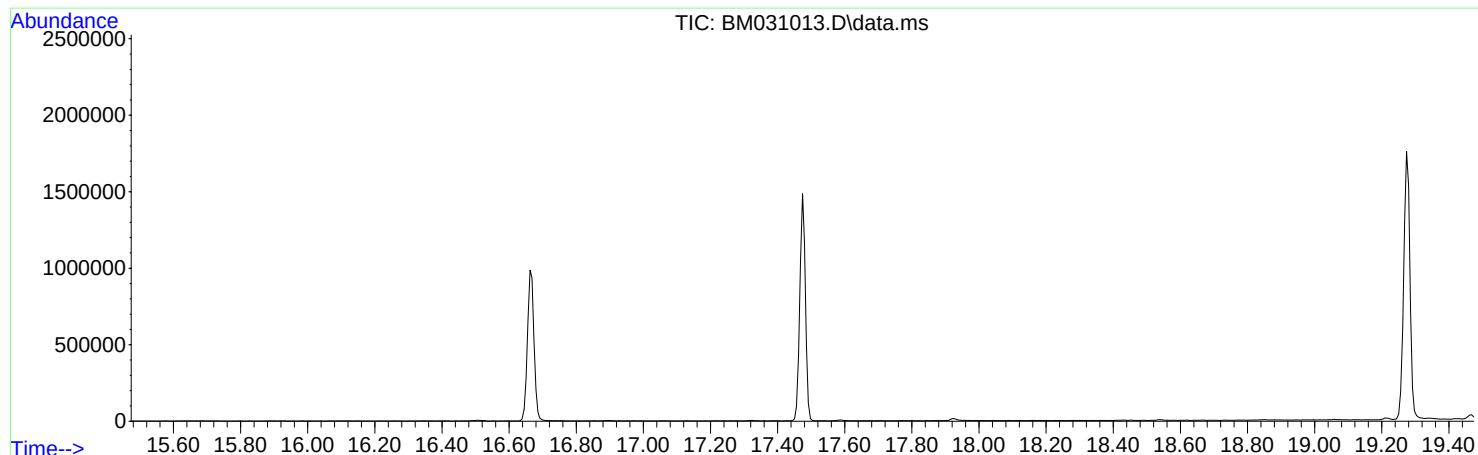




AutoFind: Scans 2445, 2446, 2447; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.7	56707	PASS
68	69	0.00	2	1.9	1141	PASS
69	198	0.00	100	50.3	58661	PASS
70	69	0.00	2	0.6	341	PASS
127	198	10	80	55.1	64227	PASS
197	198	0.00	2	0.9	1006	PASS
198	198	100	100	100.0	116507	PASS
199	198	5	9	6.7	7837	PASS
275	198	10	60	29.4	34229	PASS
365	198	1	100	5.2	6063	PASS
441	198	0.01	100	11.3	13153	PASS
442	442	50	100	100.0	78973	PASS
443	442	15	24	20.2	15977	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072021\
Data File : BM031013.D
Acq On : 20 Jul 2021 08:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 20 10:56:51 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 19 18:48:56 2021
Response via : Initial Calibration

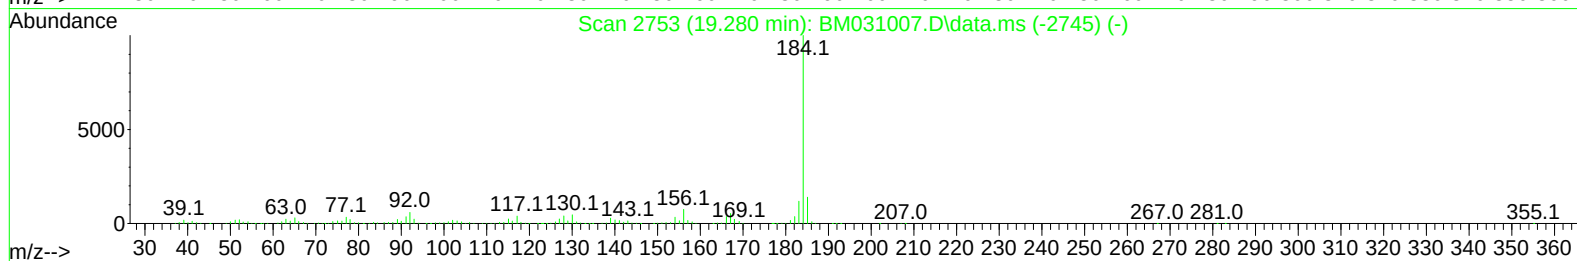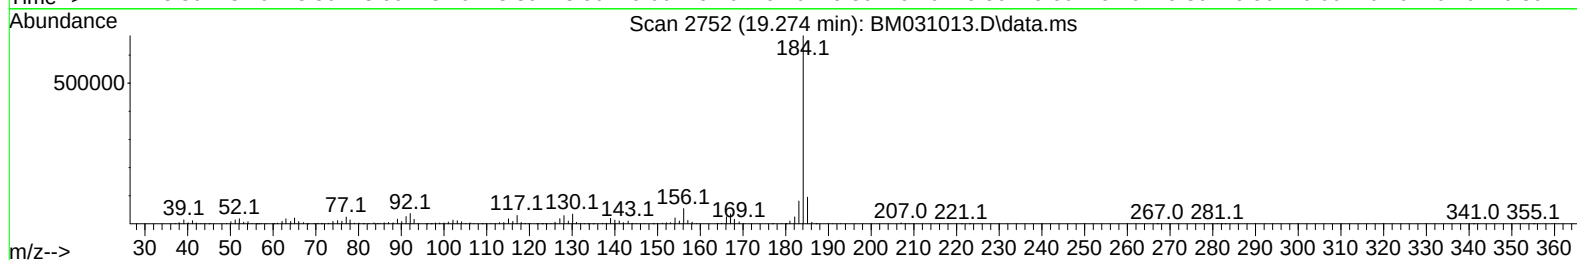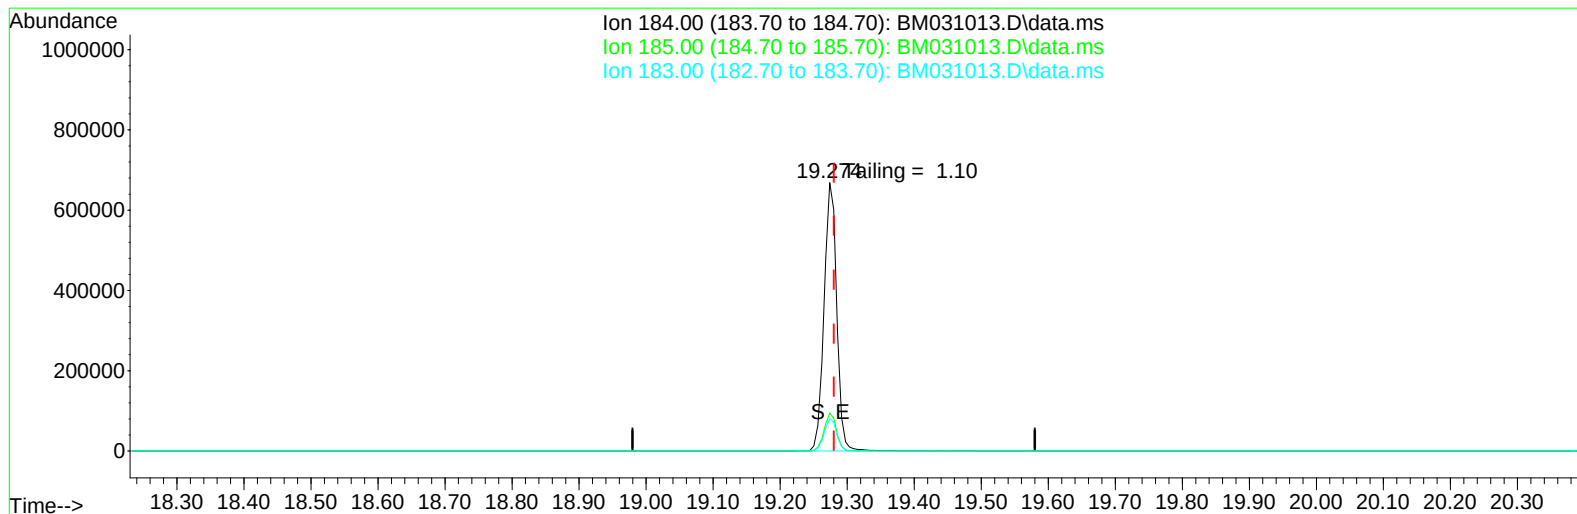

TIC: BM031013.D\data.ms

(77) Benzidine

19.274min (-0.006) 44702.49 ng




response 877812

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.17
183.00	12.30	12.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072021\
Data File : BM031013.D
Acq On : 20 Jul 2021 08:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 20 10:56:51 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 19 18:48:56 2021
Response via : Initial Calibration

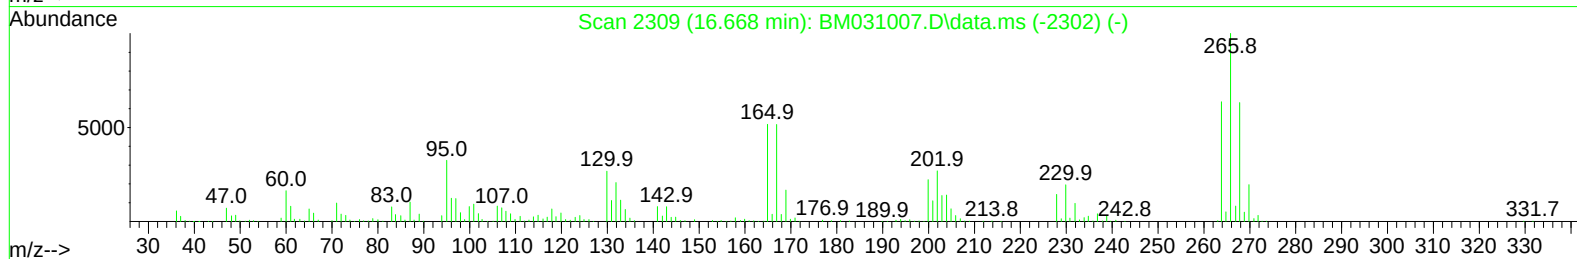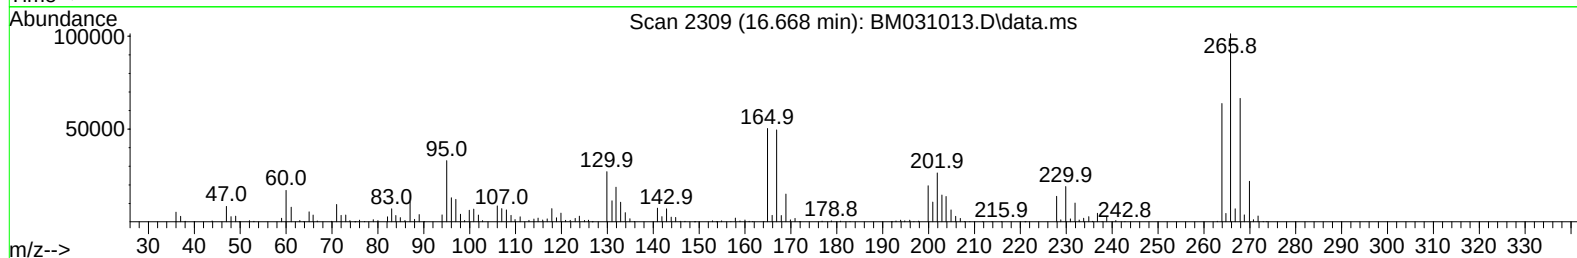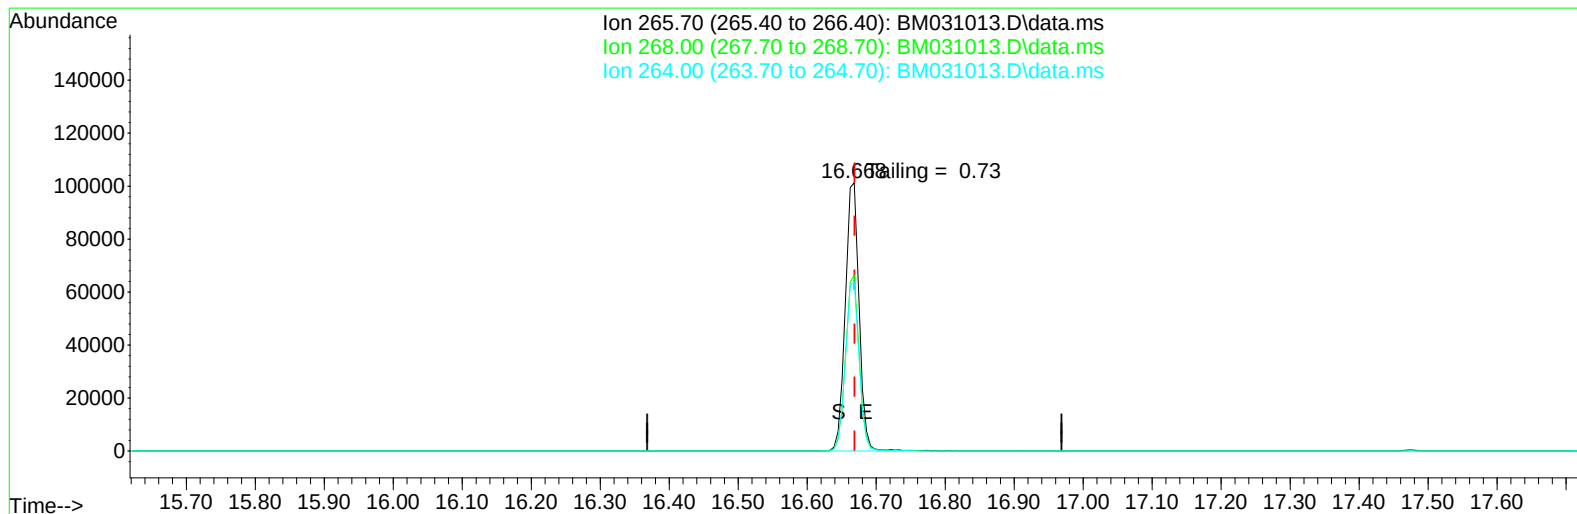

TIC: BM031013.D\data.ms

(70) Pentachlorophenol (C)

16.668min (-0.000) 314417.22 ng

response 140310

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	65.66
264.00	64.90	62.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/20/2021	BNA_M	<u>BM031013.D</u>
Compound Name	Response	Retention Time
DDT	501580	20.5
DDD	2623	20.07
DDE	0	19.56
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2623	504203	0.52

Instrument :
BNA_M
ClientSampleId :
DFTPP