
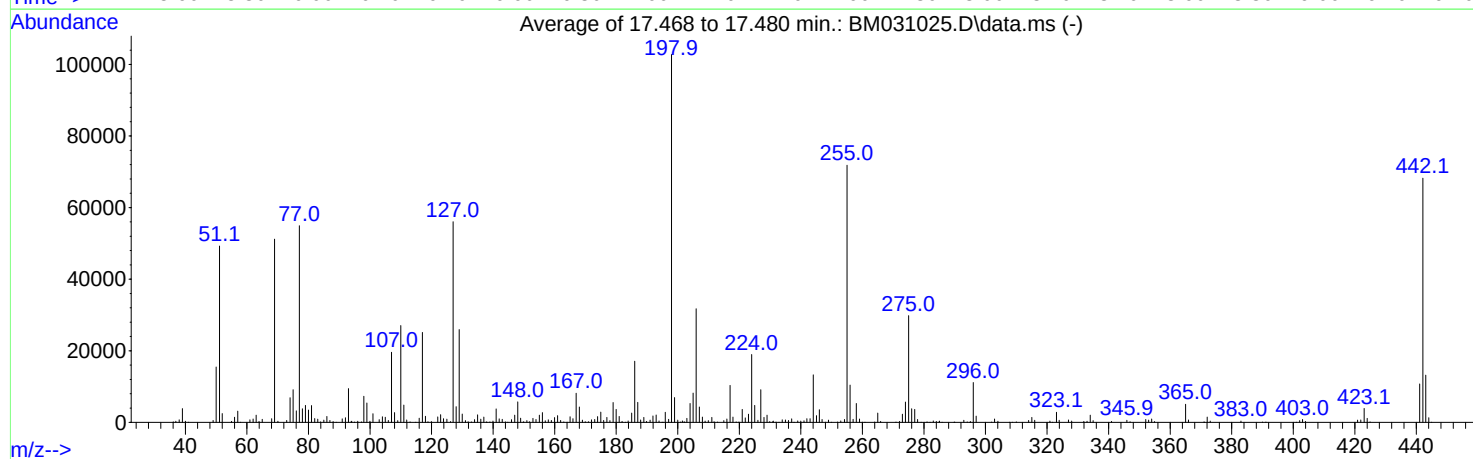


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072021\
 Data File : BM031025.D
 Acq On : 20 Jul 2021 16:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 20 13:21:40 2021

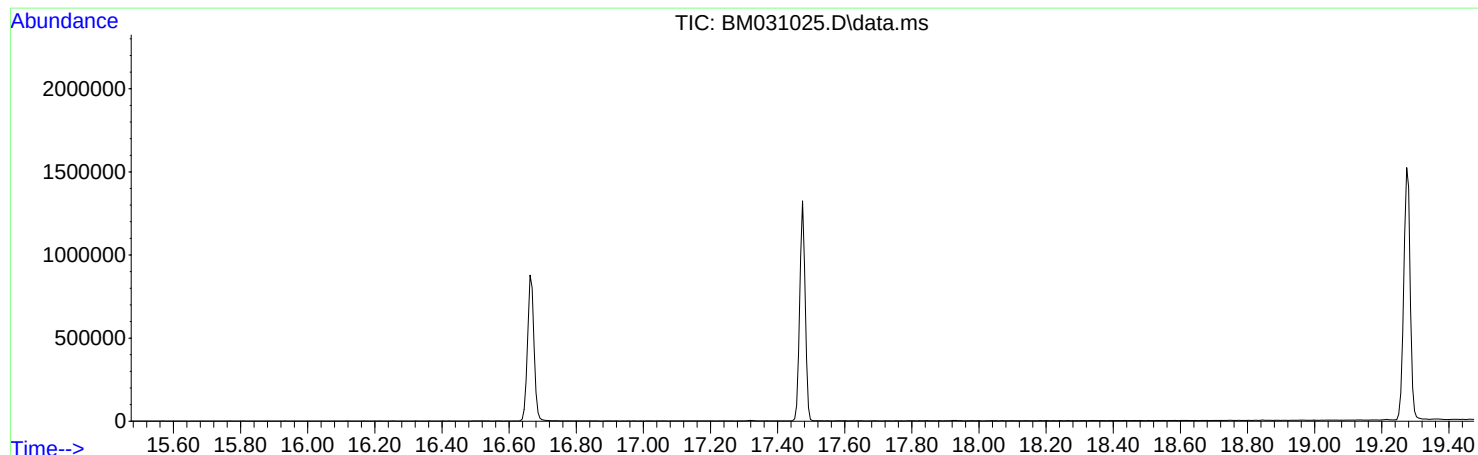




AutoFind: Scans 2445, 2446, 2447; Background Corrected with Scan 2438

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.9	49264	PASS
68	69	0.00	2	2.0	1011	PASS
69	198	0.00	100	49.8	51176	PASS
70	69	0.00	2	0.6	301	PASS
127	198	10	80	54.6	56075	PASS
197	198	0.00	2	0.9	874	PASS
198	198	100	100	100.0	102773	PASS
199	198	5	9	6.7	6937	PASS
275	198	10	60	29.0	29843	PASS
365	198	1	100	4.9	5074	PASS
441	198	0.01	100	10.5	10748	PASS
442	442	50	100	100.0	68227	PASS
443	442	15	24	19.3	13175	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072021\
Data File : BM031025.D
Acq On : 20 Jul 2021 16:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 20 17:15:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 20 13:21:40 2021
Response via : Initial Calibration

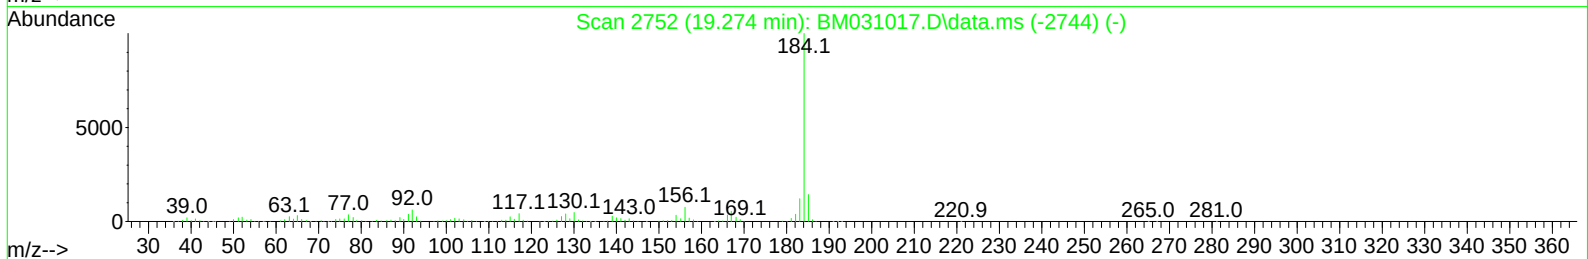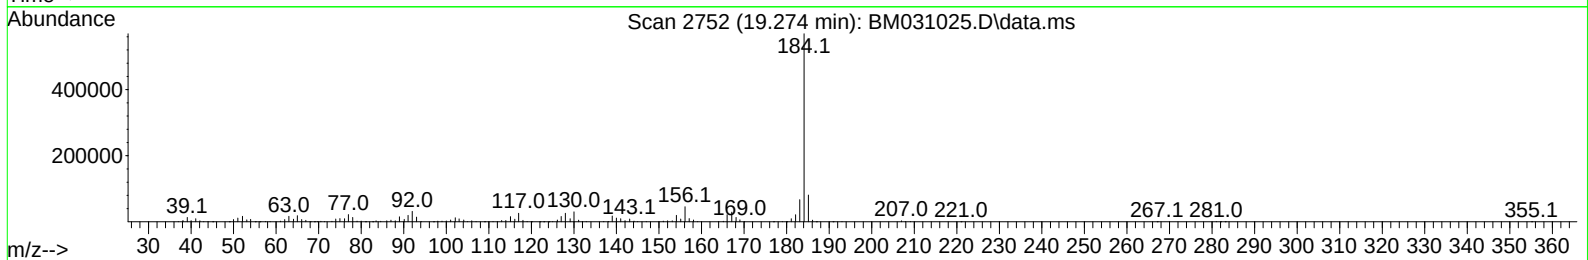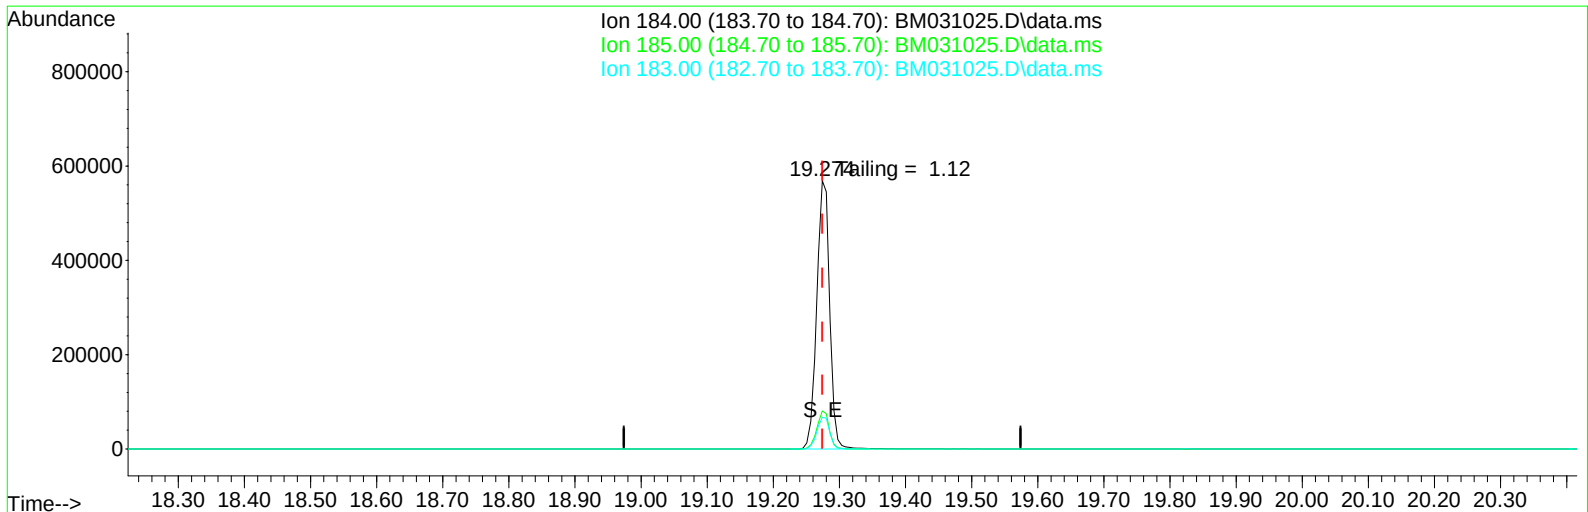

TIC: BM031025.D\data.ms

(77) Benzidine

19.274min (+ 0.000) 0.00 ng




response 773611

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.22
183.00	12.30	11.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072021\
 Data File : BM031025.D
 Acq On : 20 Jul 2021 16:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jul 20 17:15:44 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 20 13:21:40 2021
 Response via : Initial Calibration

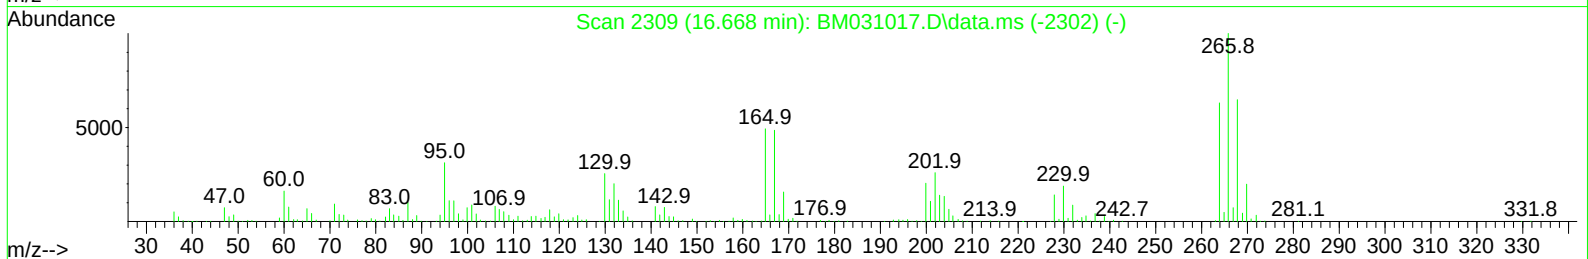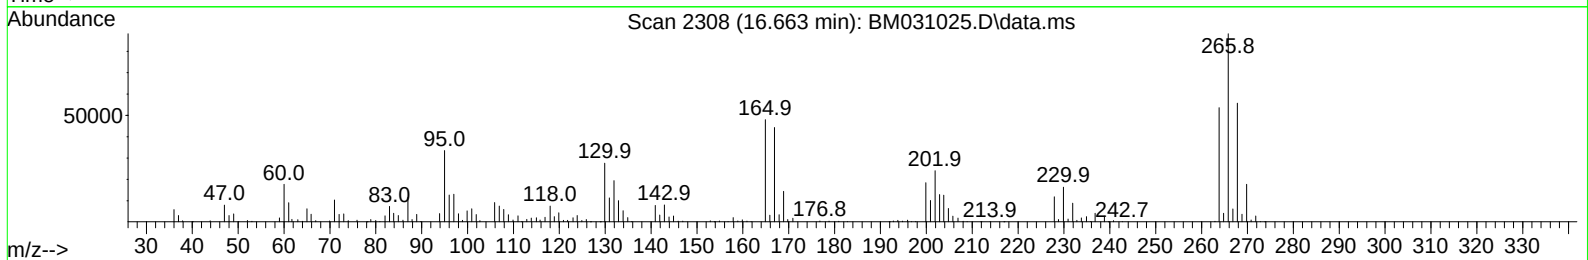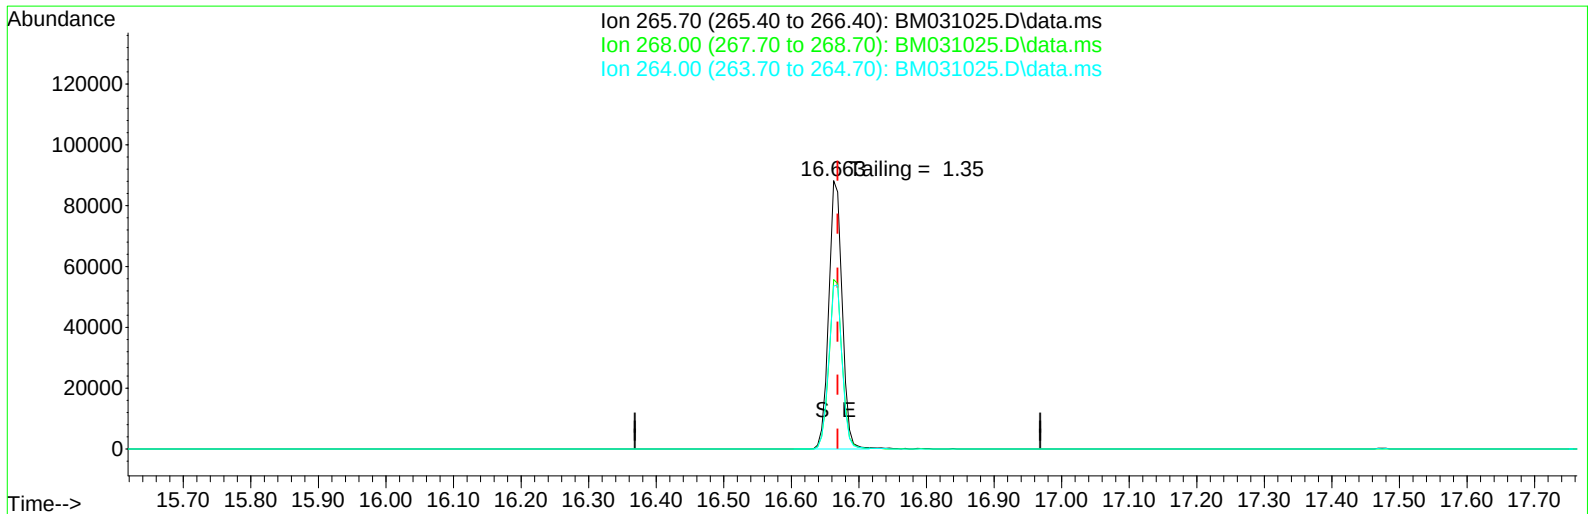

TIC: BM031025.D\data.ms

(70) Pentachlorophenol (C)

16.663min (-0.006) 0.00 ng

response 122320

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	63.13
264.00	64.90	60.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/20/2021	BNA_M	<u>BM031025.D</u>
Compound Name	Response	Retention Time
DDT	444502	20.51
DDD	3886	20.06
DDE	693	19.56
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4579	449081	1.02

Instrument :
BNA_M
ClientSampleId :
DFTPP