
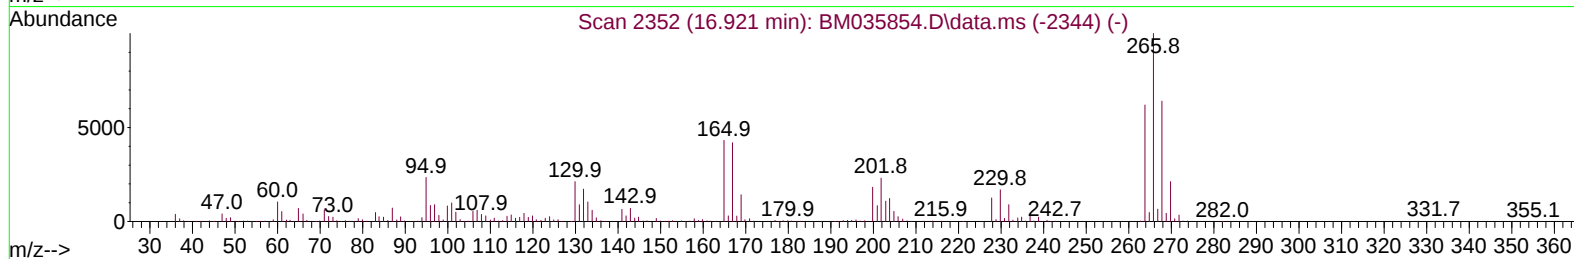
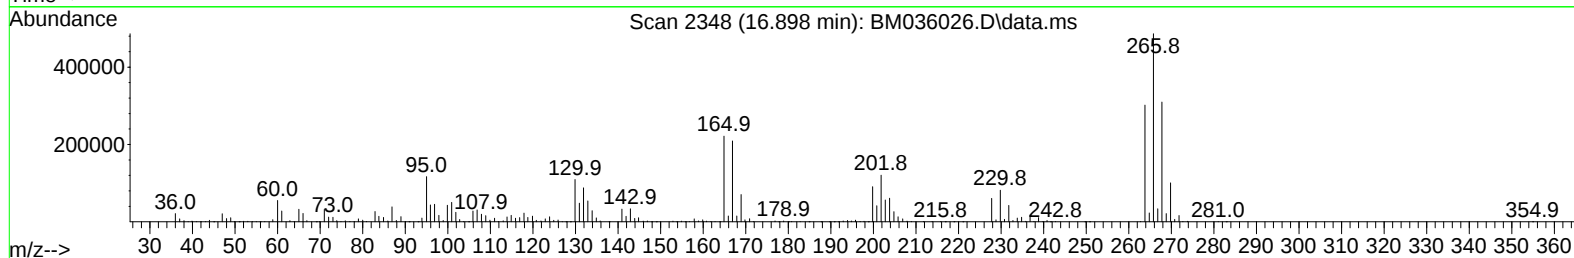


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
 Data File : BM036026.D
 Acq On : 01 Aug 2022 10:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 15:49:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 01 15:17:30 2022
 Response via : Initial Calibration

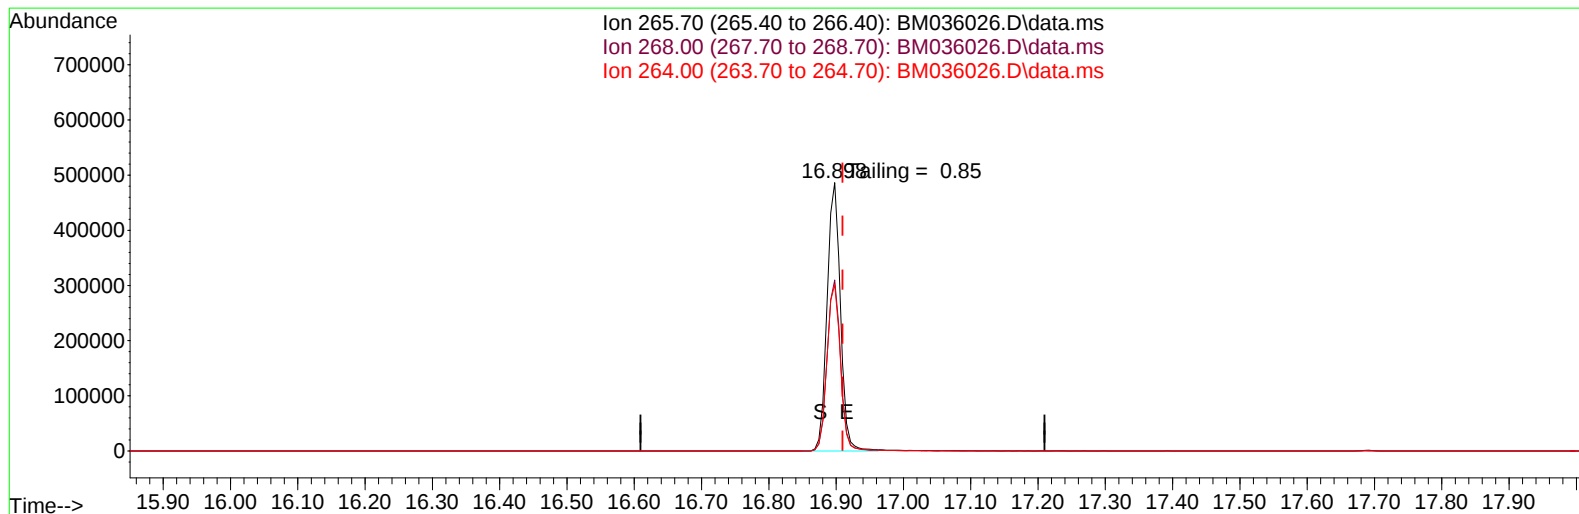

TIC: BM036026.D\data.ms

(70) Pentachlorophenol (C)




16.898min (-0.012) 24533.74 ng

response 670898

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.71
264.00	63.30	62.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
 Data File : BM036026.D
 Acq On : 01 Aug 2022 10:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 15:49:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 01 15:17:30 2022
 Response via : Initial Calibration

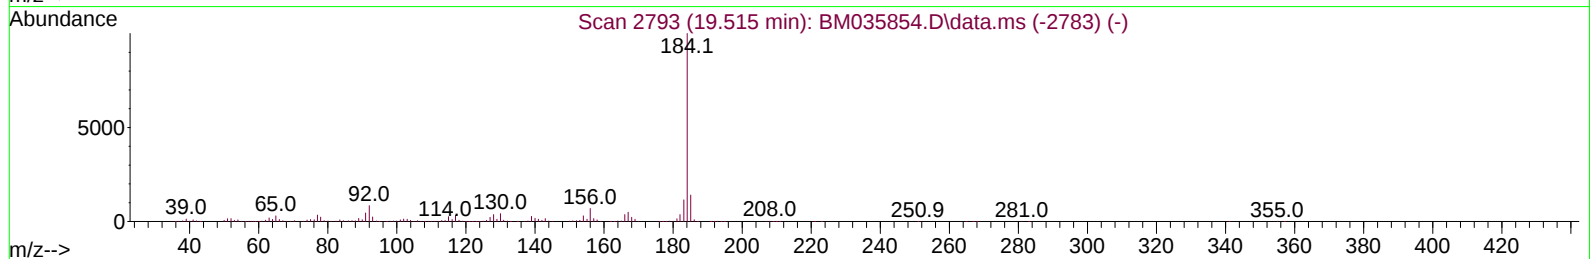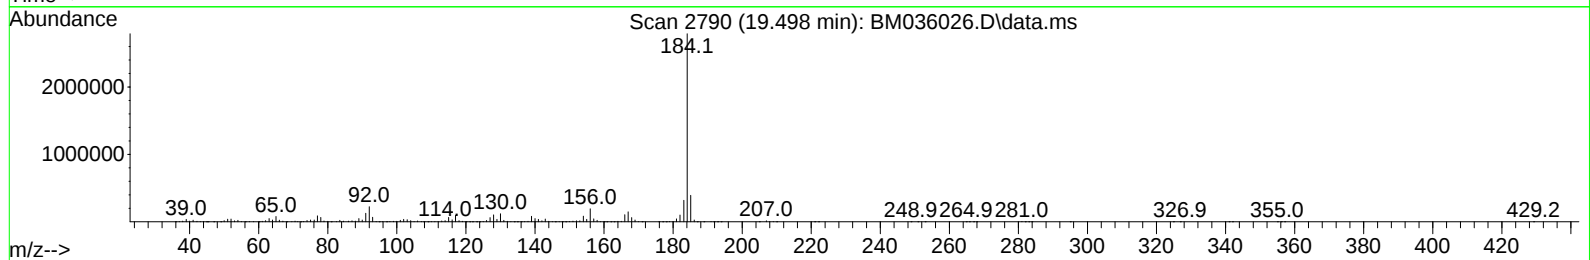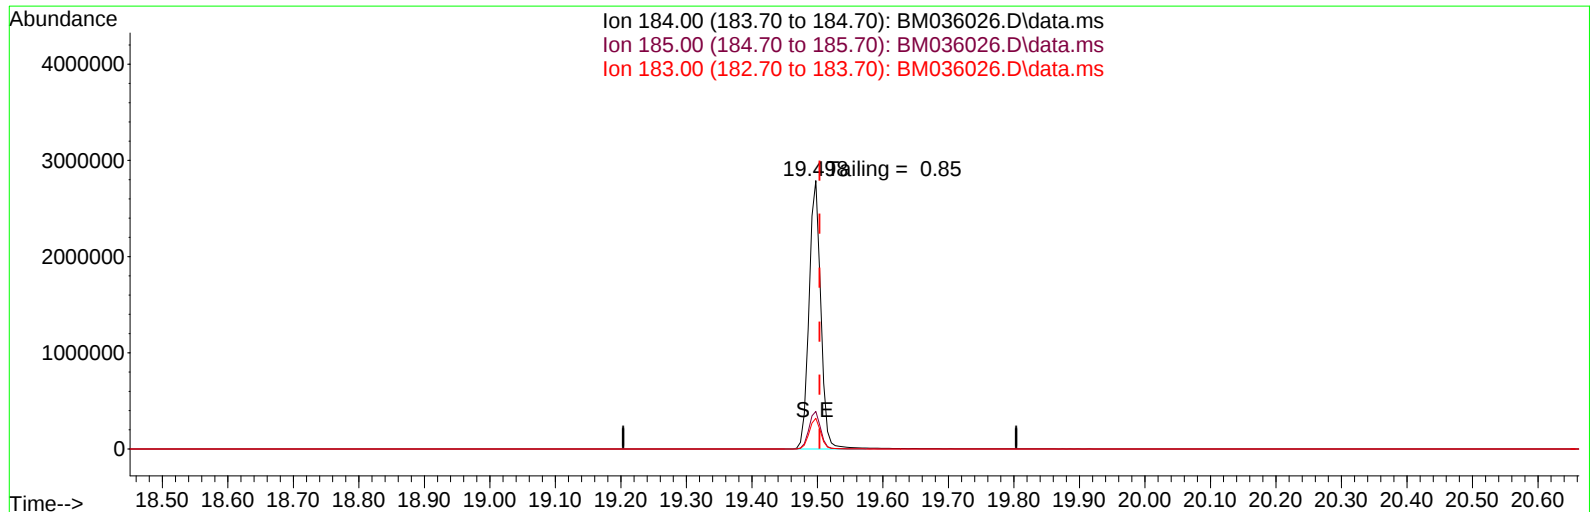

TIC: BM036026.D\data.ms

(77) Benzidine**19.498min (-0.006) 425699.60 ng****response 3490375**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.02
183.00	11.90	11.44
0.00	0.00	0.00