

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
 Data File : BM036036.D
 Acq On : 01 Aug 2022 18:41
 Operator : CG/JU
 Sample : PB146536BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB146536BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.434	392	399	415	rBV	6836402	9596576	57.72%	11.537%
2	7.040	663	672	686	rBV	6014196	9592425	57.69%	11.532%
3	7.869	807	813	821	rBV	1231173	1918135	11.54%	2.306%
4	9.040	1003	1012	1029	rBV	3964129	6355991	38.23%	7.641%
5	10.675	1282	1290	1300	rBV	1663964	2714307	16.33%	3.263%
6	13.139	1701	1709	1719	rBV	9920850	14140362	85.05%	16.999%
7	14.510	1935	1942	1954	rBV	2231659	3317353	19.95%	3.988%
8	15.992	2187	2194	2212	rBV	6911548	9352883	56.25%	11.244%
9	17.245	2400	2407	2418	rBV	2487953	3578331	21.52%	4.302%
10	19.874	2848	2854	2864	rBV	13985884	16626437	100.00%	19.987%
11	21.427	3113	3118	3124	rBV	2523161	3171331	19.07%	3.812%
12	23.792	3514	3520	3531	rVB2	1450855	2820220	16.96%	3.390%




Sum of corrected areas: 83184351

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
Data File : BM036036.D
Acq On : 01 Aug 2022 18:41
Operator : CG/JU
Sample : PB146536BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146536BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

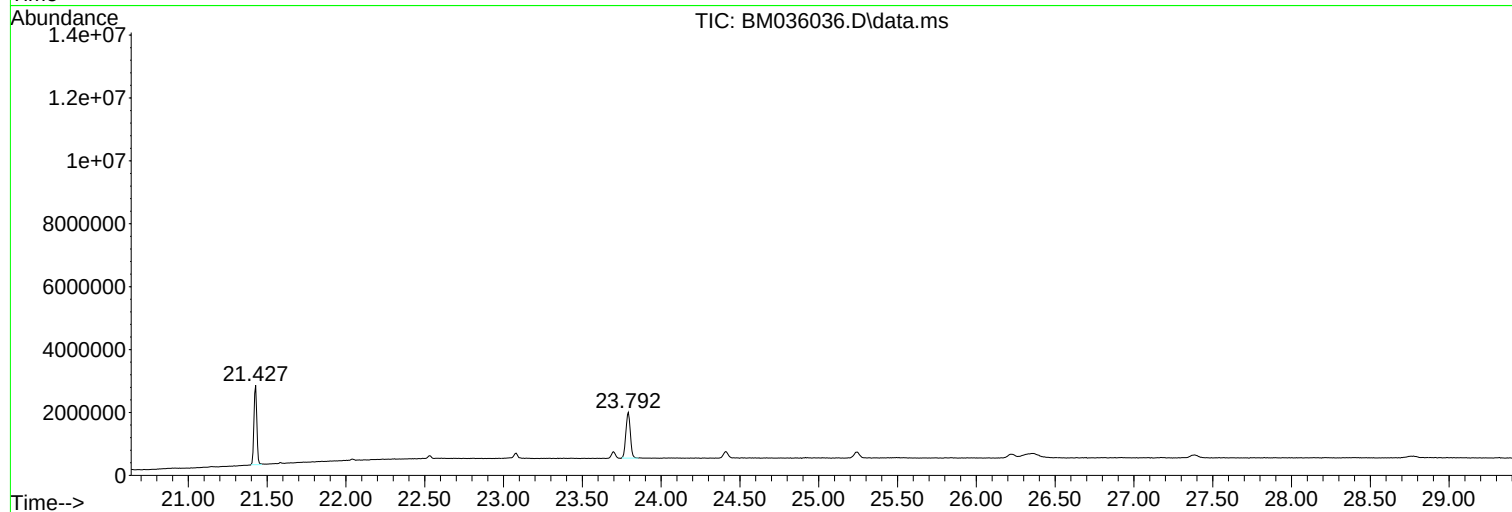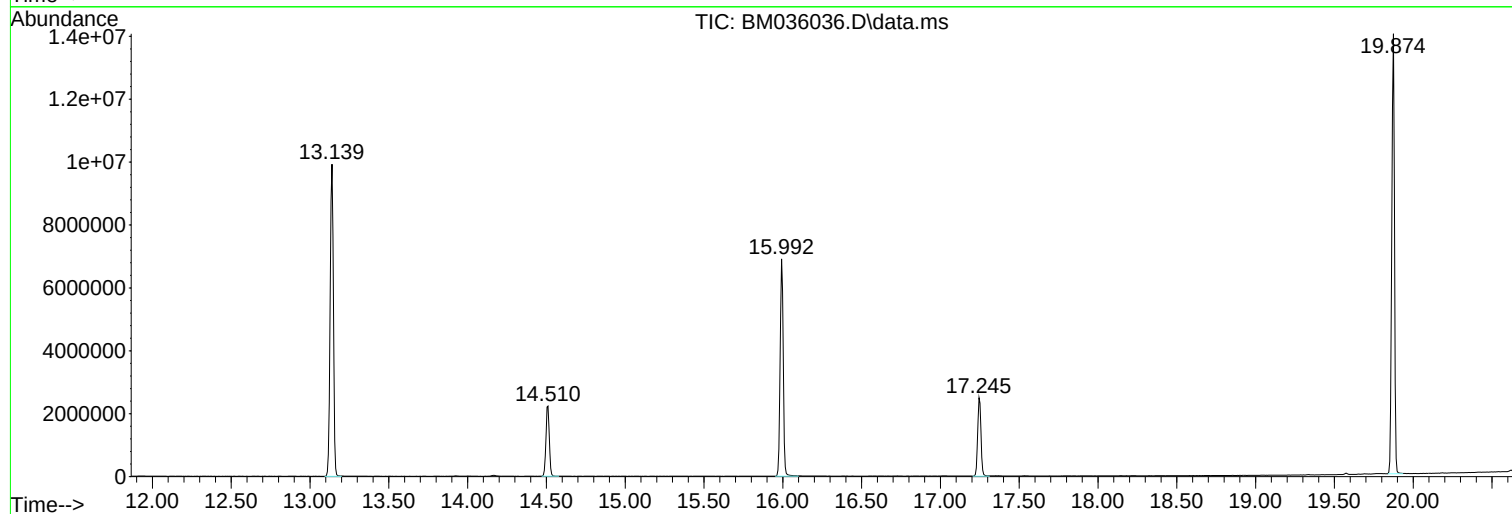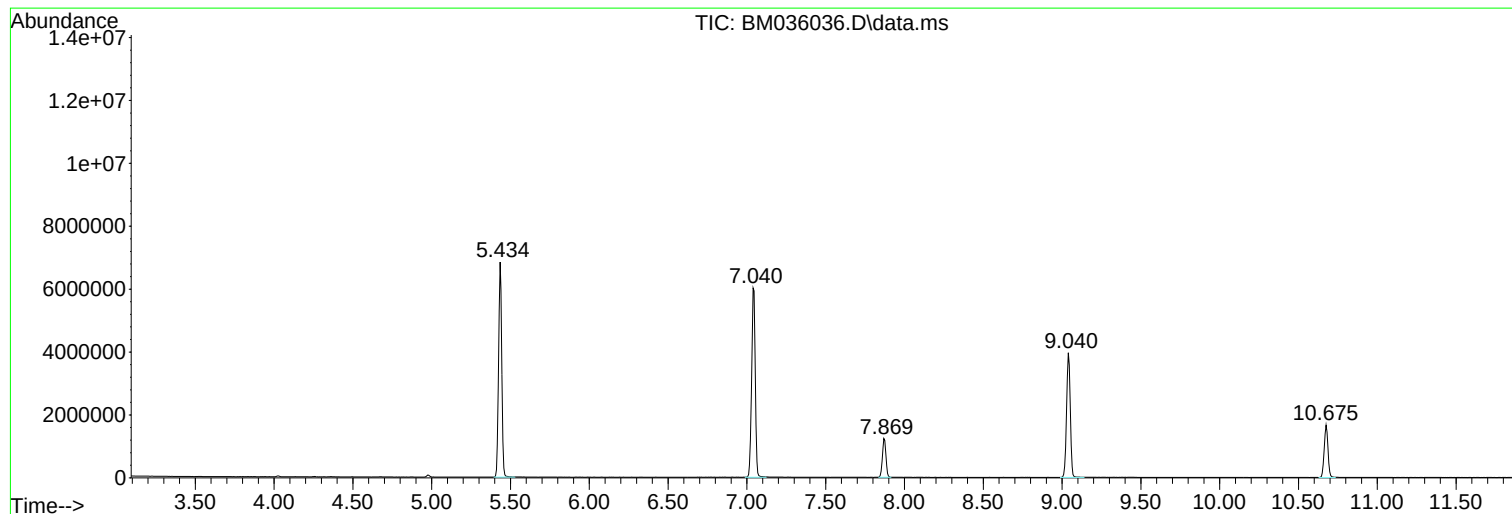

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
Data File : BM036036.D
Acq On : 01 Aug 2022 18:41
Operator : CG/JU
Sample : PB146536BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146536BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
Data File : BM036036.D
Acq On : 01 Aug 2022 18:41
Operator : CG/JU
Sample : PB146536BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146536BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------