

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
 Data File : BM036037.D
 Acq On : 01 Aug 2022 19:18
 Operator : CG/JU
 Sample : PB146582BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB146582BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036037.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.434	392	399	414	rBV	6903174	9609294	59.52%	11.666%
2	7.045	664	673	686	rBV	6068062	9676202	59.93%	11.748%
3	7.869	805	813	823	rBV	1195631	1898411	11.76%	2.305%
4	9.039	1004	1012	1025	rBV	3960049	6339740	39.27%	7.697%
5	10.675	1282	1290	1300	rBV	1616002	2674396	16.57%	3.247%
6	13.139	1701	1709	1719	rBV	10117468	14127800	87.51%	17.152%
7	14.510	1935	1942	1951	rBV	2218611	3290529	20.38%	3.995%
8	15.992	2187	2194	2216	rBV	6662565	9360482	57.98%	11.364%
9	17.245	2401	2407	2421	rBV	2534135	3501593	21.69%	4.251%
10	19.874	2848	2854	2866	rBV	13366201	16144560	100.00%	19.601%
11	21.427	3113	3118	3124	rBV	2411732	3041729	18.84%	3.693%
12	23.791	3513	3520	3529	rBV	1366576	2702806	16.74%	3.281%




Sum of corrected areas: 82367542

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
Data File : BM036037.D
Acq On : 01 Aug 2022 19:18
Operator : CG/JU
Sample : PB146582BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146582BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

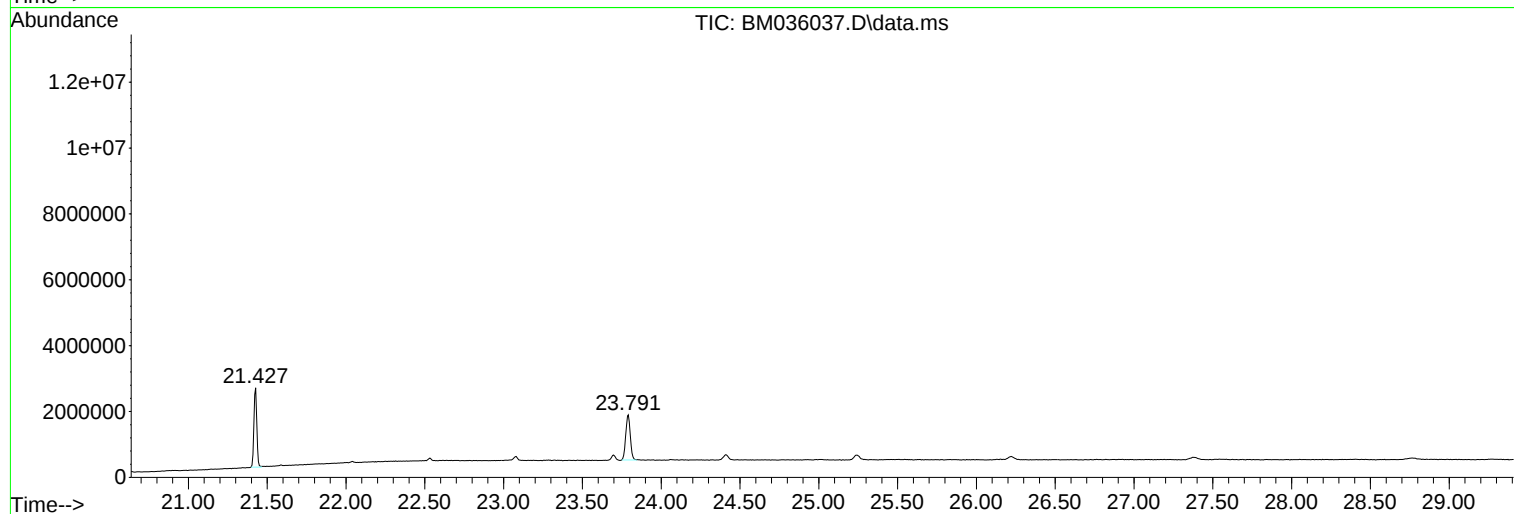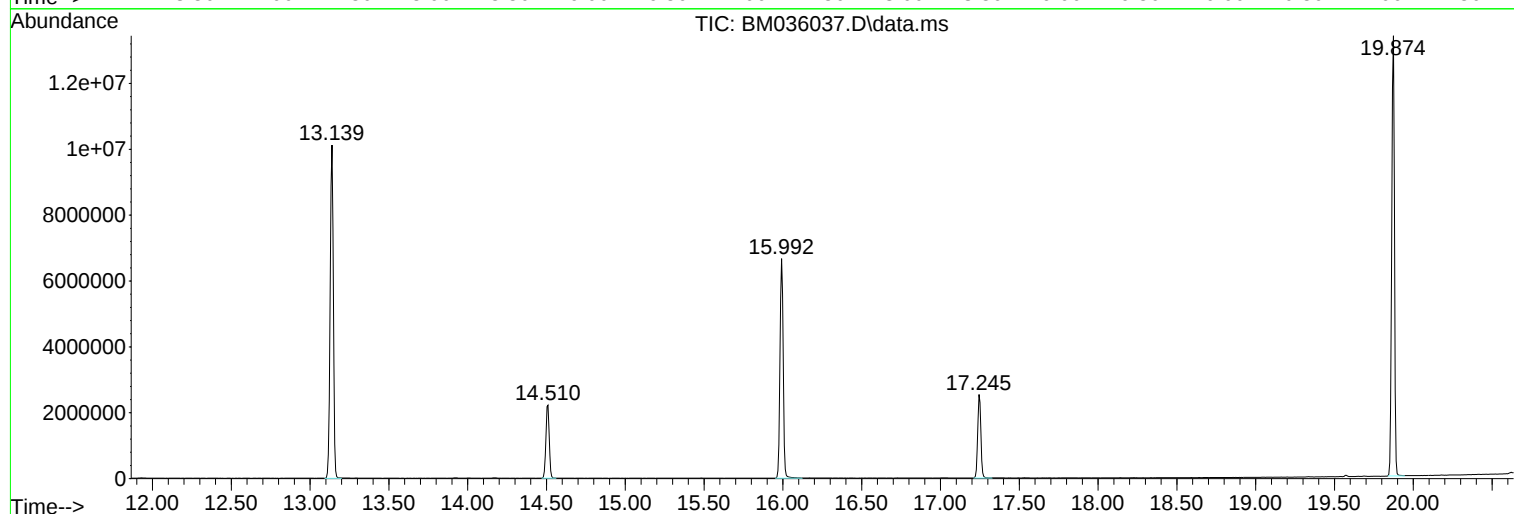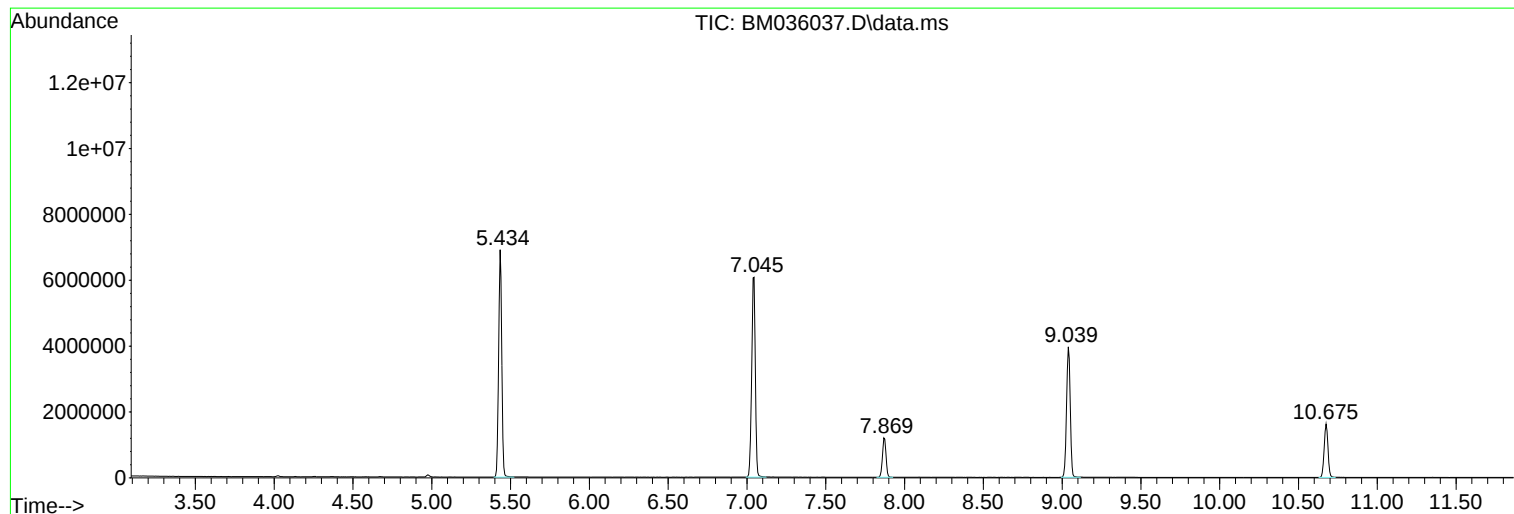

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
Data File : BM036037.D
Acq On : 01 Aug 2022 19:18
Operator : CG/JU
Sample : PB146582BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146582BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
Data File : BM036037.D
Acq On : 01 Aug 2022 19:18
Operator : CG/JU
Sample : PB146582BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146582BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------