

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
 Data File : BM036041.D
 Acq On : 01 Aug 2022 21:43
 Operator : CG/JU
 Sample : PB146577BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB146577BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.434	392	399	416	rBV	5520051	7732494	53.63%	11.154%
2	7.040	664	672	685	rBV	5074504	7795538	54.07%	11.245%
3	7.869	806	813	826	rBV	1001548	1536552	10.66%	2.216%
4	9.039	1003	1012	1026	rBV	3173248	5102172	35.39%	7.360%
5	10.675	1282	1290	1303	rBV	1305465	2178057	15.11%	3.142%
6	13.133	1701	1708	1722	rBV	7686671	11534794	80.01%	16.639%
7	14.504	1935	1941	1955	rBV	1852601	2713880	18.82%	3.915%
8	15.992	2187	2194	2213	rBV	5605016	7805413	54.14%	11.259%
9	17.245	2401	2407	2423	rBV	2142806	3019015	20.94%	4.355%
10	19.868	2848	2853	2863	rBV	11967920	14416936	100.00%	20.797%
11	21.421	3112	3117	3124	rBV	2366759	2847585	19.75%	4.108%
12	23.786	3513	3519	3532	rVB2	1355917	2641043	18.32%	3.810%




Sum of corrected areas: 69323479

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
Data File : BM036041.D
Acq On : 01 Aug 2022 21:43
Operator : CG/JU
Sample : PB146577BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146577BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

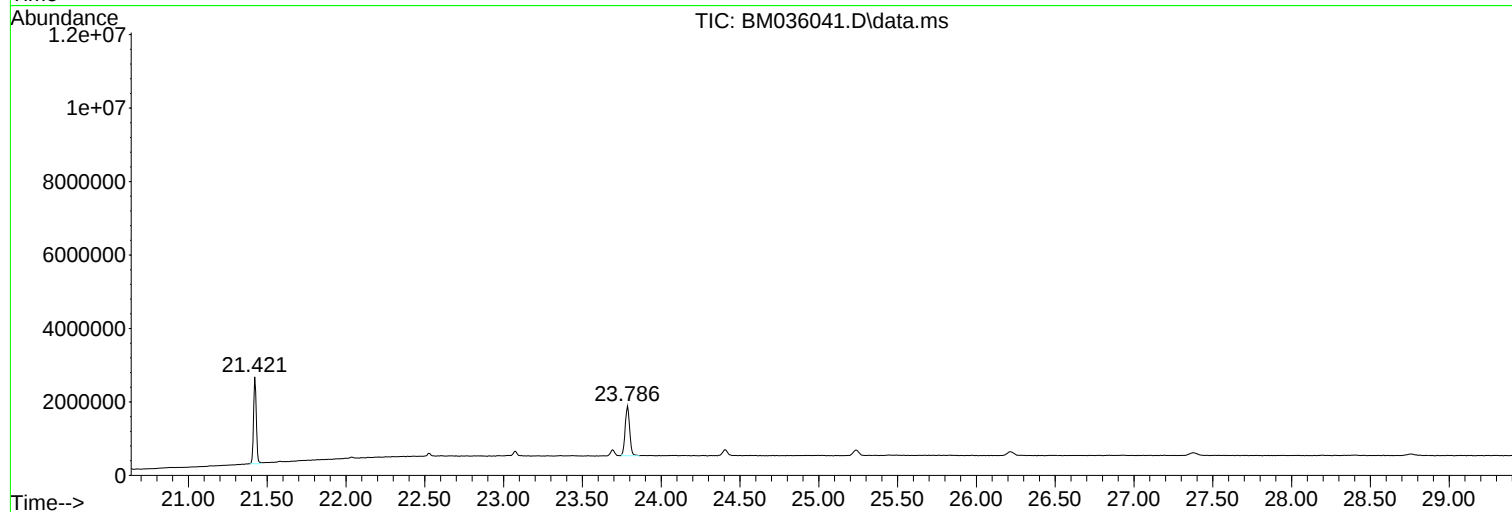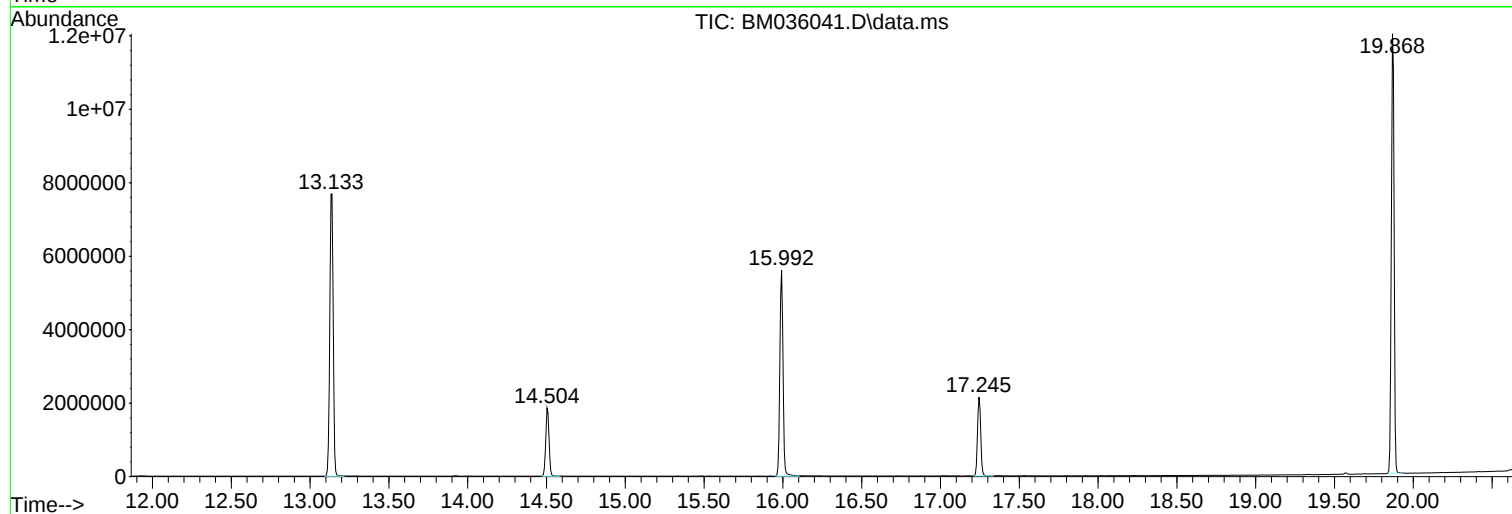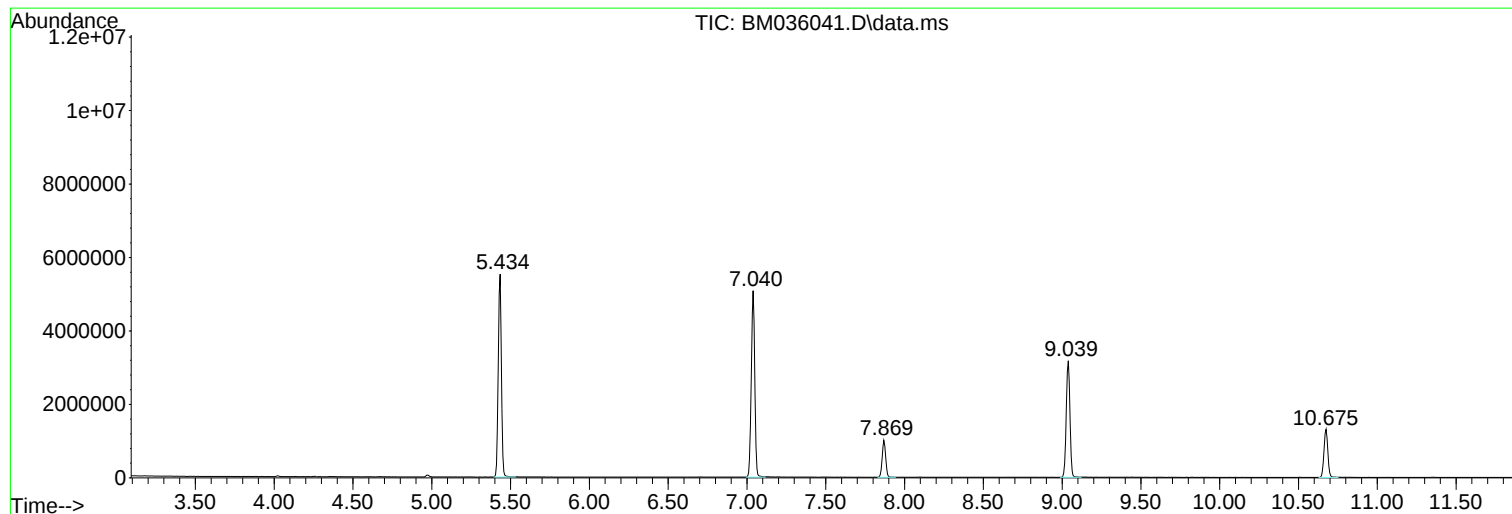

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
Data File : BM036041.D
Acq On : 01 Aug 2022 21:43
Operator : CG/JU
Sample : PB146577BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146577BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
Data File : BM036041.D
Acq On : 01 Aug 2022 21:43
Operator : CG/JU
Sample : PB146577BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146577BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------