
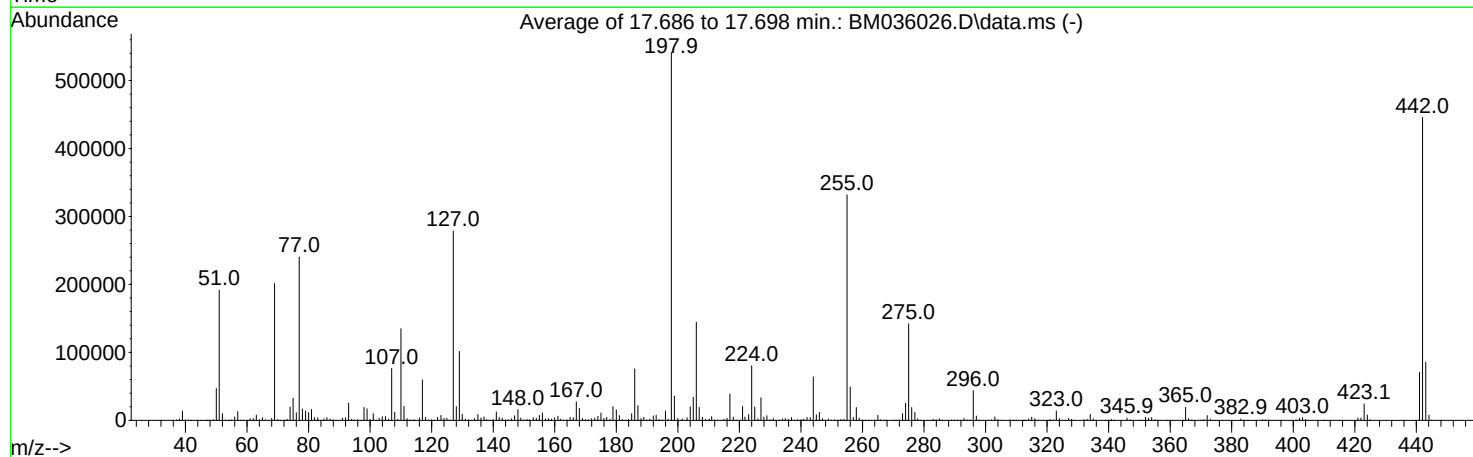


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
 Data File : BM036026.D
 Acq On : 01 Aug 2022 10:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 01 17:50:14 2022

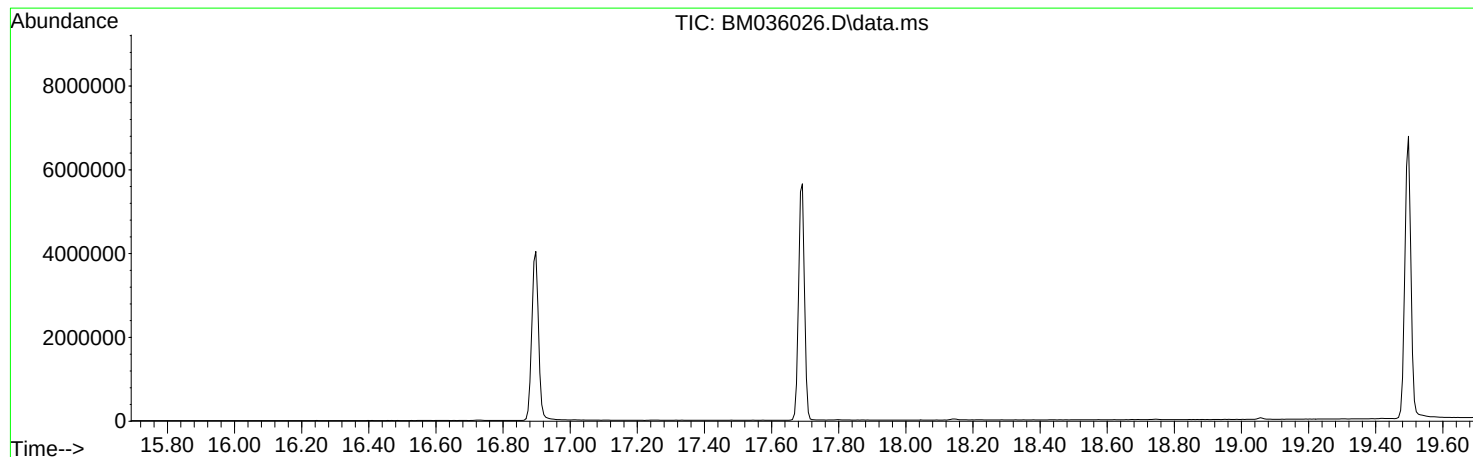

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	191563	PASS
68	69	0.00	2	1.4	2806	PASS
69	198	0.00	100	37.2	201162	PASS
70	69	0.00	2	0.6	1116	PASS
127	198	10	80	51.5	278720	PASS
197	198	0.00	2	0.3	1857	PASS
198	198	100	100	100.0	541184	PASS
199	198	5	9	6.6	35728	PASS
275	198	10	60	26.2	141952	PASS
365	198	1	100	3.6	19450	PASS
441	198	0.01	100	13.0	70459	PASS
442	442	50	100	100.0	445653	PASS
443	442	15	24	19.2	85448	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/1/2022	BNA_M	<u>BM036026.D</u>
Compound Name	Response	Retention Time
DDT	1894237	20.72
DDD	5804	20.28
DDE	744	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6548	1900785	0.34

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
 Data File : BM036026.D
 Acq On : 01 Aug 2022 10:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 01 15:49:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 01 15:17:30 2022
 Response via : Initial Calibration

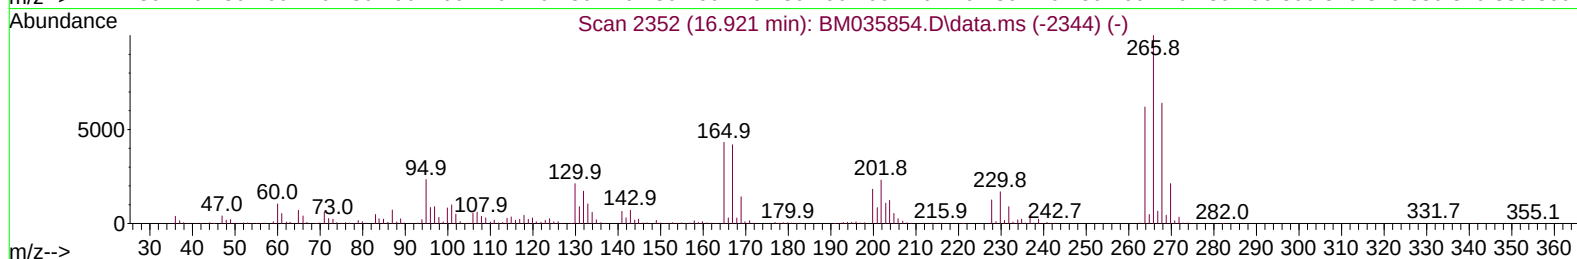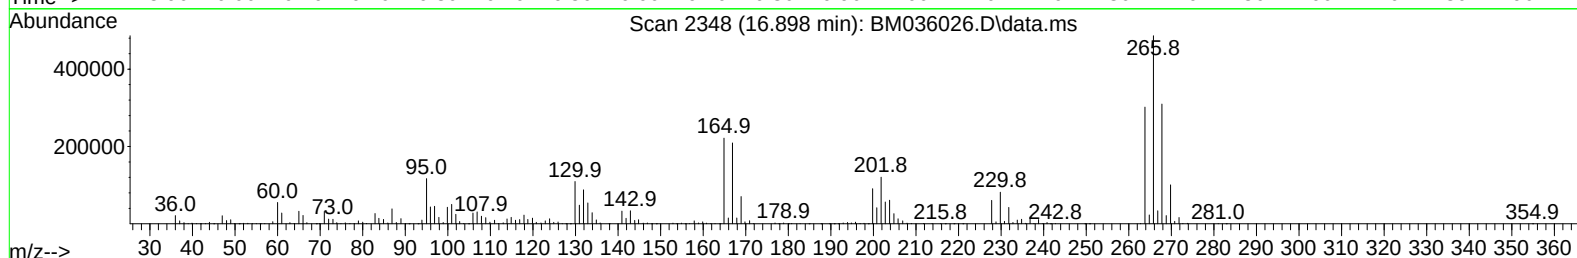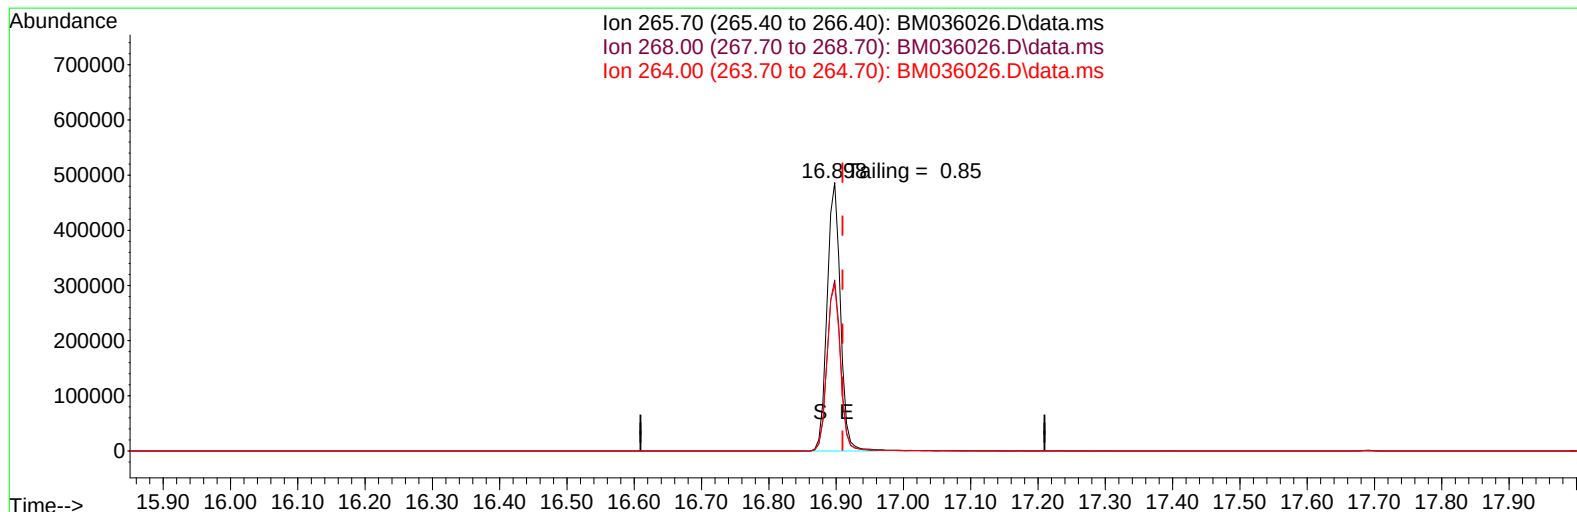

TIC: BM036026.D\data.ms

(70) Pentachlorophenol (C)

16.898min (-0.012) 24533.74 ng




response 670898

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.71
264.00	63.30	62.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080122\
 Data File : BM036026.D
 Acq On : 01 Aug 2022 10:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 01 15:49:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 01 15:17:30 2022
 Response via : Initial Calibration

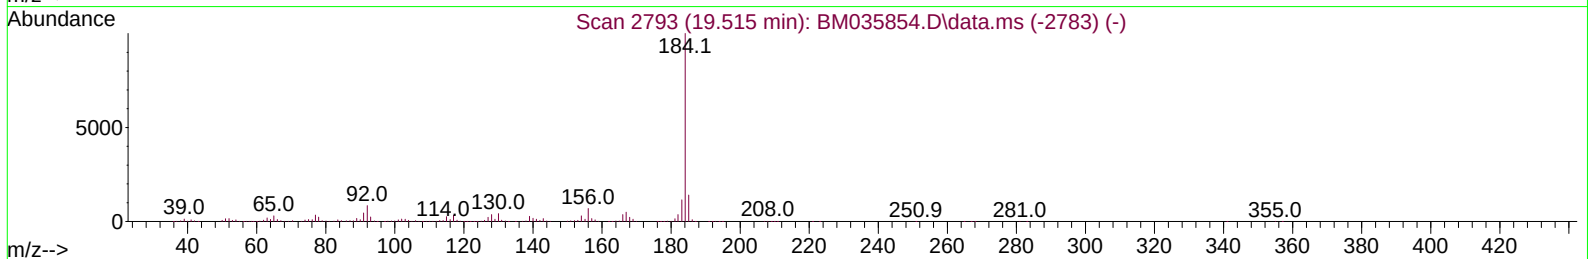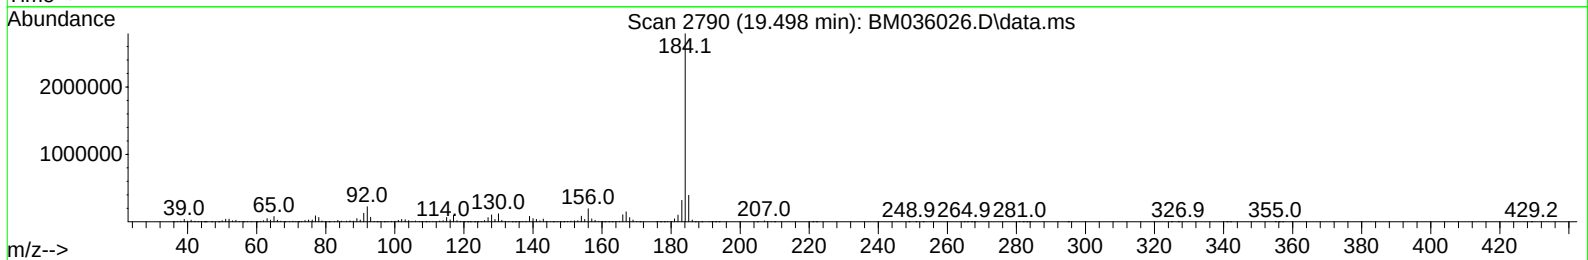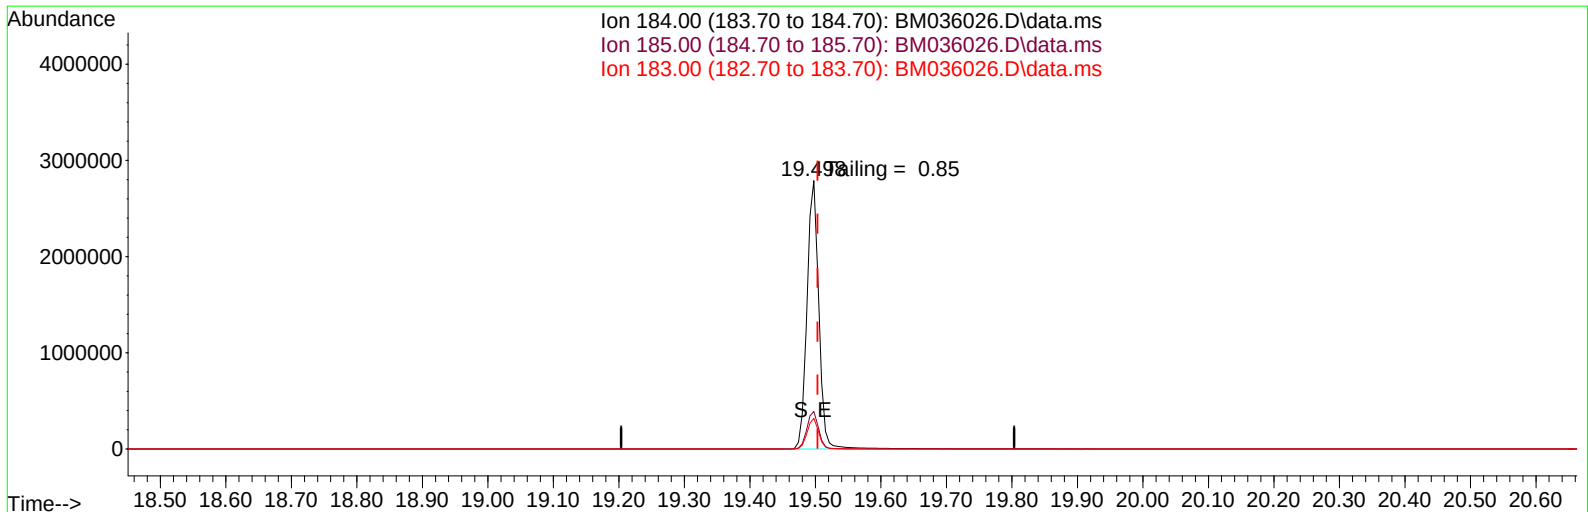

TIC: BM036026.D\data.ms

(77) Benzidine

19.498min (-0.006) 425699.60 ng

response 3490375

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.02
183.00	11.90	11.44
0.00	0.00	0.00