
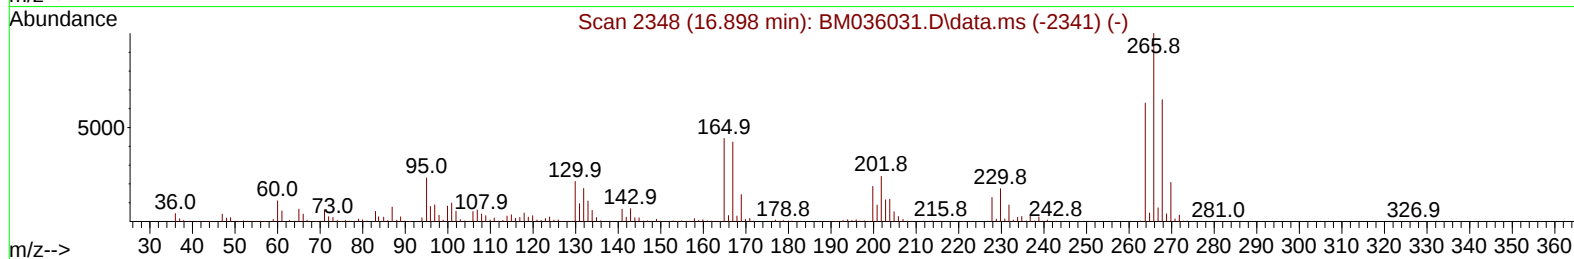
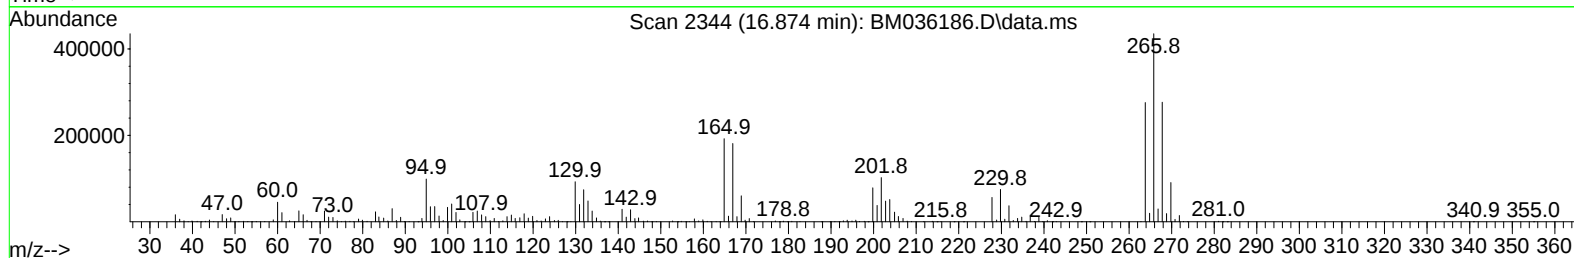


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081022\
Data File : BM036186.D
Acq On : 10 Aug 2022 11:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 03:22:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 10 22:19:26 2022
Response via : Initial Calibration

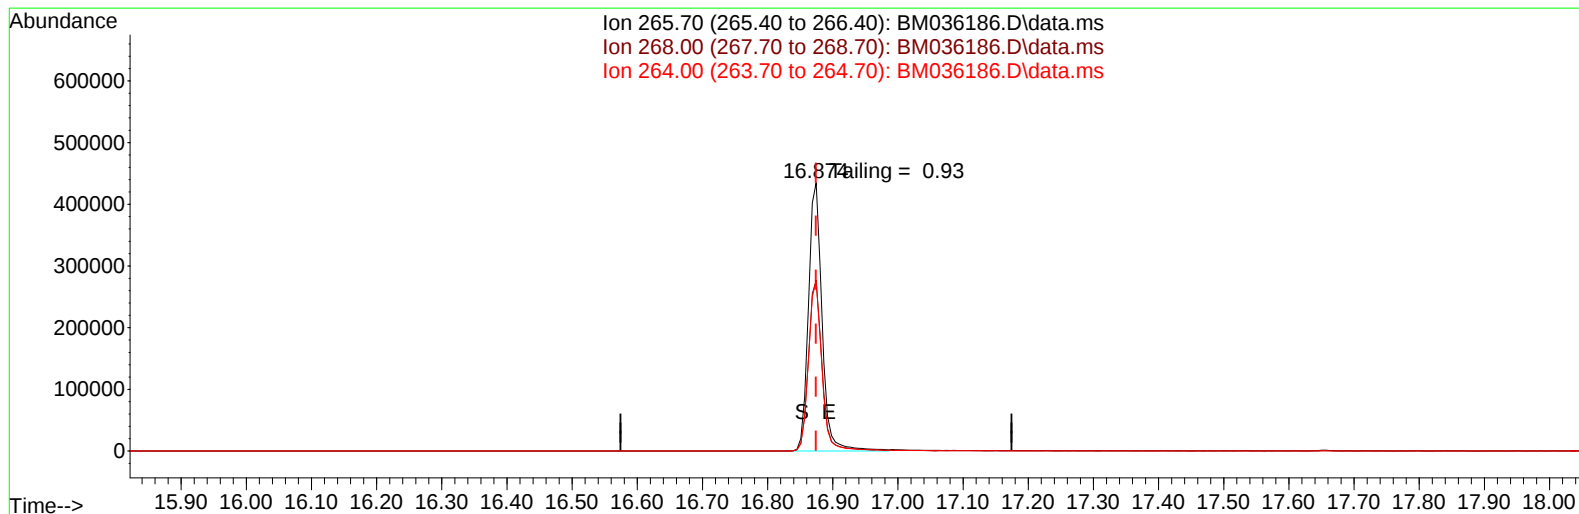

TIC: BM036186.D\data.ms

(70) Pentachlorophenol (C)




16.874min (+ 0.000) 114492.47 ng

response 637975

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.55
264.00	63.30	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081022\
Data File : BM036186.D
Acq On : 10 Aug 2022 11:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 03:22:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 10 22:19:26 2022
Response via : Initial Calibration

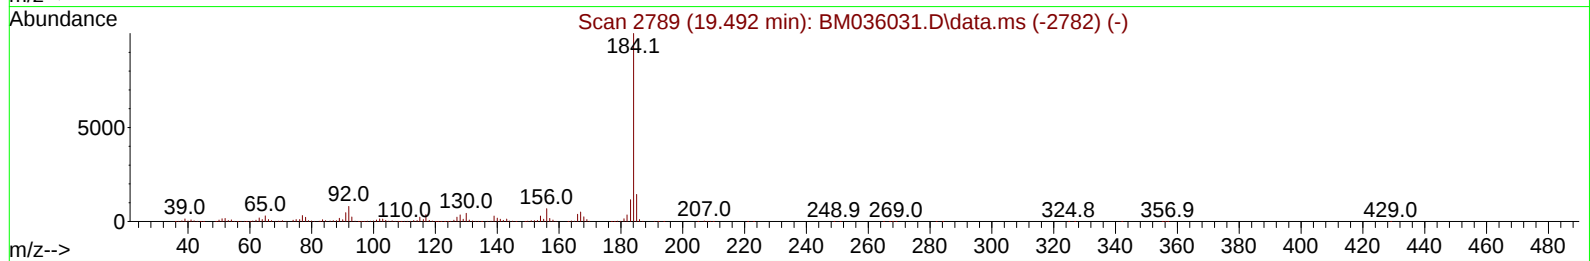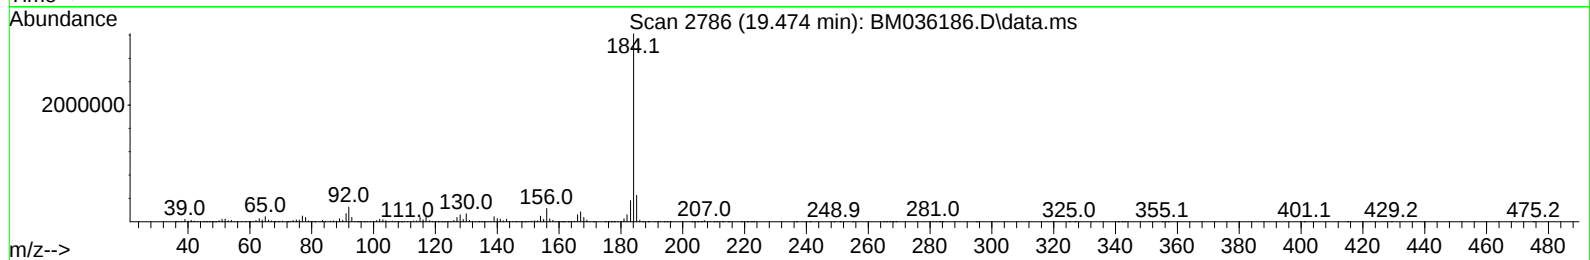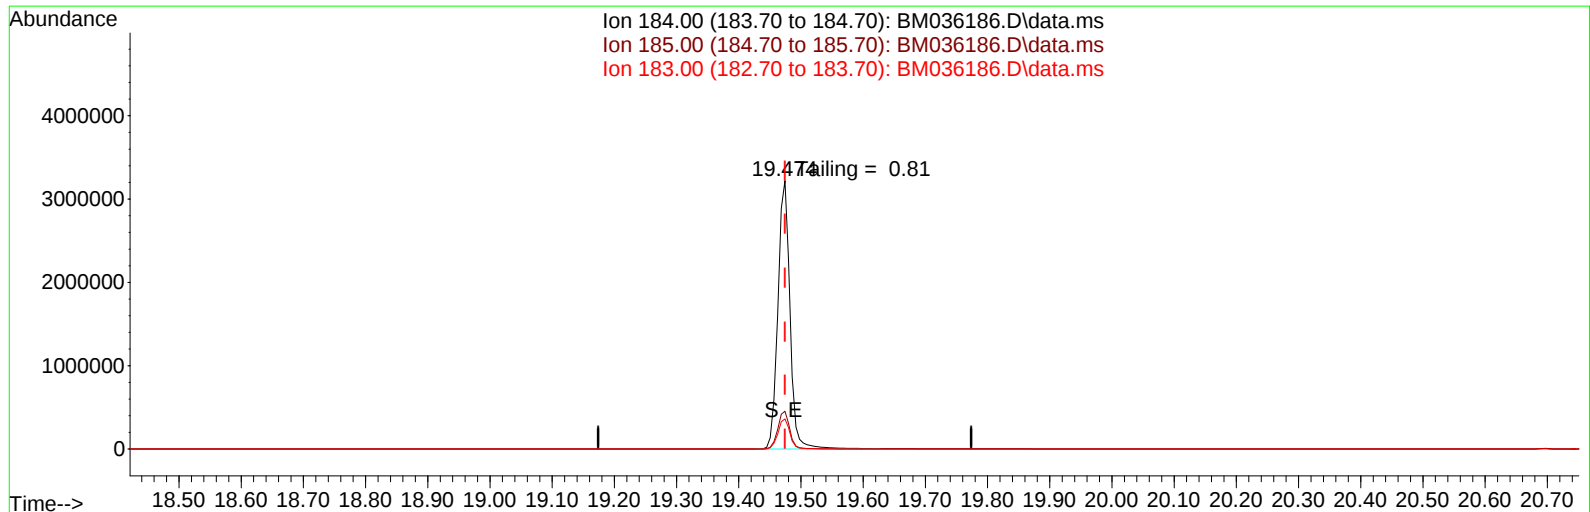

TIC: BM036186.D\data.ms

(77) Benzidine**19.474min (+ 0.000) 110885.74 ng****response 4396863**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.07
183.00	11.90	11.25
0.00	0.00	0.00