

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081022\
 Data File : BM036188.D
 Acq On : 10 Aug 2022 12:31
 Operator : CG/JU
 Sample : PB146851BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB146851BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036188.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.422	390	397	416	rBV	4750244	6960175	66.88%	12.333%
2	7.040	664	672	688	rBV	4505846	7020865	67.46%	12.441%
3	7.834	800	807	817	rBV	897423	1389257	13.35%	2.462%
4	9.004	998	1006	1021	rBV	2754722	4479414	43.04%	7.937%
5	10.639	1276	1284	1297	rBV	1098634	1912976	18.38%	3.390%
6	13.104	1695	1703	1719	rBV	6625869	9366766	90.00%	16.598%
7	14.474	1930	1936	1948	rBV	1529639	2238081	21.50%	3.966%
8	15.968	2183	2190	2205	rBV	4114624	5946335	57.13%	10.537%
9	17.215	2396	2402	2411	rBV	1681437	2330985	22.40%	4.130%
10	19.839	2843	2848	2857	rBV	8333066	10407589	100.00%	18.442%
11	21.398	3108	3113	3118	rBV	1760733	2215705	21.29%	3.926%
12	23.744	3507	3512	3523	rVB2	1129016	2166189	20.81%	3.838%




Sum of corrected areas: 56434337

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081022\
Data File : BM036188.D
Acq On : 10 Aug 2022 12:31
Operator : CG/JU
Sample : PB146851BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146851BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

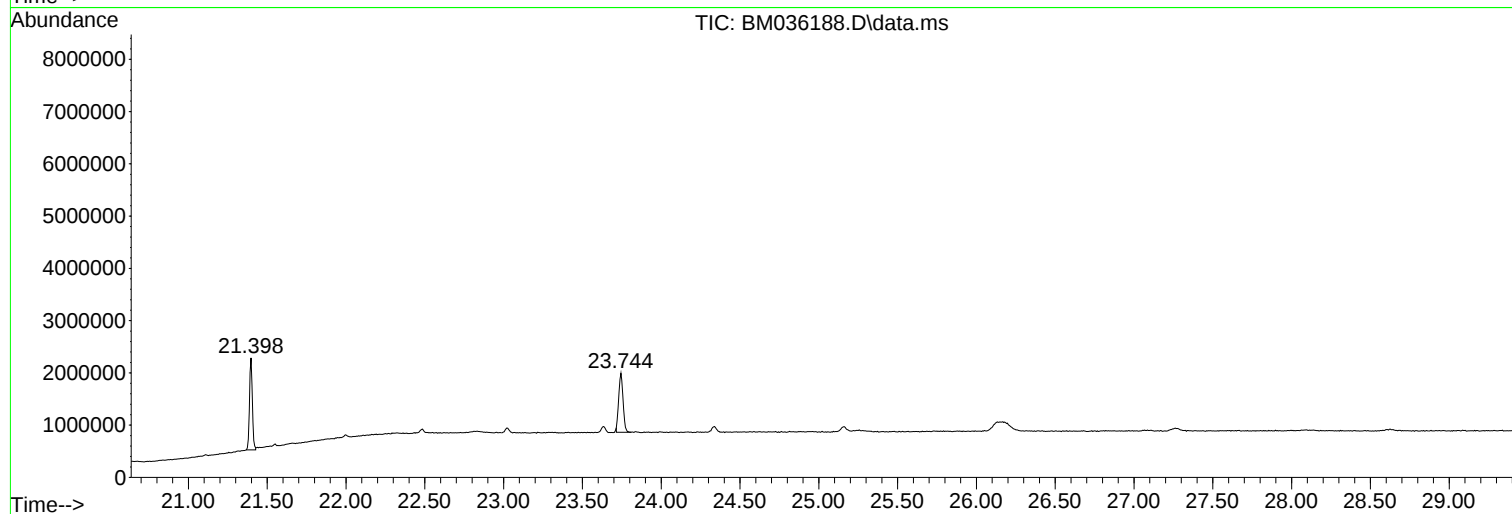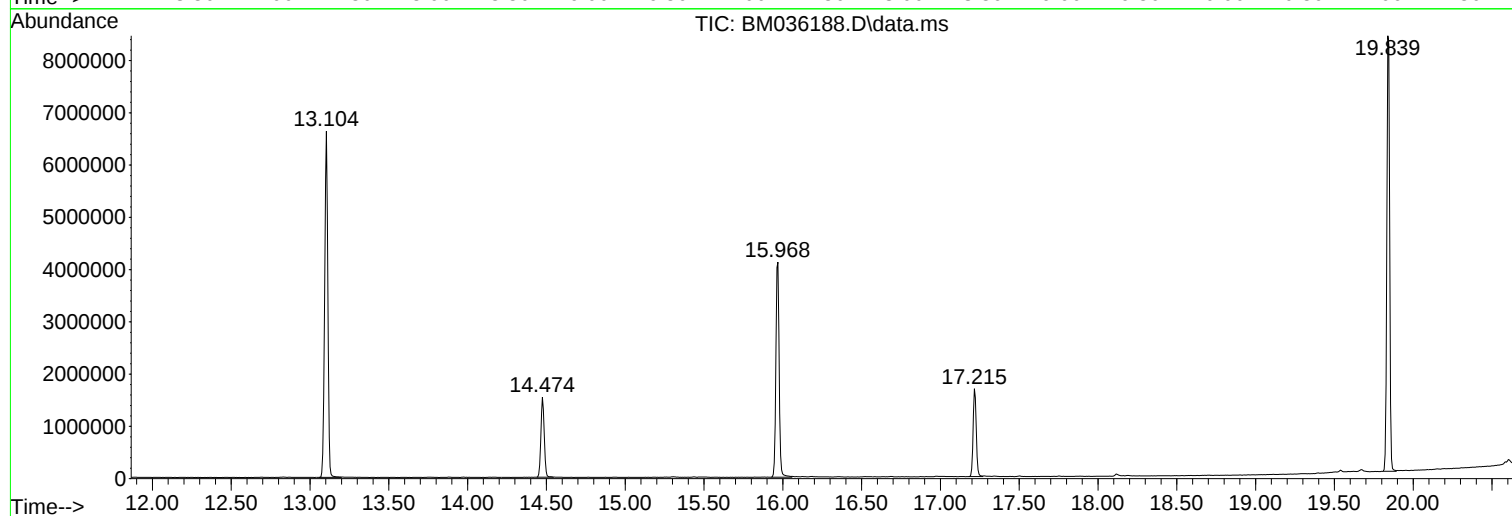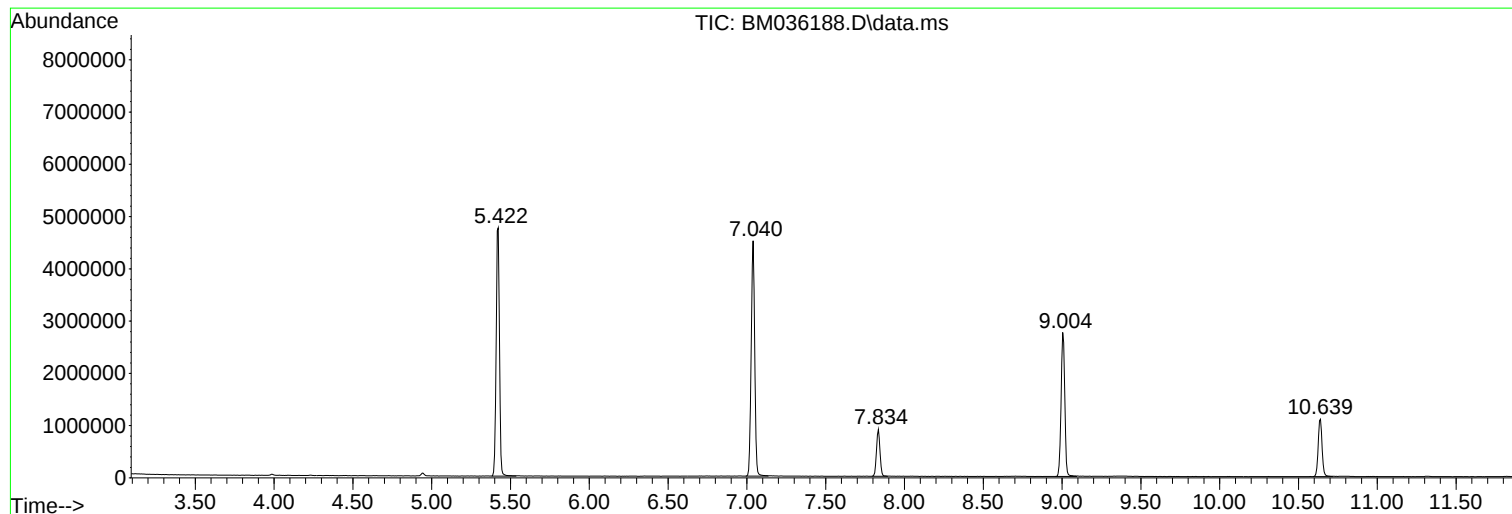

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081022\
Data File : BM036188.D
Acq On : 10 Aug 2022 12:31
Operator : CG/JU
Sample : PB146851BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146851BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081022\
Data File : BM036188.D
Acq On : 10 Aug 2022 12:31
Operator : CG/JU
Sample : PB146851BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146851BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------