


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081022\
 Data File : BM036186.D
 Acq On : 10 Aug 2022 11:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 10 22:19:26 2022

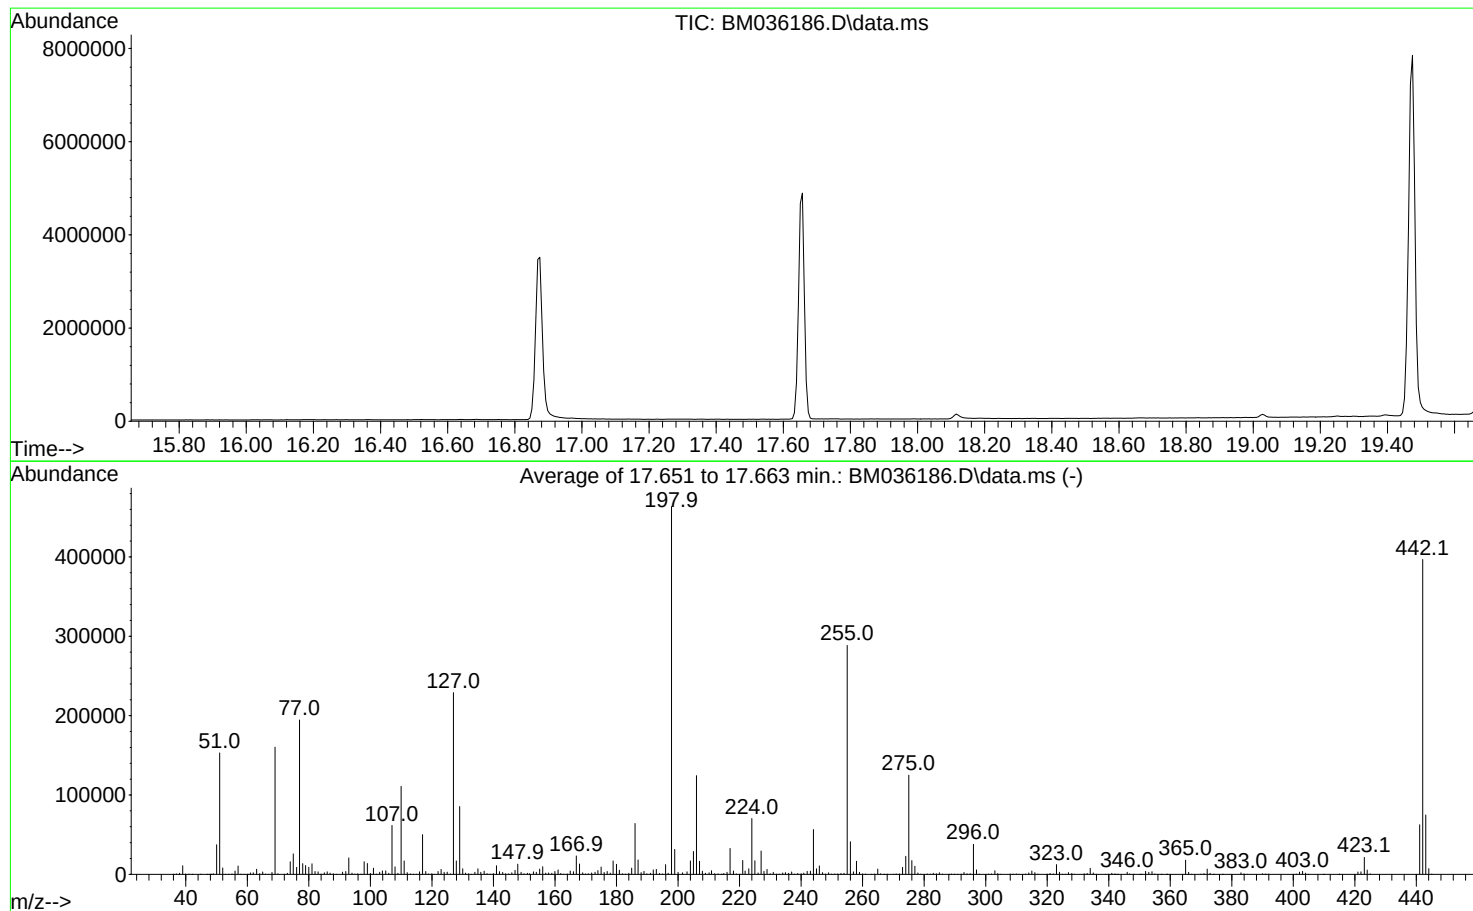




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	153109	PASS
68	69	0.00	2	1.5	2386	PASS
69	198	0.00	100	34.6	160351	PASS
70	69	0.00	2	0.5	808	PASS
127	198	10	80	49.4	229035	PASS
197	198	0.00	2	0.3	1434	PASS
198	198	100	100	100.0	463573	PASS
199	198	5	9	6.8	31557	PASS
275	198	10	60	27.0	124947	PASS
365	198	1	100	3.9	18053	PASS
441	198	0.01	100	13.5	62448	PASS
442	442	50	100	100.0	396779	PASS
443	442	15	24	18.8	74747	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081022\
Data File : BM036186.D
Acq On : 10 Aug 2022 11:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 11 03:22:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 10 22:19:26 2022
Response via : Initial Calibration

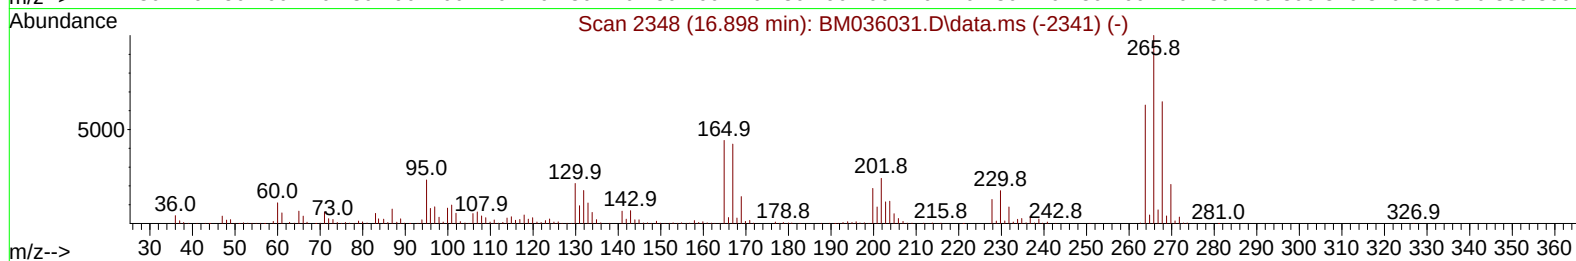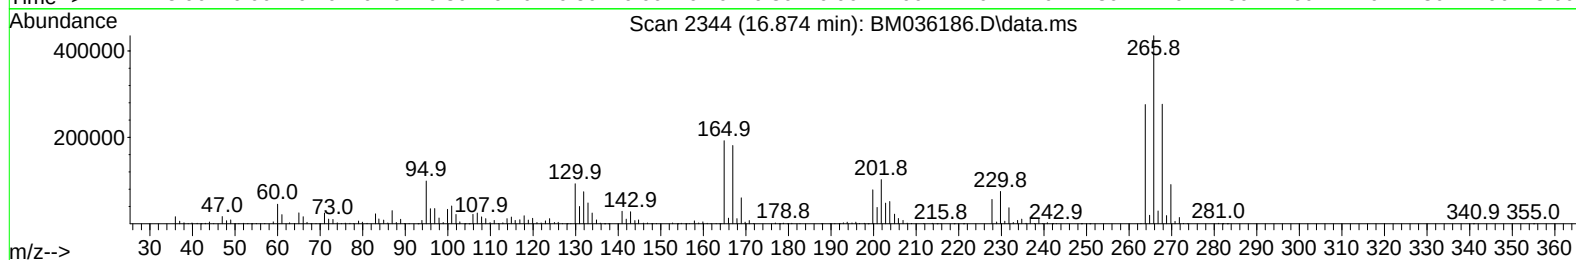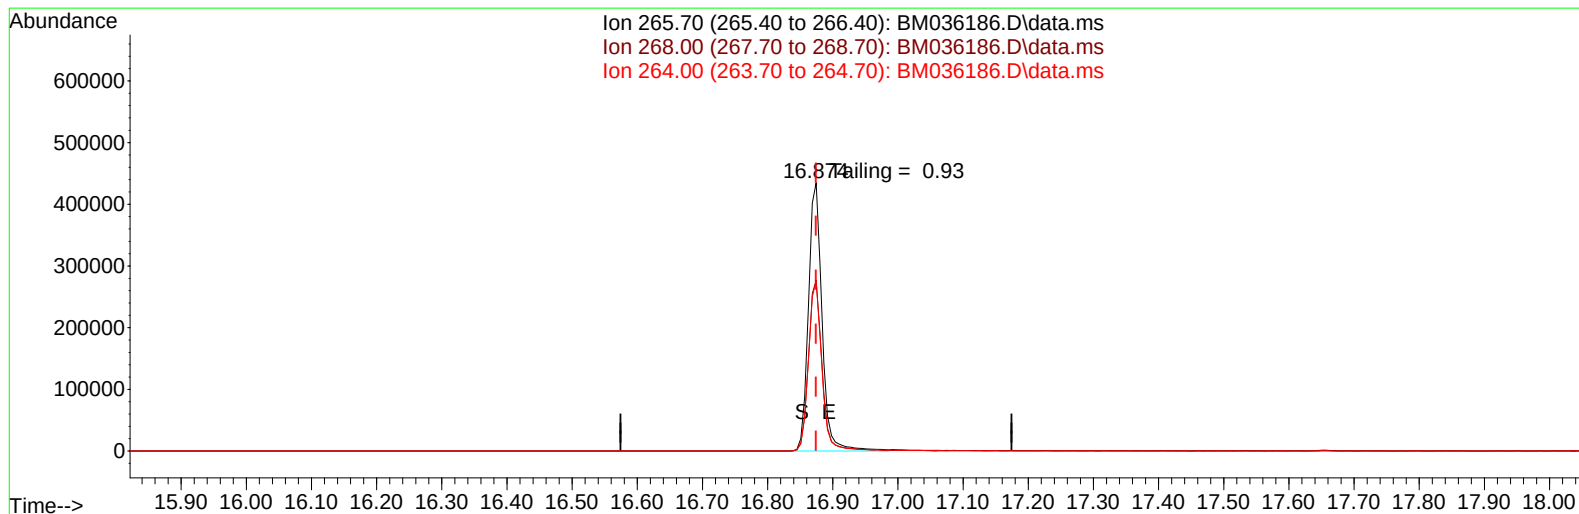

TIC: BM036186.D\data.ms

(70) Pentachlorophenol (C)

16.874min (+ 0.000) 114492.47 ng




response 637975

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.55
264.00	63.30	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081022\
Data File : BM036186.D
Acq On : 10 Aug 2022 11:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 11 03:22:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 10 22:19:26 2022
Response via : Initial Calibration

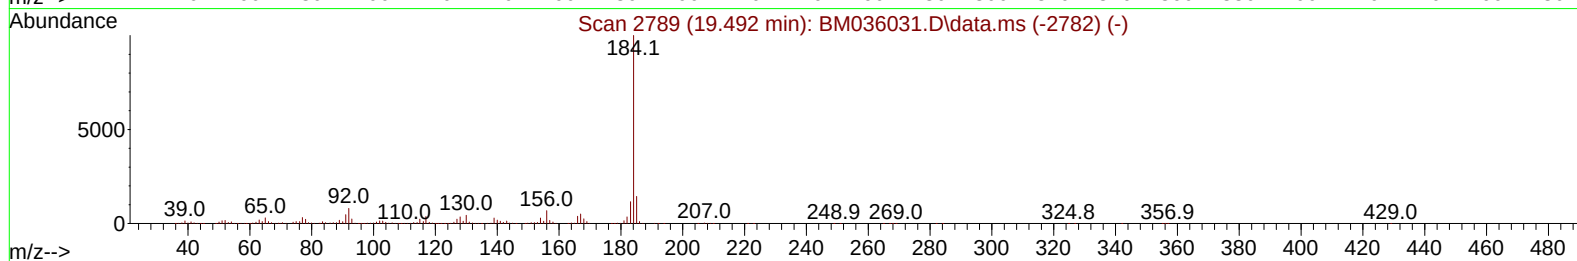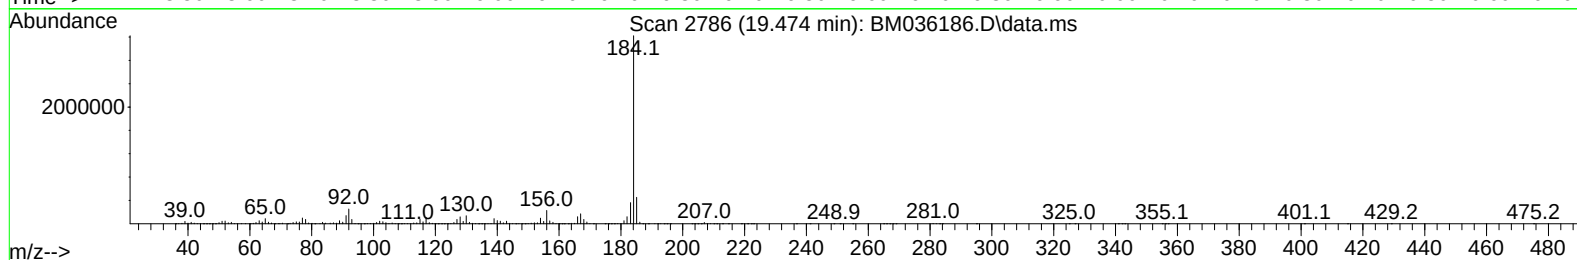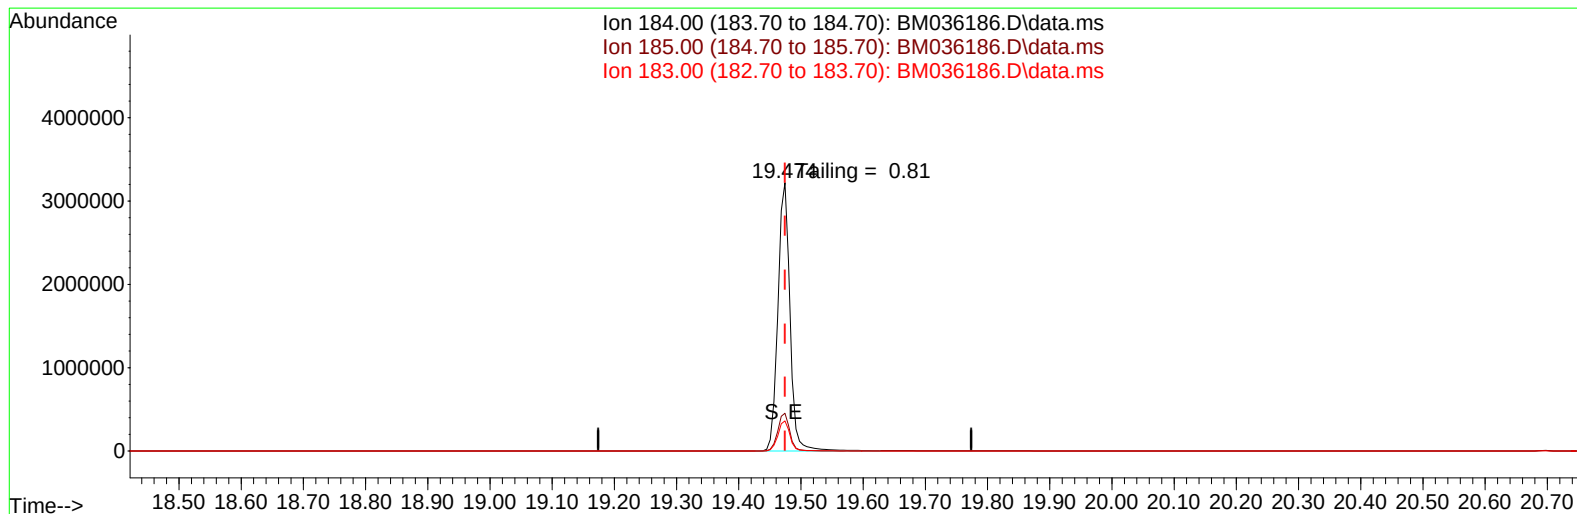

TIC: BM036186.D\data.ms

(77) Benzidine

19.474min (+ 0.000) 110885.74 ng

response 4396863

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.07
183.00	11.90	11.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/10/2022	BNA_M	<u>BM036186.D</u>
Compound Name	Response	Retention Time
DDT	1876336	20.698
DDD	20643	20.257
DDE	2149	19.751
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22792	1899128	1.20

Instrument :
BNA_M
ClientSampleId :
DFTPP