




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036263.D
Acq On : 13 Aug 2022 12:10
Operator : CG/JU
Sample : N4165-07
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBZ5

Manual IntegrationsAPPROVED

Quant Time: Aug 14 23:01:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 11:23:11 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/16/2022
Supervised By :Sohil Jodhani 08/16/2022

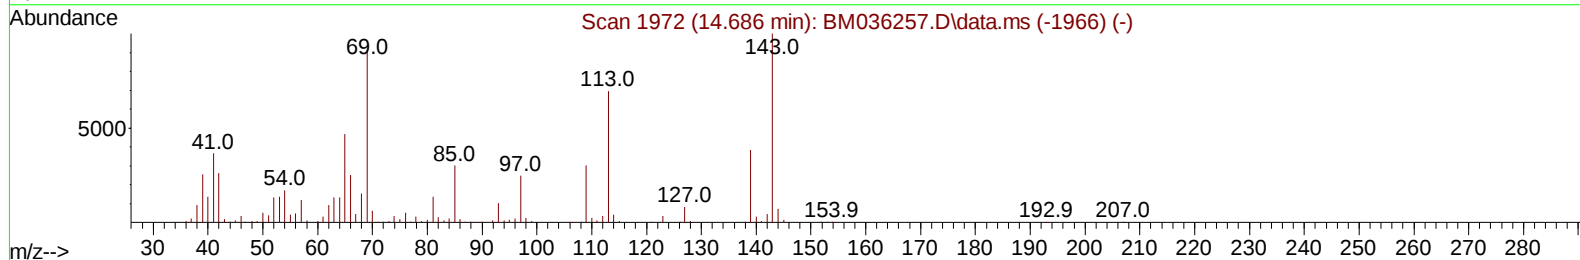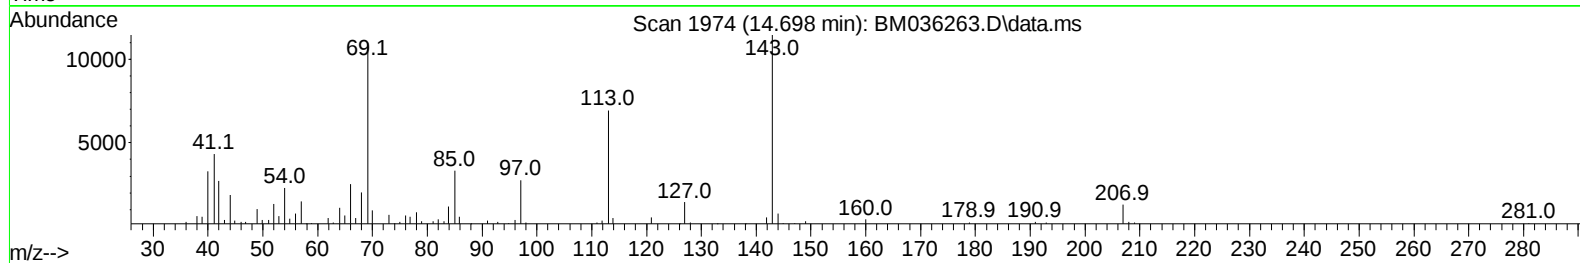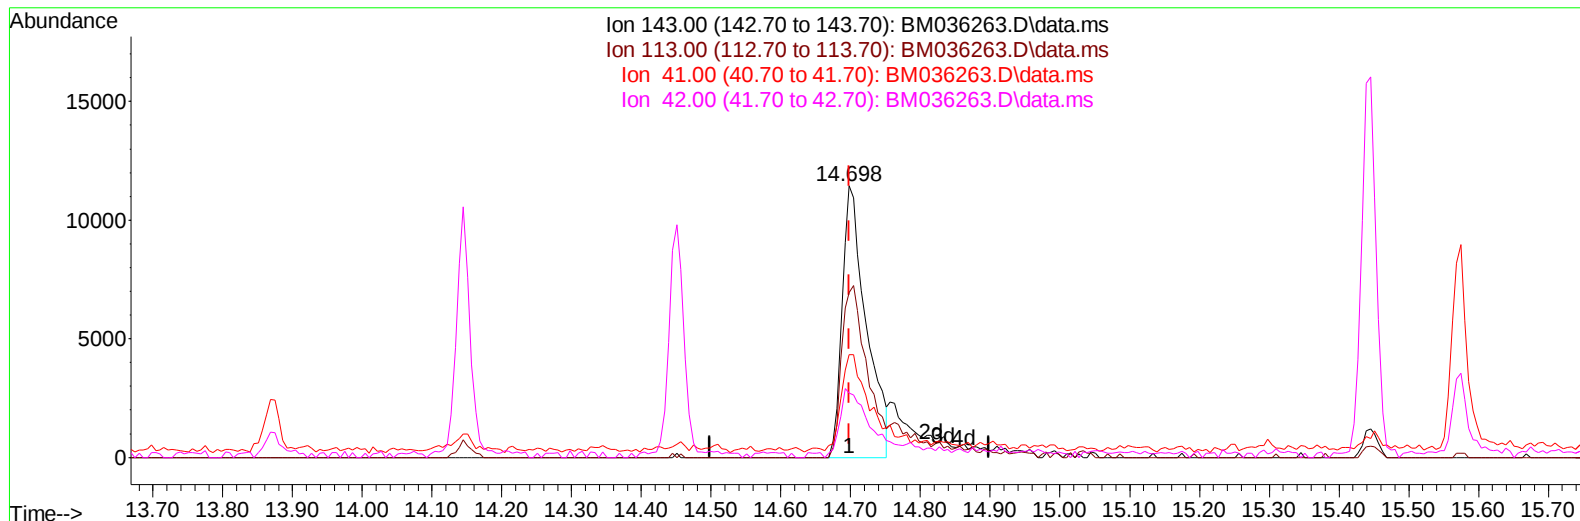

TIC: BM036263.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.698min (-0.000) 3.81 ng/u1

response 27326

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	61.40	60.66
41.00	41.00	37.86
42.00	29.30	23.71




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036263.D
 Acq On : 13 Aug 2022 12:10
 Operator : CG/JU
 Sample : N4165-07
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBZ5

Manual IntegrationsAPPROVED

Quant Time: Aug 14 23:01:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 12 11:23:11 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/16/2022
 Supervised By :Sohil Jodhani 08/16/2022

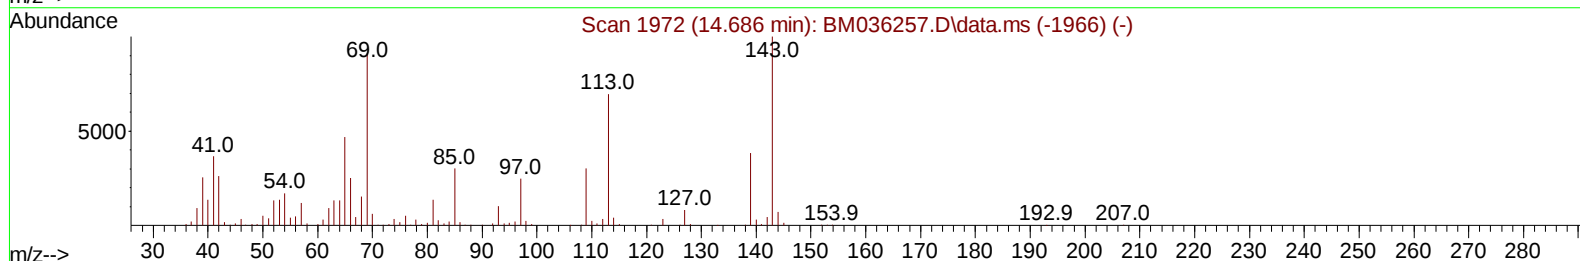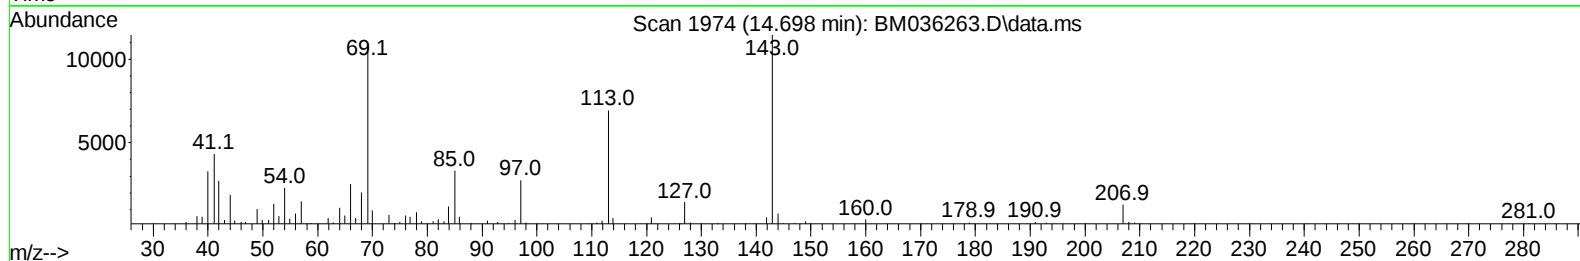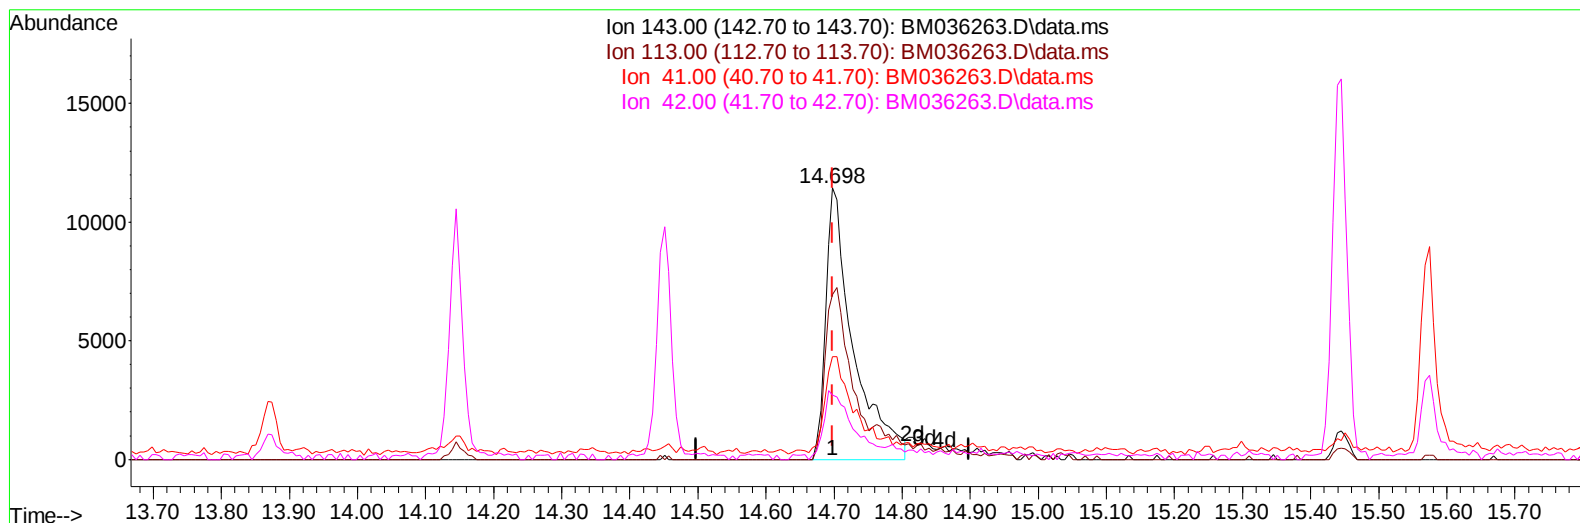

TIC: BM036263.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.698min (-0.000) 4.46 ng/ul m

response 31992

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	61.40	60.66
41.00	41.00	37.86
42.00	29.30	23.71

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036263.D
 Acq On : 13 Aug 2022 12:10
 Operator : CG/JU
 Sample : N4165-07
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBZ5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/16/2022
 Supervised By :Sohil Jodhani 08/16/2022

Quant Time: Aug 14 23:01:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 12 11:23:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	209992	20.000	ng/ul	0.00
20) Naphthalene-d8	10.610	136	882276	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.451	164	512683	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	1078584	20.000	ng/ul	-0.01
79) Chrysene-d12	21.380	240	1176580	20.000	ng/ul	0.00
88) Perylene-d12	23.709	264	1299839	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.216	96	21395	3.834	ng/uL	0.00
4) Pyridine-d5	3.646	84	148665	9.724	ng/ul	0.00
7) Phenol-d5	6.998	99	104980	5.961	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.145	67	331323	28.223	ng/ul	0.00
11) 2-Chlorophenol-d4	7.345	132	323390	22.124	ng/ul	0.00
15) 4-Methylphenol-d8	8.540	113	187218	13.123	ng/ul	-0.01
21) Nitrobenzene-d5	8.981	128	205439	29.385	ng/ul	0.00
24) 2-Nitrophenol-d4	9.698	143	195449	28.695	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.245	165	312149	25.338	ng/ul	0.00
31) 4-Chloroaniline-d4	10.763	131	499223	23.938	ng/ul	0.00
46) Dimethylphthalate-d6	13.874	166	1067346	30.563	ng/ul	0.00
49) Acenaphthylene-d8	14.145	160	1277573	28.672	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.698	143	31992m	4.461	ng/ul	0.00
60) Fluorene-d10	15.445	176	999901	31.685	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.574	200	142606	24.597	ng/ul	0.00
73) Anthracene-d10	17.292	188	1731872	35.516	ng/ul	-0.01
81) Pyrene-d10	19.586	212	2082585	31.937	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.562	264	2348986	35.595	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036263.D
Acq On : 13 Aug 2022 12:10
Operator : CG/JU
Sample : N4165-07
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBZ5

Manual IntegrationsAPPROVED

Quant Time: Aug 14 23:01:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 11:23:11 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/16/2022
Supervised By :Sohil Jodhani 08/16/2022

