

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036225.D
 Acq On : 12 Aug 2022 11:58
 Operator : CG/JU
 Sample : PB146936BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK936

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	18	22	28	rVB	78838	95279	1.53%	0.140%
2	3.646	92	95	113	rBV	671200	992792	15.92%	1.456%
3	3.969	146	150	155	rVB	19206	23777	0.38%	0.035%
4	7.010	659	667	678	rBV	1050045	1661865	26.64%	2.437%
5	7.157	685	692	702	rVB	919806	1429936	22.92%	2.097%
6	7.351	717	725	737	rBV	1078093	1735858	27.83%	2.546%
7	7.816	797	804	813	rBV	1017341	1554694	24.92%	2.280%
8	8.551	921	929	942	rBV	1314731	2154234	34.53%	3.159%
9	8.986	994	1003	1015	rBV	1062288	1718071	27.54%	2.520%
10	9.704	1118	1125	1136	rBV	835879	1435791	23.02%	2.106%
11	10.251	1211	1218	1239	rBV	1200912	2182810	34.99%	3.201%
12	10.622	1272	1281	1290	rBV	1499268	2460590	39.45%	3.608%
13	10.769	1299	1306	1324	rBV	1025303	1851035	29.67%	2.714%
14	12.222	1546	1553	1563	rBV2	20089	43120	0.69%	0.063%
15	12.816	1648	1654	1658	rBV7	5082	9546	0.15%	0.014%
16	13.433	1755	1759	1763	rVB6	5566	8807	0.14%	0.013%
17	13.880	1828	1835	1849	rBV	2599977	3513433	56.32%	5.152%
18	14.157	1873	1882	1895	rBV	2971882	4315054	69.17%	6.328%
19	14.463	1927	1934	1946	rBV	2407627	3462220	55.50%	5.077%
20	14.698	1968	1974	2000	rBV	843557	1563267	25.06%	2.292%
21	14.927	2006	2013	2016	rBV8	4115	10273	0.16%	0.015%
22	15.292	2070	2075	2080	rVB3	6317	11241	0.18%	0.016%
23	15.451	2094	2102	2116	rBV	3846225	5397962	86.53%	7.916%
24	15.580	2118	2124	2140	rVV	965669	1501644	24.07%	2.202%
25	15.692	2140	2143	2150	rVB2	25566	46470	0.74%	0.068%
26	16.168	2221	2224	2228	rBV5	4462	6558	0.11%	0.010%
27	16.233	2232	2235	2240	rBV6	4824	7706	0.12%	0.011%
28	16.509	2278	2282	2285	rBV5	6036	9765	0.16%	0.014%
29	16.668	2307	2309	2316	rVB8	6153	9261	0.15%	0.014%
30	16.880	2342	2345	2350	rVB7	7419	9722	0.16%	0.014%
31	16.962	2355	2359	2361	rBV5	8764	11279	0.18%	0.017%
32	16.992	2361	2364	2369	rVB	7491	12788	0.21%	0.019%
33	17.204	2393	2400	2408	rBV	2938535	3988742	63.94%	5.849%
34	17.304	2410	2417	2431	rVV	4149916	5759481	92.33%	8.446%
35	17.874	2512	2514	2518	rVB5	7333	8219	0.13%	0.012%
36	18.109	2550	2554	2559	rBV5	16255	28910	0.46%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036225.D
Acq On : 12 Aug 2022 11:58
Operator : CG/JU
Sample : PB146936BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK936

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M

Title : SVOA CALIBRATION

37	19.162	2729	2733	2738	rBV2	48087	64177	1.03%	0.094%
38	19.233	2741	2745	2750	rVV	45054	64643	1.04%	0.095%
39	19.598	2801	2807	2816	rBV	4765584	6238008	100.00%	9.148%
40	20.592	2973	2976	2982	rBV2	117086	149468	2.40%	0.219%
41	21.386	3106	3111	3119	rBV	2967379	3757570	60.24%	5.510%
42	23.574	3477	3483	3495	rVB2	2771658	5399834	86.56%	7.919%
43	23.727	3503	3509	3521	rVB2	1761676	3484781	55.86%	5.110%




Sum of corrected areas: 68190681

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036225.D
Acq On : 12 Aug 2022 11:58
Operator : CG/JU
Sample : PB146936BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK936

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

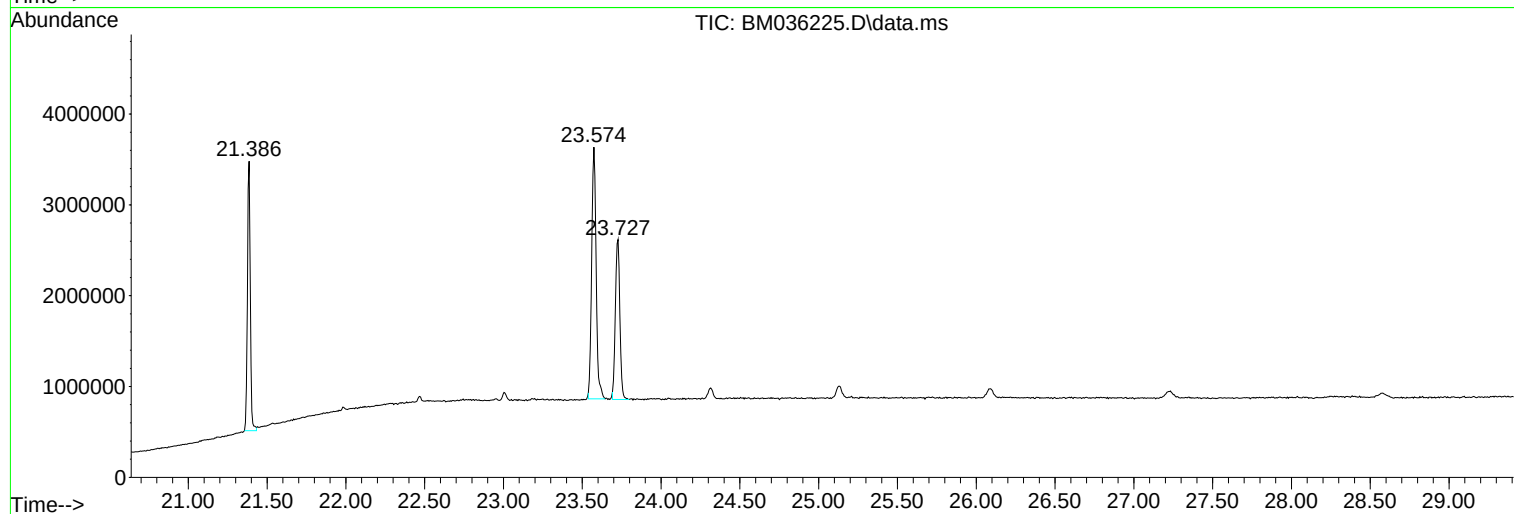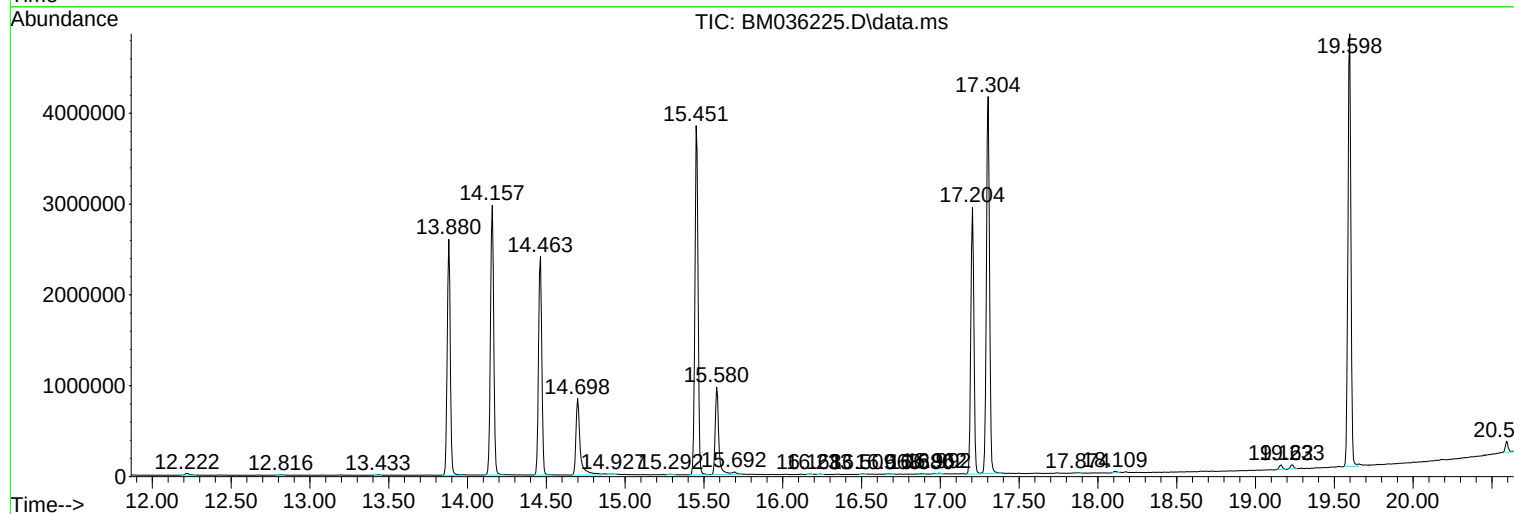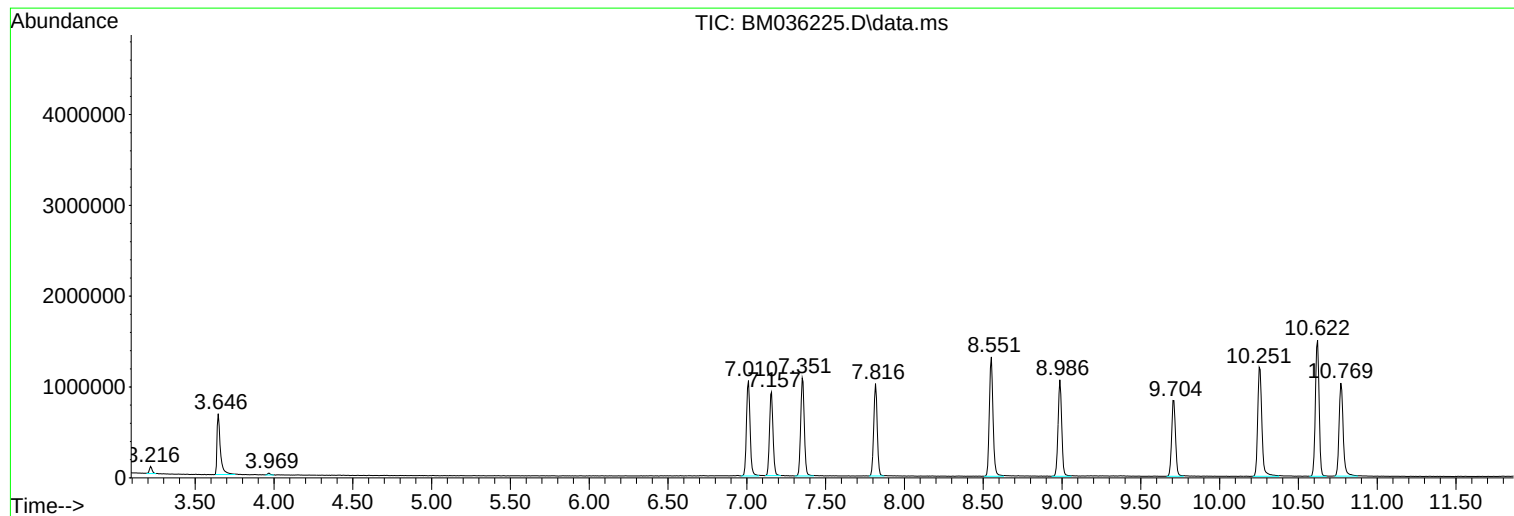

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036225.D
Acq On : 12 Aug 2022 11:58
Operator : CG/JU
Sample : PB146936BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK936

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036225.D
Acq On : 12 Aug 2022 11:58
Operator : CG/JU
Sample : PB146936BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK936

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc