

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036227.D
 Acq On : 12 Aug 2022 13:12
 Operator : CG/JU
 Sample : N4129-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036227.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	18	22	31	rVB	87015	111566	1.27%	0.126%
2	3.646	92	95	112	rBV	427735	651745	7.42%	0.733%
3	3.875	128	134	140	rVB	38236	54673	0.62%	0.062%
4	3.969	146	150	156	rVB	22539	30991	0.35%	0.035%
5	4.416	222	226	234	rVB	78993	102752	1.17%	0.116%
6	4.904	305	309	312	rBV	7445	9203	0.10%	0.010%
7	5.028	324	330	334	rVB4	11314	17411	0.20%	0.020%
8	6.934	649	654	660	rBV	45840	66514	0.76%	0.075%
9	7.010	660	667	677	rBV	321415	526722	5.99%	0.593%
10	7.157	685	692	702	rBV	1321300	2080153	23.67%	2.340%
11	7.351	718	725	735	rBV	1249449	1979100	22.52%	2.227%
12	7.428	735	738	743	rVB	13493	17071	0.19%	0.019%
13	7.816	797	804	813	rBV	1289877	1974878	22.48%	2.222%
14	7.887	813	816	820	rVB5	7825	11558	0.13%	0.013%
15	8.551	922	929	943	rBV	990788	1619889	18.44%	1.822%
16	8.987	995	1003	1010	rBV	1590651	2541601	28.93%	2.859%
17	9.039	1010	1012	1019	rVB4	16018	22574	0.26%	0.025%
18	9.139	1024	1029	1036	rBV6	11489	28686	0.33%	0.032%
19	9.381	1065	1070	1076	rVB	48786	72385	0.82%	0.081%
20	9.710	1117	1126	1140	rBV	1225843	2073045	23.59%	2.332%
21	10.251	1211	1218	1243	rBV	1668278	2953579	33.61%	3.323%
22	10.622	1269	1281	1292	rBV	1864842	3068449	34.92%	3.452%
23	10.769	1296	1306	1323	rBV	1695212	2978408	33.90%	3.351%
24	11.816	1477	1484	1487	rBV8	4749	9550	0.11%	0.011%
25	11.875	1490	1494	1499	rVB	32524	50217	0.57%	0.056%
26	12.039	1517	1522	1532	rVB2	31164	50604	0.58%	0.057%
27	12.216	1547	1552	1560	rBV2	30660	56160	0.64%	0.063%
28	12.822	1651	1655	1659	rVV4	14172	24781	0.28%	0.028%
29	12.857	1659	1661	1667	rVB7	9211	11694	0.13%	0.013%
30	13.075	1690	1698	1703	rBV3	12240	20077	0.23%	0.023%
31	13.280	1729	1733	1740	rVB	51102	70393	0.80%	0.079%
32	13.439	1756	1760	1765	rVB5	8621	17588	0.20%	0.020%
33	13.686	1797	1802	1808	rBV8	8805	15886	0.18%	0.018%
34	13.880	1828	1835	1849	rVV	3740834	4974938	56.62%	5.597%
35	13.980	1849	1852	1857	rVB6	11378	15039	0.17%	0.017%
36	14.157	1869	1882	1891	rBV	4300274	6154841	70.05%	6.925%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036227.D
 Acq On : 12 Aug 2022 13:12
 Operator : CG/JU
 Sample : N4129-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	14.357	1910	1916	1923	rBV	70828	96673	1.10%	0.109%
38	14.463	1925	1934	1950	rBV	2848948	4156275	47.30%	4.676%
39	14.704	1968	1975	1990	rBV	171380	396757	4.52%	0.446%
40	14.898	2005	2008	2015	rVV8	10945	21479	0.24%	0.024%
41	14.974	2018	2021	2025	rVV6	8270	11841	0.13%	0.013%
42	15.257	2063	2069	2071	rBV2	8315	12441	0.14%	0.014%
43	15.304	2071	2077	2084	rVB2	67318	101560	1.16%	0.114%
44	15.451	2092	2102	2116	rBV	5248278	7638165	86.93%	8.593%
45	15.580	2118	2124	2138	rVV	1491622	2130941	24.25%	2.397%
46	15.692	2139	2143	2151	rVB2	61621	105557	1.20%	0.119%
47	15.863	2169	2172	2178	rVV8	7124	8997	0.10%	0.010%
48	15.927	2179	2183	2187	rVB7	7250	10387	0.12%	0.012%
49	16.021	2194	2199	2203	rBV7	8430	13265	0.15%	0.015%
50	16.168	2220	2224	2232	rVV2	87597	142420	1.62%	0.160%
51	16.239	2232	2236	2240	rVB4	19723	28929	0.33%	0.033%
52	16.510	2276	2282	2286	rBV7	11073	25019	0.28%	0.028%
53	16.574	2289	2293	2298	rVB7	8982	14994	0.17%	0.017%
54	16.627	2298	2302	2305	rBV6	7917	10487	0.12%	0.012%
55	16.668	2305	2309	2315	rVV4	33229	47920	0.55%	0.054%
56	16.880	2342	2345	2350	rVB7	8298	13948	0.16%	0.016%
57	16.963	2354	2359	2363	rBV	70575	104163	1.19%	0.117%
58	17.204	2393	2400	2409	rBV	3317892	4571486	52.03%	5.143%
59	17.304	2410	2417	2429	rVB	5825082	8044524	91.55%	9.051%
60	17.492	2446	2449	2455	rVB7	12962	24059	0.27%	0.027%
61	17.698	2480	2484	2488	rBV	56537	70709	0.80%	0.080%
62	17.739	2488	2491	2496	rVB3	24043	33849	0.39%	0.038%
63	17.874	2510	2514	2522	rVB	67076	93040	1.06%	0.105%
64	18.104	2548	2553	2558	rBV	51646	85735	0.98%	0.096%
65	18.174	2562	2565	2572	rVB	22696	36422	0.41%	0.041%
66	18.392	2598	2602	2607	rVB	47804	56766	0.65%	0.064%
67	18.686	2649	2652	2655	rVB2	19770	24670	0.28%	0.028%
68	19.021	2705	2709	2712	rBV2	88000	114001	1.30%	0.128%
69	19.051	2712	2714	2720	rVB4	55753	62990	0.72%	0.071%
70	19.162	2729	2733	2740	rVB2	63505	99742	1.14%	0.112%
71	19.233	2741	2745	2751	rBV	65077	92938	1.06%	0.105%
72	19.598	2801	2807	2814	rBV	6664564	8786697	100.00%	9.886%
73	20.598	2974	2977	2980	rVB	127846	137118	1.56%	0.154%
74	21.098	3059	3062	3069	rBV	177630	256622	2.92%	0.289%
75	21.386	3106	3111	3119	rBV	3495642	4389634	49.96%	4.939%
76	23.574	3476	3483	3500	rVB2	4002292	8158163	92.85%	9.178%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036227.D
Acq On : 12 Aug 2022 13:12
Operator : CG/JU
Sample : N4129-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBW1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Title : SVOA CALIBRATION

77 23.727 3503 3509 3520 rVB2 2200226 4188148 47.66% 4.712%




Sum of corrected areas: 88884252

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036227.D
Acq On : 12 Aug 2022 13:12
Operator : CG/JU
Sample : N4129-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBW1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

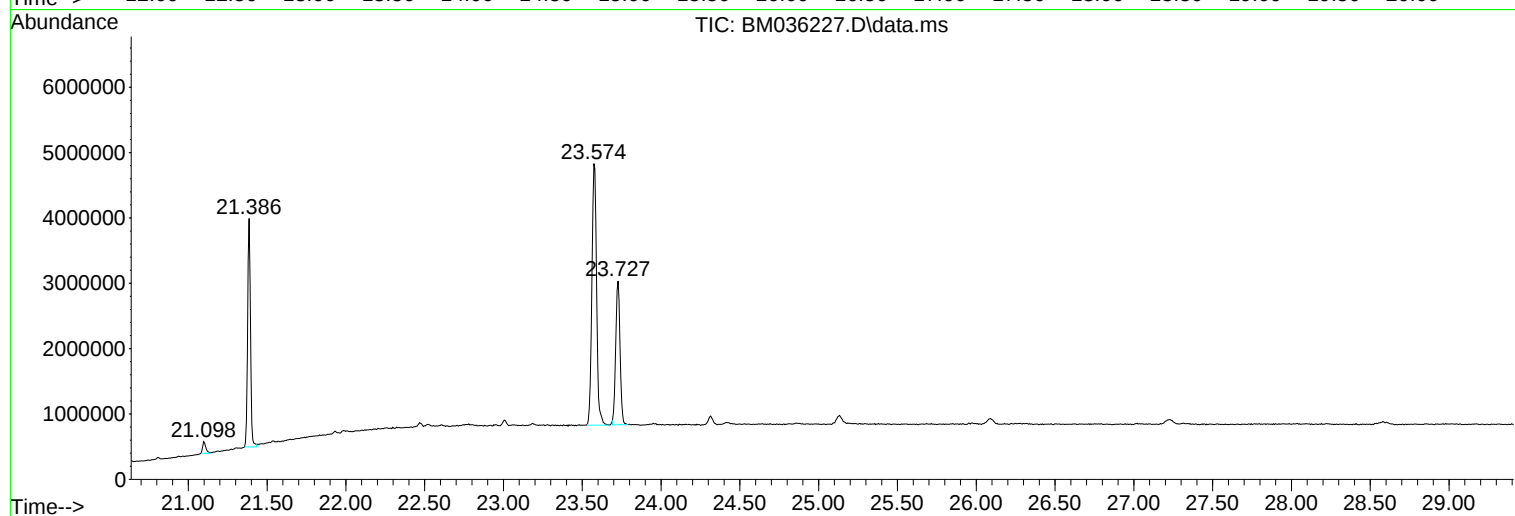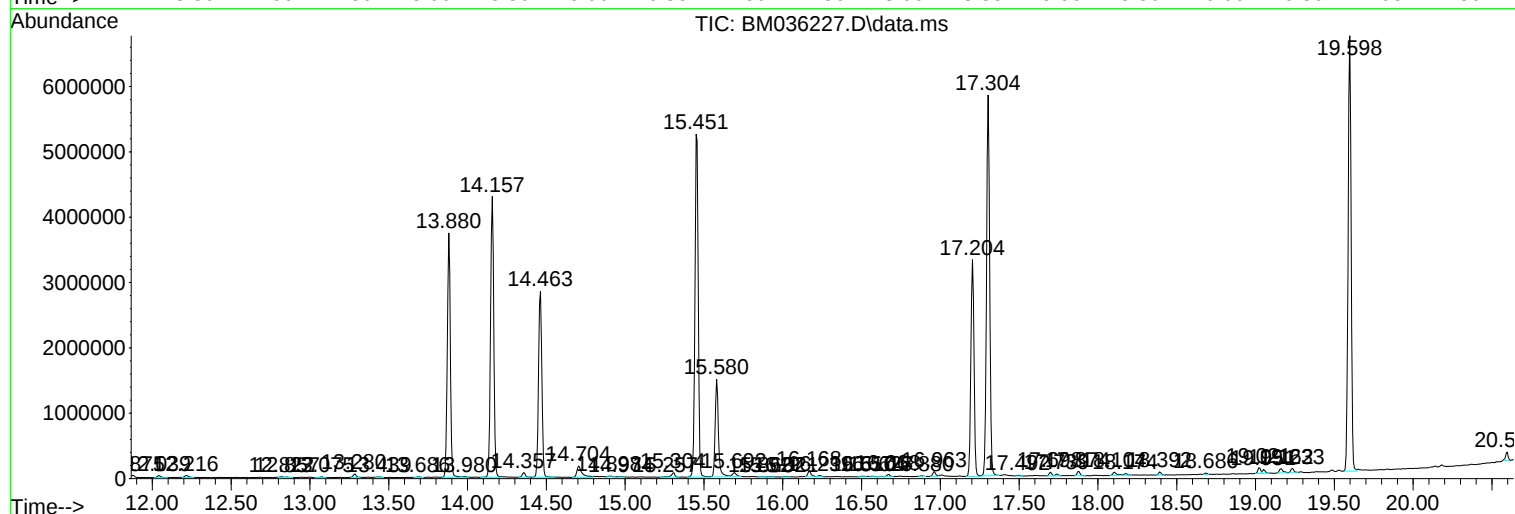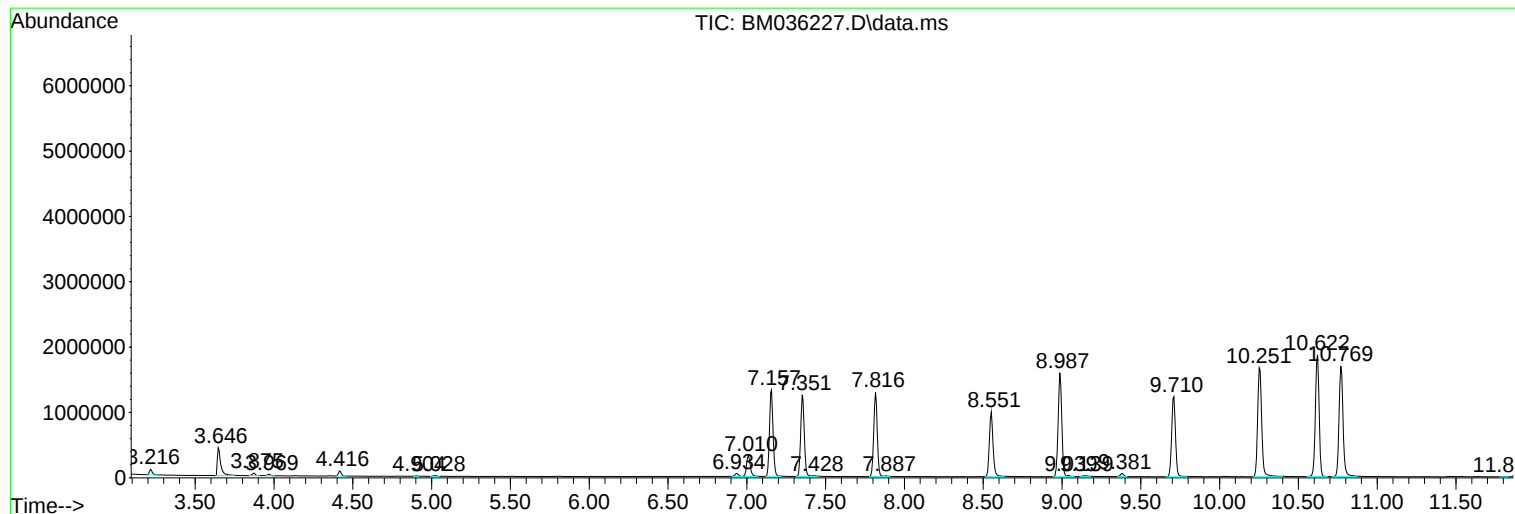

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036227.D
Acq On : 12 Aug 2022 13:12
Operator : CG/JU
Sample : N4129-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBW1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036227.D
Acq On : 12 Aug 2022 13:12
Operator : CG/JU
Sample : N4129-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBW1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc