

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036229.D
 Acq On : 12 Aug 2022 14:25
 Operator : CG/JU
 Sample : N4129-16
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	18	22	27	rVB	64254	75520	1.34%	0.135%
2	3.658	94	97	116	rVB	126066	205975	3.66%	0.367%
3	3.869	129	133	139	rVB	22110	33744	0.60%	0.060%
4	3.969	146	150	155	rVB	46029	62298	1.11%	0.111%
5	4.416	222	226	232	rVB	42440	58915	1.05%	0.105%
6	5.022	327	329	334	rVB4	7011	8318	0.15%	0.015%
7	6.934	648	654	661	rVB	24469	36972	0.66%	0.066%
8	7.010	661	667	676	rBV	155216	266521	4.73%	0.475%
9	7.151	685	691	704	rBV	794521	1264997	22.46%	2.257%
10	7.351	718	725	735	rBV	702439	1136561	20.18%	2.027%
11	7.422	735	737	746	rVB8	8371	16502	0.29%	0.029%
12	7.816	796	804	813	rBV	995259	1537114	27.29%	2.742%
13	8.551	922	929	942	rBV	480286	837461	14.87%	1.494%
14	8.987	995	1003	1016	rBV	930123	1526156	27.09%	2.722%
15	9.381	1065	1070	1076	rVB	25465	41313	0.73%	0.074%
16	9.710	1116	1126	1141	rBV	664414	1173201	20.83%	2.093%
17	9.810	1141	1143	1151	rVB8	2938	6053	0.11%	0.011%
18	10.251	1211	1218	1232	rBV	887040	1625744	28.86%	2.900%
19	10.622	1272	1281	1288	rBV	1334038	2251473	39.97%	4.016%
20	10.769	1299	1306	1323	rBV	931938	1716161	30.47%	3.061%
21	11.804	1475	1482	1488	rBV	3172	6736	0.12%	0.012%
22	11.875	1488	1494	1500	rVB2	16672	27600	0.49%	0.049%
23	12.222	1547	1553	1559	rBV3	15662	34127	0.61%	0.061%
24	12.680	1626	1631	1636	rBV8	2766	5733	0.10%	0.010%
25	12.816	1651	1654	1660	rVB7	4814	7483	0.13%	0.013%
26	13.363	1741	1747	1752	rBV4	15096	23204	0.41%	0.041%
27	13.445	1755	1761	1763	rBV5	5908	11180	0.20%	0.020%
28	13.880	1828	1835	1846	rBV	2076237	2877058	51.08%	5.132%
29	14.157	1874	1882	1893	rBV	2437032	3592965	63.79%	6.409%
30	14.357	1912	1916	1919	rVB4	5804	7420	0.13%	0.013%
31	14.463	1926	1934	1945	rBV	1950738	2909303	51.65%	5.190%
32	14.710	1969	1976	1994	rBV2	54844	175255	3.11%	0.313%
33	14.904	2006	2009	2010	rBV2	6543	6642	0.12%	0.012%
34	15.298	2071	2076	2081	rVB2	9019	18908	0.34%	0.034%
35	15.451	2093	2102	2117	rBV	3242656	4546021	80.71%	8.109%
36	15.580	2118	2124	2139	rVV	768021	1165486	20.69%	2.079%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036229.D
 Acq On : 12 Aug 2022 14:25
 Operator : CG/JU
 Sample : N4129-16
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	15.692	2139	2143	2151	rVB2	34738	63160	1.12%	0.113%
38	15.868	2168	2173	2176	rVB7	4060	6773	0.12%	0.012%
39	16.163	2221	2223	2227	rBV3	9430	9049	0.16%	0.016%
40	16.233	2232	2235	2240	rVB6	11432	14083	0.25%	0.025%
41	16.674	2306	2310	2314	rVB2	14901	21614	0.38%	0.039%
42	16.880	2343	2345	2350	rVB6	6986	7958	0.14%	0.014%
43	16.957	2355	2358	2362	rBV2	14081	22405	0.40%	0.040%
44	17.204	2394	2400	2408	rBV	2313468	3235633	57.44%	5.772%
45	17.304	2410	2417	2428	rVV	3518982	4942505	87.75%	8.817%
46	17.498	2447	2450	2452	rBV3	5125	5955	0.11%	0.011%
47	17.704	2481	2485	2487	rBV4	7796	9374	0.17%	0.017%
48	17.739	2488	2491	2495	rVB2	12660	14524	0.26%	0.026%
49	18.104	2549	2553	2558	rBV3	36014	55772	0.99%	0.099%
50	18.174	2563	2565	2572	rVB2	12448	17256	0.31%	0.031%
51	18.686	2649	2652	2655	rVB5	9458	12081	0.21%	0.022%
52	19.162	2729	2733	2737	rBV2	47157	63998	1.14%	0.114%
53	19.233	2742	2745	2752	rVV2	37550	53996	0.96%	0.096%
54	19.480	2785	2787	2790	rBV4	16203	18869	0.33%	0.034%
55	19.527	2793	2795	2799	rBV4	16703	17677	0.31%	0.032%
56	19.598	2801	2807	2815	rBV	4059084	5539971	98.35%	9.882%
57	20.598	2974	2977	2981	rVB	109875	120456	2.14%	0.215%
58	21.386	3106	3111	3120	rBV	2698510	3479995	61.78%	6.208%
59	23.574	3477	3483	3496	rVB2	2876469	5632757	100.00%	10.048%
60	23.727	3503	3509	3521	rVB2	1728826	3396613	60.30%	6.059%




Sum of corrected areas: 56058594

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036229.D
Acq On : 12 Aug 2022 14:25
Operator : CG/JU
Sample : N4129-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBW8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

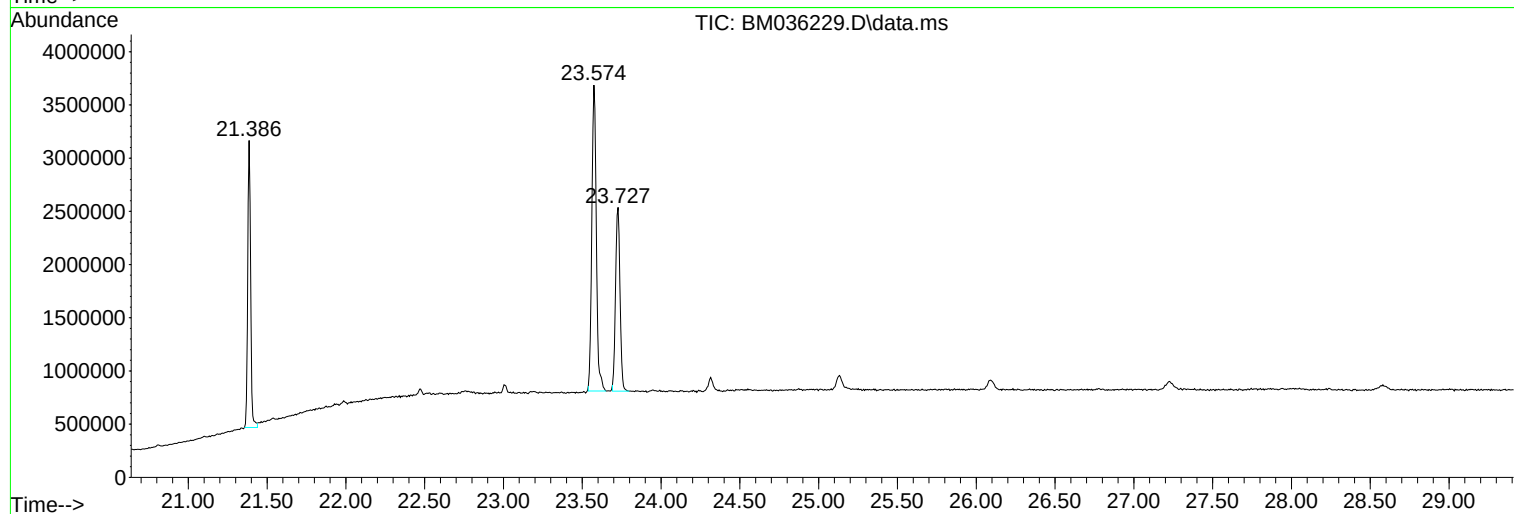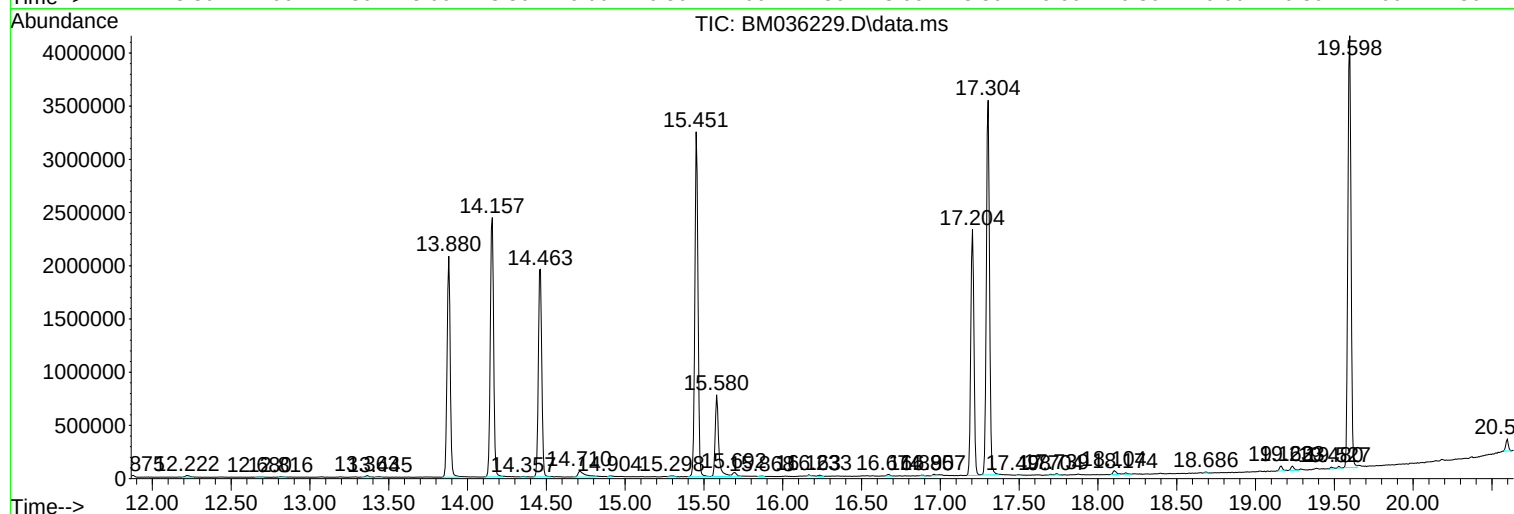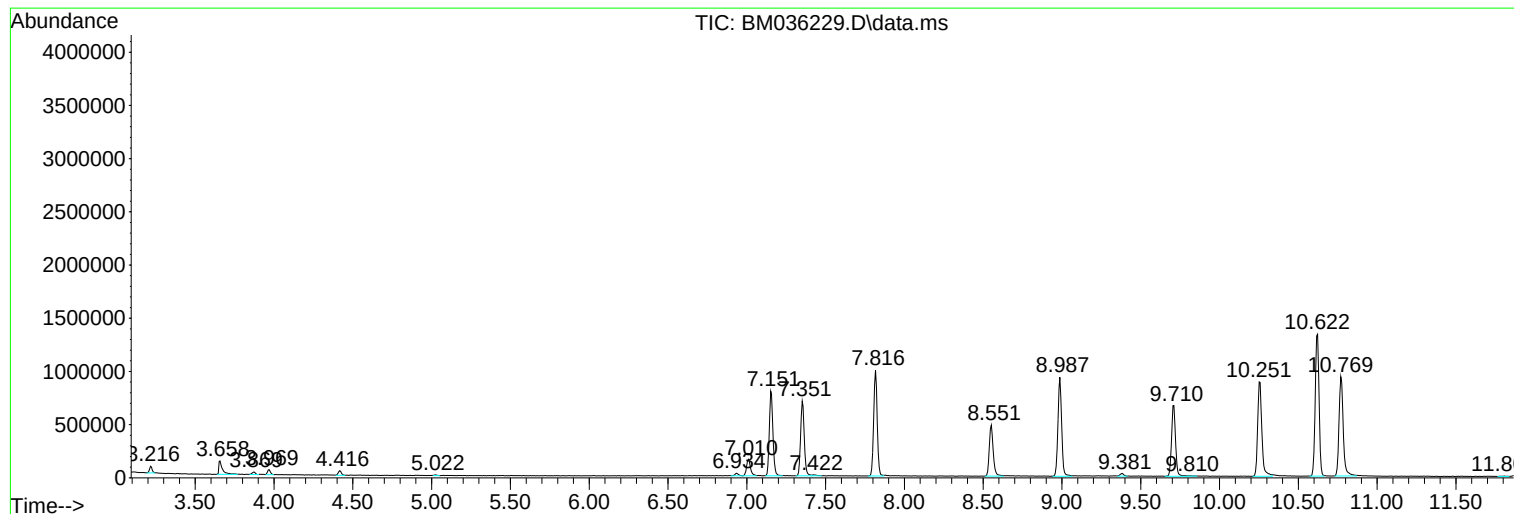

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036229.D
Acq On : 12 Aug 2022 14:25
Operator : CG/JU
Sample : N4129-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBW8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036229.D
Acq On : 12 Aug 2022 14:25
Operator : CG/JU
Sample : N4129-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBW8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc