

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036230.D
 Acq On : 12 Aug 2022 15:02
 Operator : CG/JU
 Sample : N4129-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036230.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	19	22	30	rVB	57788	73169	1.22%	0.139%
2	3.658	94	97	108	rBV	99040	155249	2.59%	0.295%
3	3.875	129	134	138	rVB	25431	37687	0.63%	0.072%
4	3.969	145	150	157	rVB	51174	68363	1.14%	0.130%
5	4.416	222	226	233	rVB	45524	60776	1.01%	0.115%
6	4.904	305	309	310	rBV4	5110	6474	0.11%	0.012%
7	5.028	325	330	336	rVB7	6815	10626	0.18%	0.020%
8	6.934	649	654	660	rVB	25183	38103	0.64%	0.072%
9	7.010	660	667	678	rBV	167491	292202	4.87%	0.555%
10	7.151	685	691	701	rBV	736694	1190066	19.85%	2.261%
11	7.351	718	725	736	rBV	700215	1140046	19.01%	2.166%
12	7.428	736	738	742	rVB5	7270	8532	0.14%	0.016%
13	7.816	796	804	813	rBV	820783	1282084	21.38%	2.435%
14	8.551	922	929	939	rBV	500405	854905	14.26%	1.624%
15	8.987	996	1003	1019	rBV	848548	1426485	23.79%	2.710%
16	9.381	1064	1070	1076	rVB	26874	41129	0.69%	0.078%
17	9.704	1118	1125	1139	rBV	630631	1081089	18.03%	2.054%
18	10.251	1210	1218	1241	rBV	849659	1593335	26.57%	3.027%
19	10.616	1272	1280	1289	rBV	1101649	1823203	30.40%	3.463%
20	10.769	1299	1306	1321	rBV	775040	1422469	23.72%	2.702%
21	11.875	1489	1494	1500	rVB	16619	28159	0.47%	0.053%
22	12.216	1546	1552	1561	rVB	14789	33461	0.56%	0.064%
23	12.822	1648	1655	1660	rBV7	7478	12903	0.22%	0.025%
24	13.075	1693	1698	1702	rBV7	4253	7166	0.12%	0.014%
25	13.363	1741	1747	1753	rBV4	14495	25495	0.43%	0.048%
26	13.439	1754	1760	1763	rVB5	4790	7517	0.13%	0.014%
27	13.880	1827	1835	1847	rBV	1986571	2750617	45.87%	5.225%
28	14.151	1874	1881	1893	rBV	2239021	3325304	55.45%	6.316%
29	14.463	1926	1934	1947	rBV	1612066	2343909	39.09%	4.452%
30	14.710	1968	1976	1990	rBV2	73492	210792	3.52%	0.400%
31	14.904	2005	2009	2015	rVB8	7077	13461	0.22%	0.026%
32	15.257	2061	2069	2071	rBV4	5066	10058	0.17%	0.019%
33	15.286	2071	2074	2080	rVB3	10360	16719	0.28%	0.032%
34	15.451	2094	2102	2118	rBV	3082738	4304382	71.78%	8.176%
35	15.580	2118	2124	2138	rBV	826657	1212002	20.21%	2.302%
36	15.692	2138	2143	2149	rVB2	31530	57443	0.96%	0.109%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036230.D
 Acq On : 12 Aug 2022 15:02
 Operator : CG/JU
 Sample : N4129-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBX0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	16.116	2211	2215	2217	rBV5	4980	8064	0.13%	0.015%
38	16.168	2220	2224	2226	rBV2	6457	8392	0.14%	0.016%
39	16.233	2232	2235	2240	rVB5	10760	11559	0.19%	0.022%
40	16.668	2305	2309	2314	rBV4	14063	22075	0.37%	0.042%
41	16.963	2355	2359	2361	rBV3	11481	15167	0.25%	0.029%
42	17.127	2384	2387	2391	rBV6	4112	7194	0.12%	0.014%
43	17.204	2394	2400	2409	rBV	1892923	2689453	44.85%	5.109%
44	17.304	2410	2417	2429	rVV	3403645	4796298	79.98%	9.111%
45	17.492	2447	2449	2454	rVB5	5110	6045	0.10%	0.011%
46	17.739	2487	2491	2495	rVV2	11429	17544	0.29%	0.033%
47	17.874	2511	2514	2519	rVB5	11537	15572	0.26%	0.030%
48	18.104	2548	2553	2559	rBV4	32397	57621	0.96%	0.109%
49	18.174	2562	2565	2570	rVB	12540	19527	0.33%	0.037%
50	18.568	2628	2632	2633	rBV4	5785	7129	0.12%	0.014%
51	19.162	2728	2733	2736	rBV	45951	68783	1.15%	0.131%
52	19.233	2741	2745	2752	rVV	39783	62541	1.04%	0.119%
53	19.598	2801	2807	2814	rBV	4220420	5621126	93.74%	10.677%
54	20.598	2974	2977	2980	rVB	123751	125024	2.08%	0.237%
55	21.386	3106	3111	3121	rBV	2484491	3091083	51.55%	5.872%
56	23.574	3477	3483	3496	rVB2	3066777	5996678	100.00%	11.391%
57	23.727	3503	3509	3517	rVB2	1605398	3032577	50.57%	5.760%




Sum of corrected areas: 52644832

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036230.D
Acq On : 12 Aug 2022 15:02
Operator : CG/JU
Sample : N4129-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

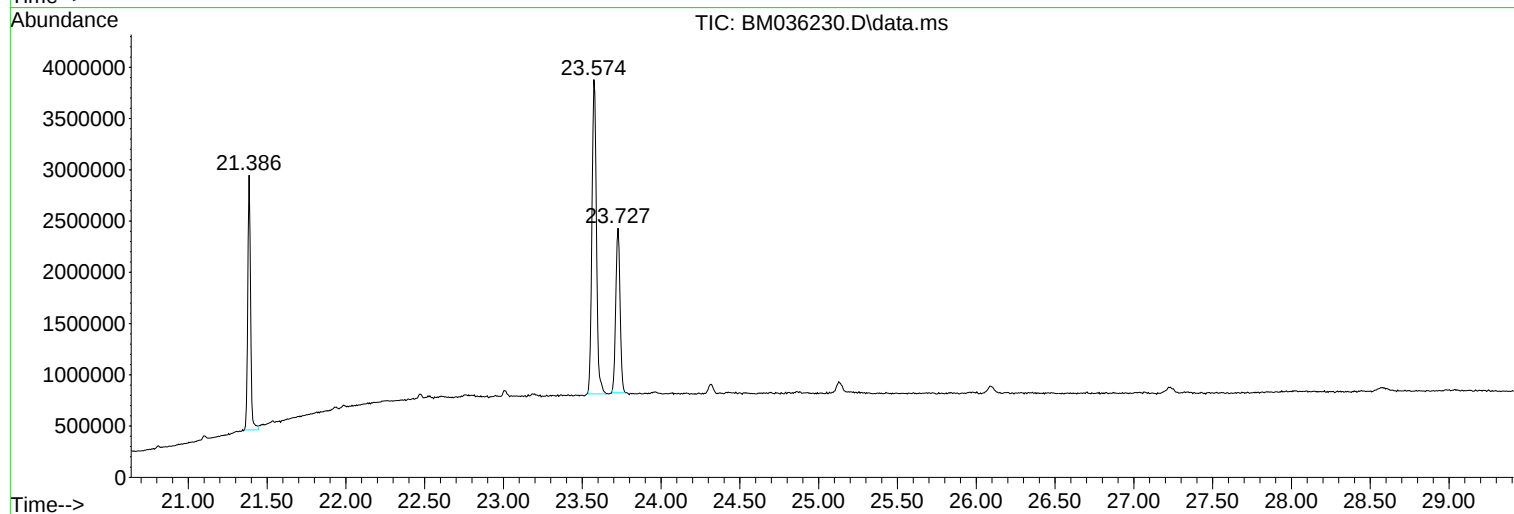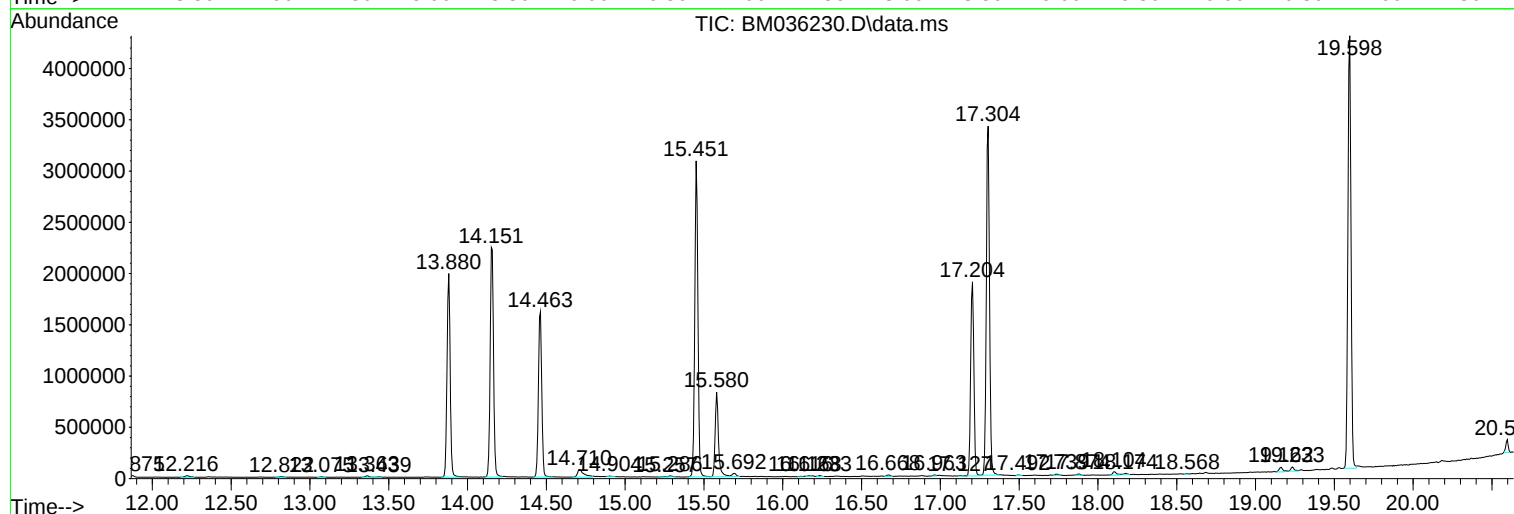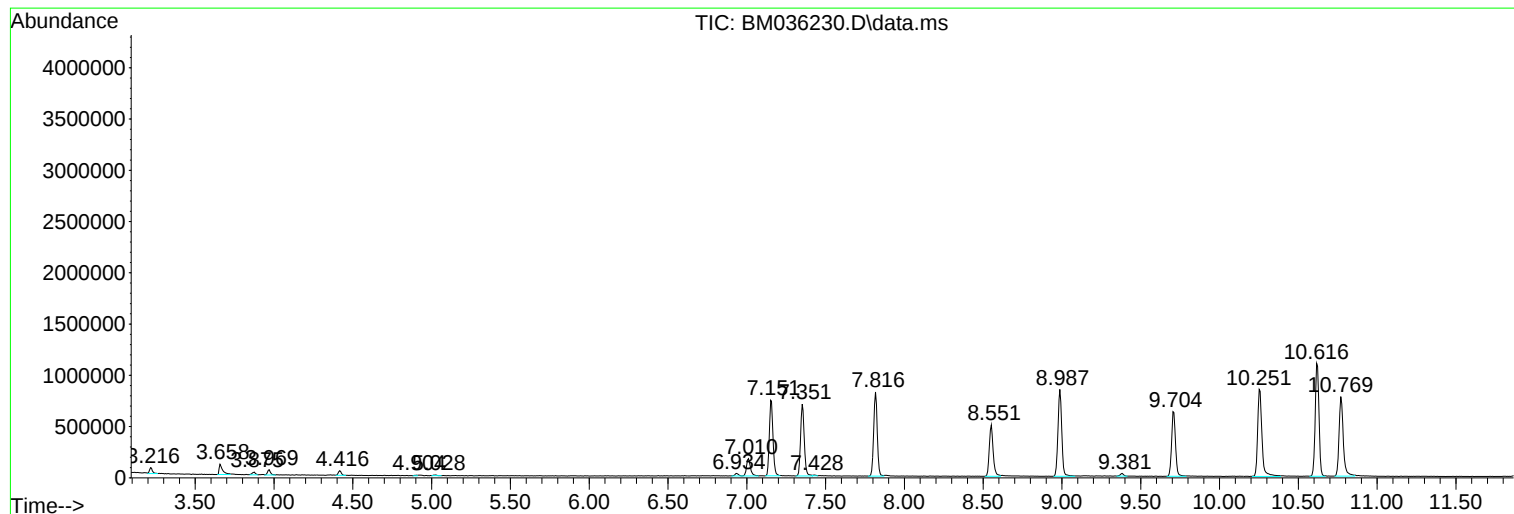

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036230.D
Acq On : 12 Aug 2022 15:02
Operator : CG/JU
Sample : N4129-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036230.D
Acq On : 12 Aug 2022 15:02
Operator : CG/JU
Sample : N4129-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc